

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
 Data File : PD058882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 08:50
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 09:41:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 09:11:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	37189084	56128534	37.981	37.798
27)	SA Decachlor...	7.841	8.858	77748661	98363340	73.036	71.886
Target Compounds							
2)	A alpha-BHC	3.629	4.247	56418117	83109040	39.705	39.678
3)	MA gamma-BHC...	3.900	4.528	53336510	75314715	38.826	38.594
4)	MA Heptachlor	4.179	5.028	46773411	72679796	39.355	38.468
9)	A Endosulfan I	5.172	6.064	42544242	59193045	38.812	37.604
13)	MA Dieldrin	5.409	6.319	96721007	132.2E6	79.290	78.315
14)	MA Endrin	5.660	6.535	77715540	108.8E6	80.253	80.023
16)	A 4,4'-DDD	5.798	6.663	74006595	104.5E6	78.479	78.528
17)	MA 4,4'-DDT	6.031	6.960	71821678	107.3E6	79.372	81.536
20)	A Methoxychlor	6.580	7.420	176.2E6	271.2E6	389.799	391.042


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
Data File : PD058882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 08:50
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 09:41:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 09:11:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

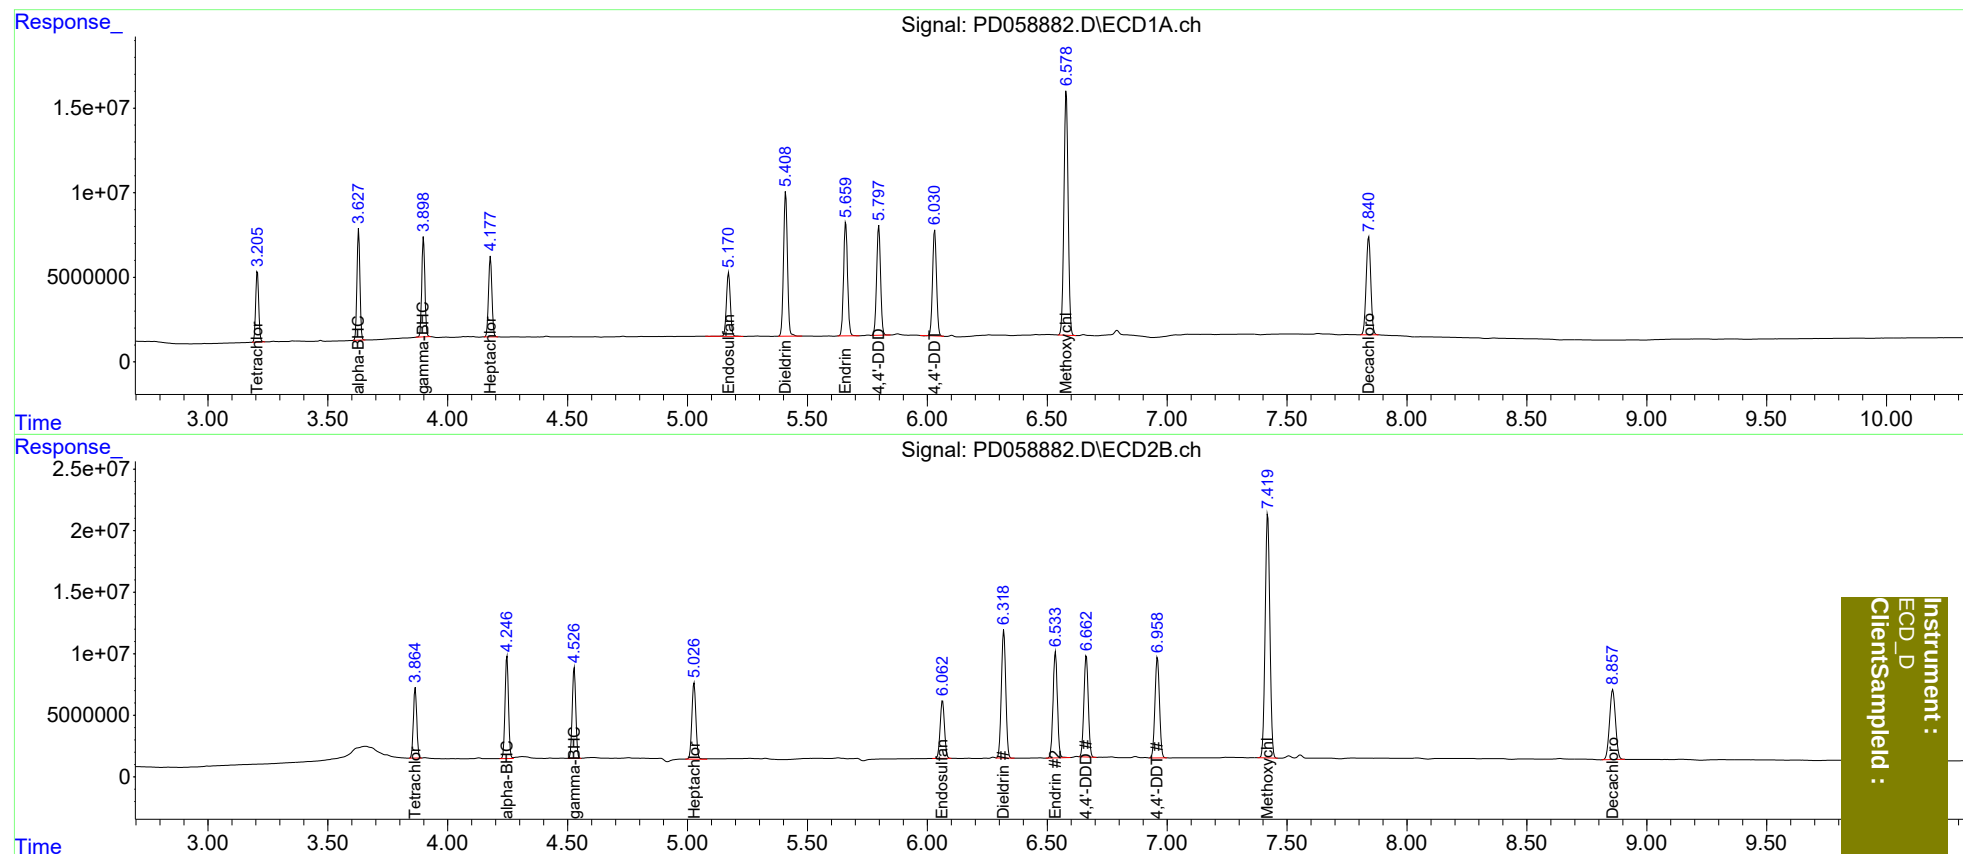


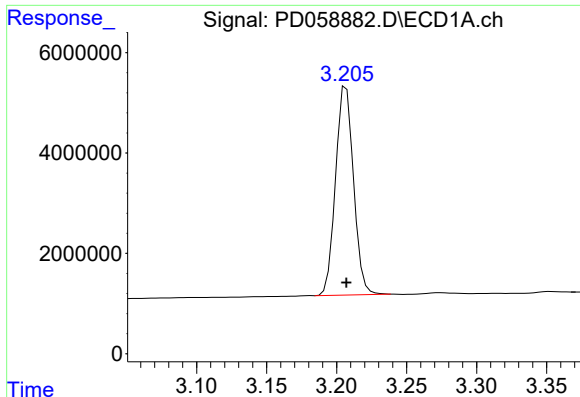

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 37189084
Conc: 37.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

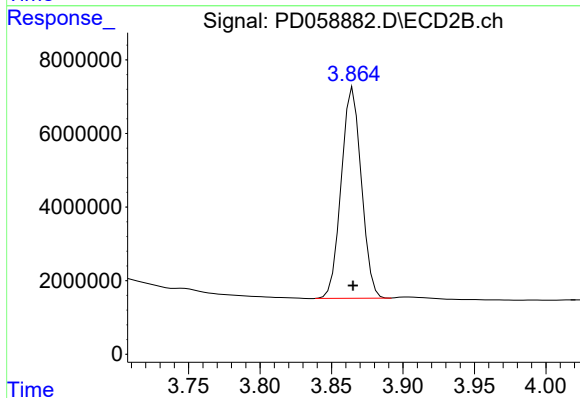


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 56128534
Conc: 37.80 ng/ml

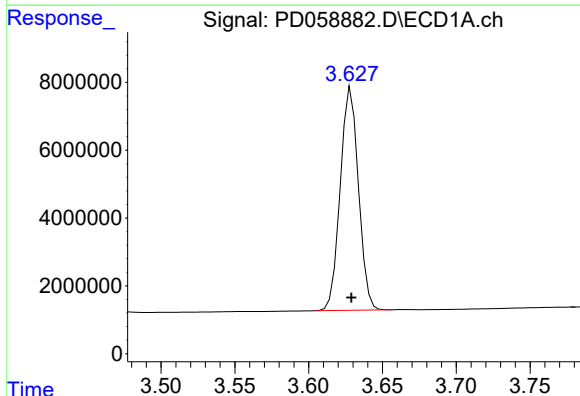


#2 alpha-BHC

R.T.: 3.629 min
Delta R.T.: 0.000 min
Response: 56418117
Conc: 39.71 ng/ml

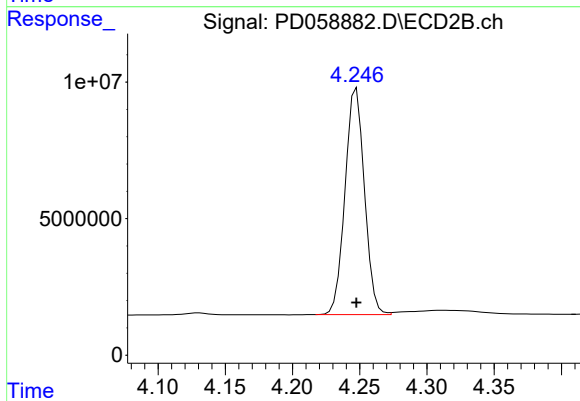

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 83109040
Conc: 39.68 ng/ml

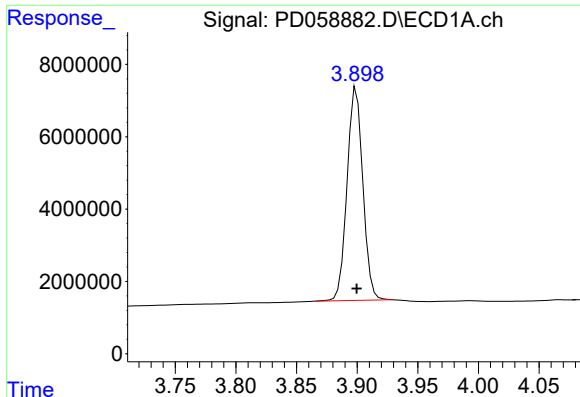

#3 gamma-BHC (Lindane)


R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 53336510
Conc: 38.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

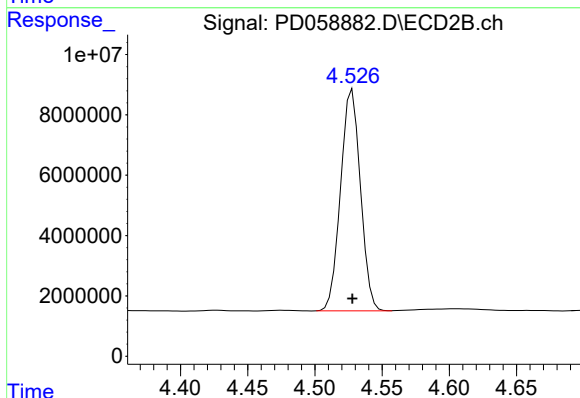


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 75314715
Conc: 38.59 ng/ml

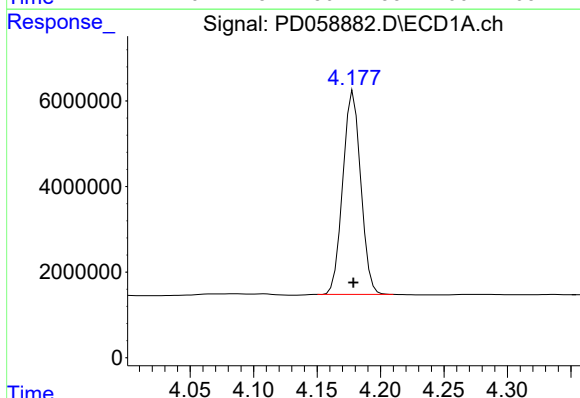


#4 Heptachlor

R.T.: 4.179 min
Delta R.T.: 0.000 min
Response: 46773411
Conc: 39.35 ng/ml

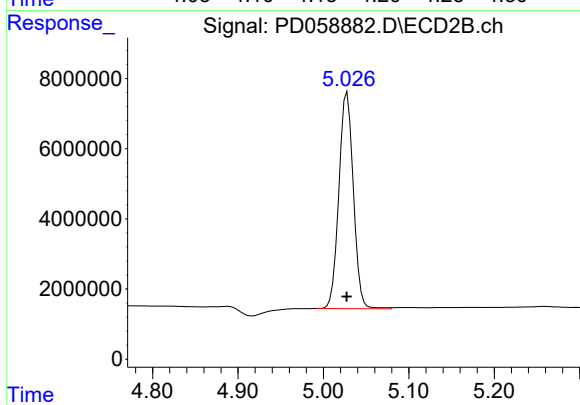

#4 Heptachlor


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 72679796
Conc: 38.47 ng/ml

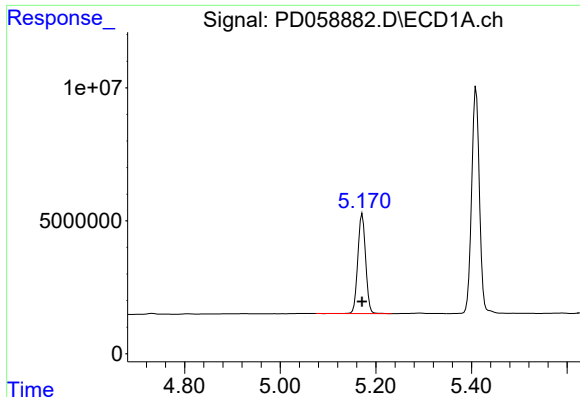

#9 Endosulfan I


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 42544242
Conc: 38.81 ng/ml

Instrument :
ECD_D
ClientSampleId :

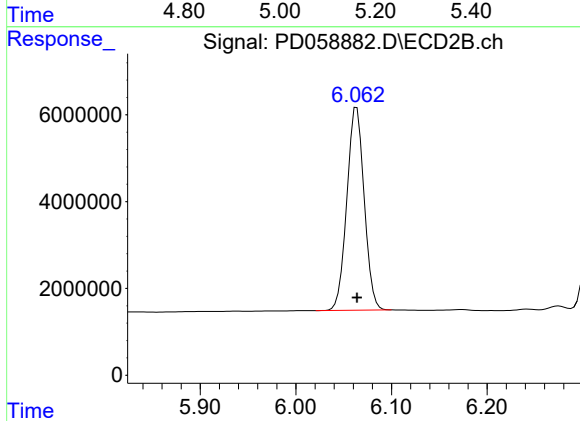


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 59193045
Conc: 37.60 ng/ml

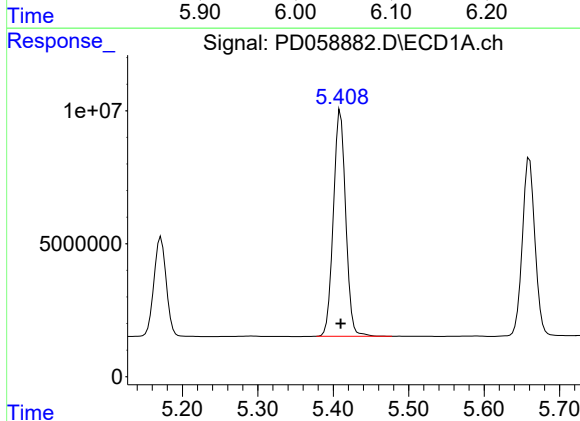


#13 Dieldrin

R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 96721007
Conc: 79.29 ng/ml

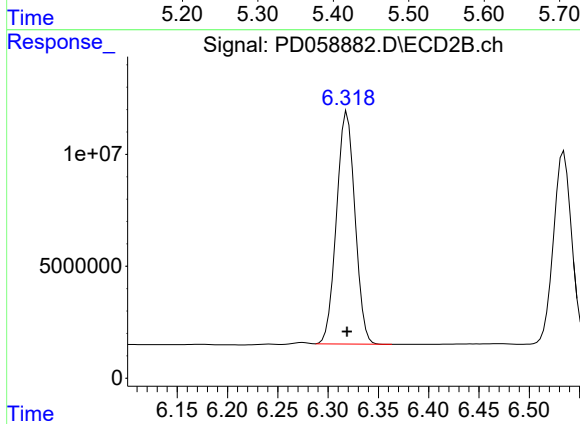

#13 Dieldrin


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 132220367
Conc: 78.31 ng/ml

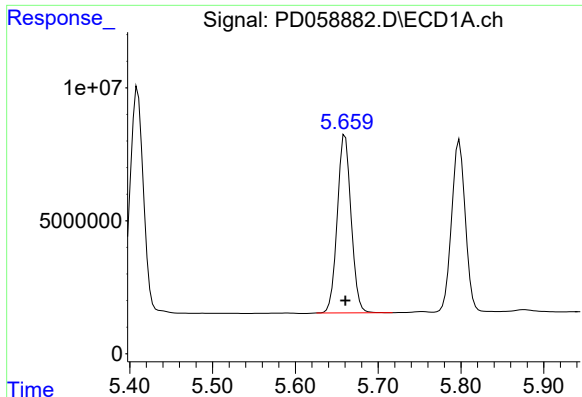

#14 Endrin


R.T.: 5.660 min
Delta R.T.: 0.000 min
Response: 77715540
Conc: 80.25 ng/ml

Instrument :
ECD_D
ClientSampleId :

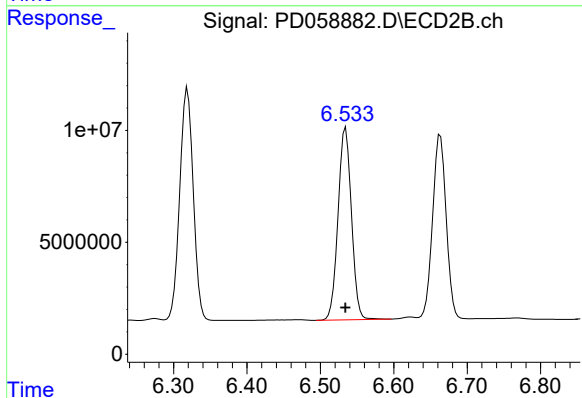


#14 Endrin

R.T.: 6.535 min
Delta R.T.: 0.000 min
Response: 108804443
Conc: 80.02 ng/ml

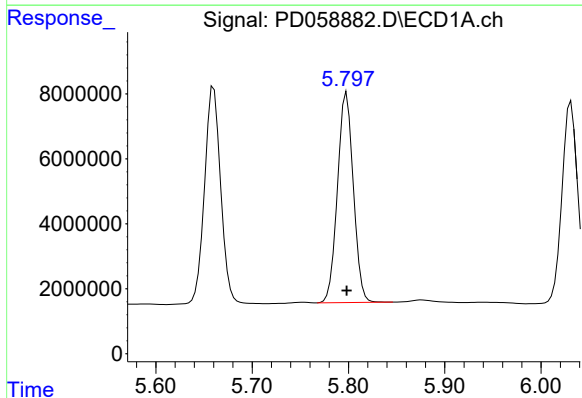


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 74006595
Conc: 78.48 ng/ml

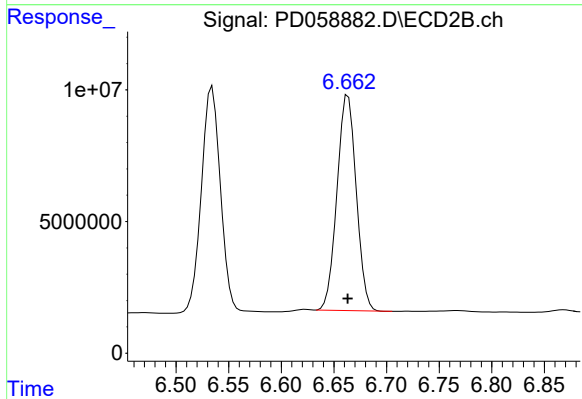

#16 4,4'-DDD


R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 104546810
Conc: 78.53 ng/ml

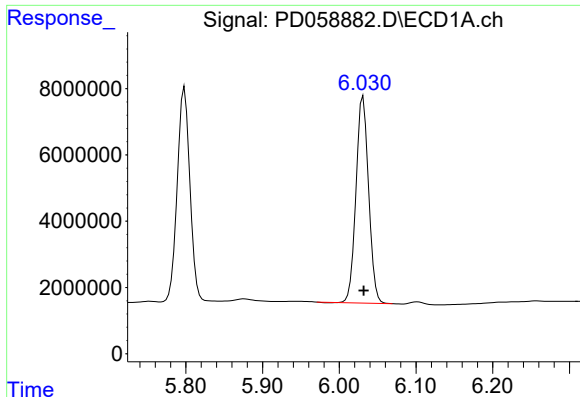

#17 4,4'-DDT


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 71821678
Conc: 79.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

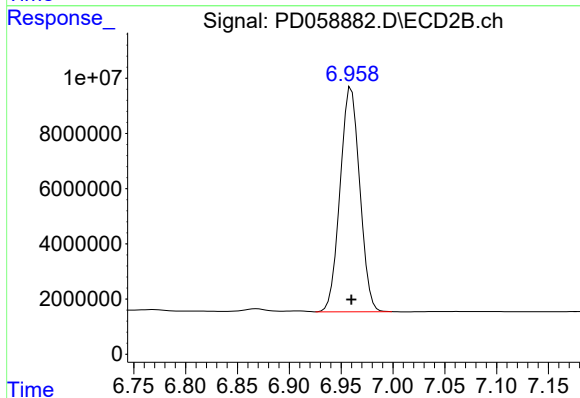


#17 4,4'-DDT

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 107333789
Conc: 81.54 ng/ml

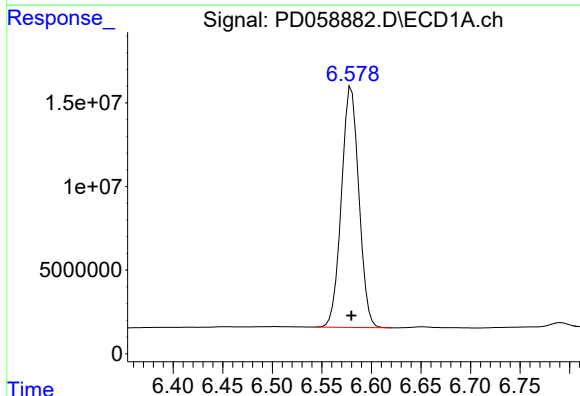


#20 Methoxychlor

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 176247431
Conc: 389.80 ng/ml

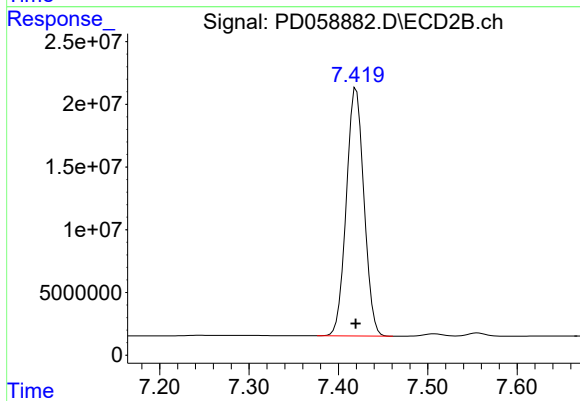

#20 Methoxychlor


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 271161800
Conc: 391.04 ng/ml

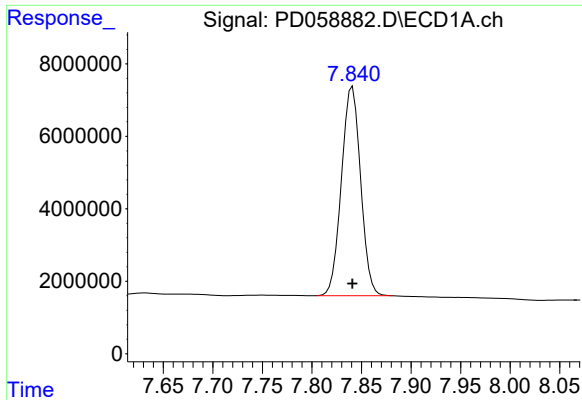

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 77748661
Conc: 73.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

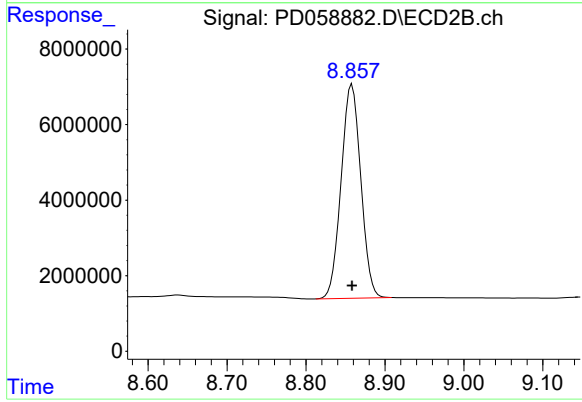

#27 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 98363340
Conc: 71.89 ng/ml