

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
 Data File : PD058884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2020 09:19
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 06 09:41:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 09:11:39 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.865	75731994	113.5E6	77.344	76.449
27)	SA Decachlor...	7.841	8.858	155.1E6	190.8E6	145.662	139.465
Target Compounds							
2)	A alpha-BHC	3.628	4.247	119.7E6	173.1E6	84.247	82.661
3)	MA gamma-BHC...	3.899	4.528	110.9E6	157.1E6	80.709	80.482
4)	MA Heptachlor	4.178	5.028	97316502	149.7E6	81.881	79.210
9)	A Endosulfan I	5.172	6.064	86805422	120.4E6	79.190	76.485
13)	MA Dieldrin	5.410	6.319	201.1E6	270.8E6	164.855	160.390
14)	MA Endrin	5.661	6.535	156.9E6	218.6E6	162.025	160.809
16)	A 4,4'-DDD	5.798	6.663	154.7E6	215.4E6	164.002	161.790
17)	MA 4,4'-DDT	6.032	6.960	158.6E6	222.2E6	175.278	168.774
20)	A Methoxychlor	6.580	7.420	345.8E6	491.6E6	764.767	708.957


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080620\
Data File : PD058884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2020 09:19
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 06 09:41:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 09:11:39 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

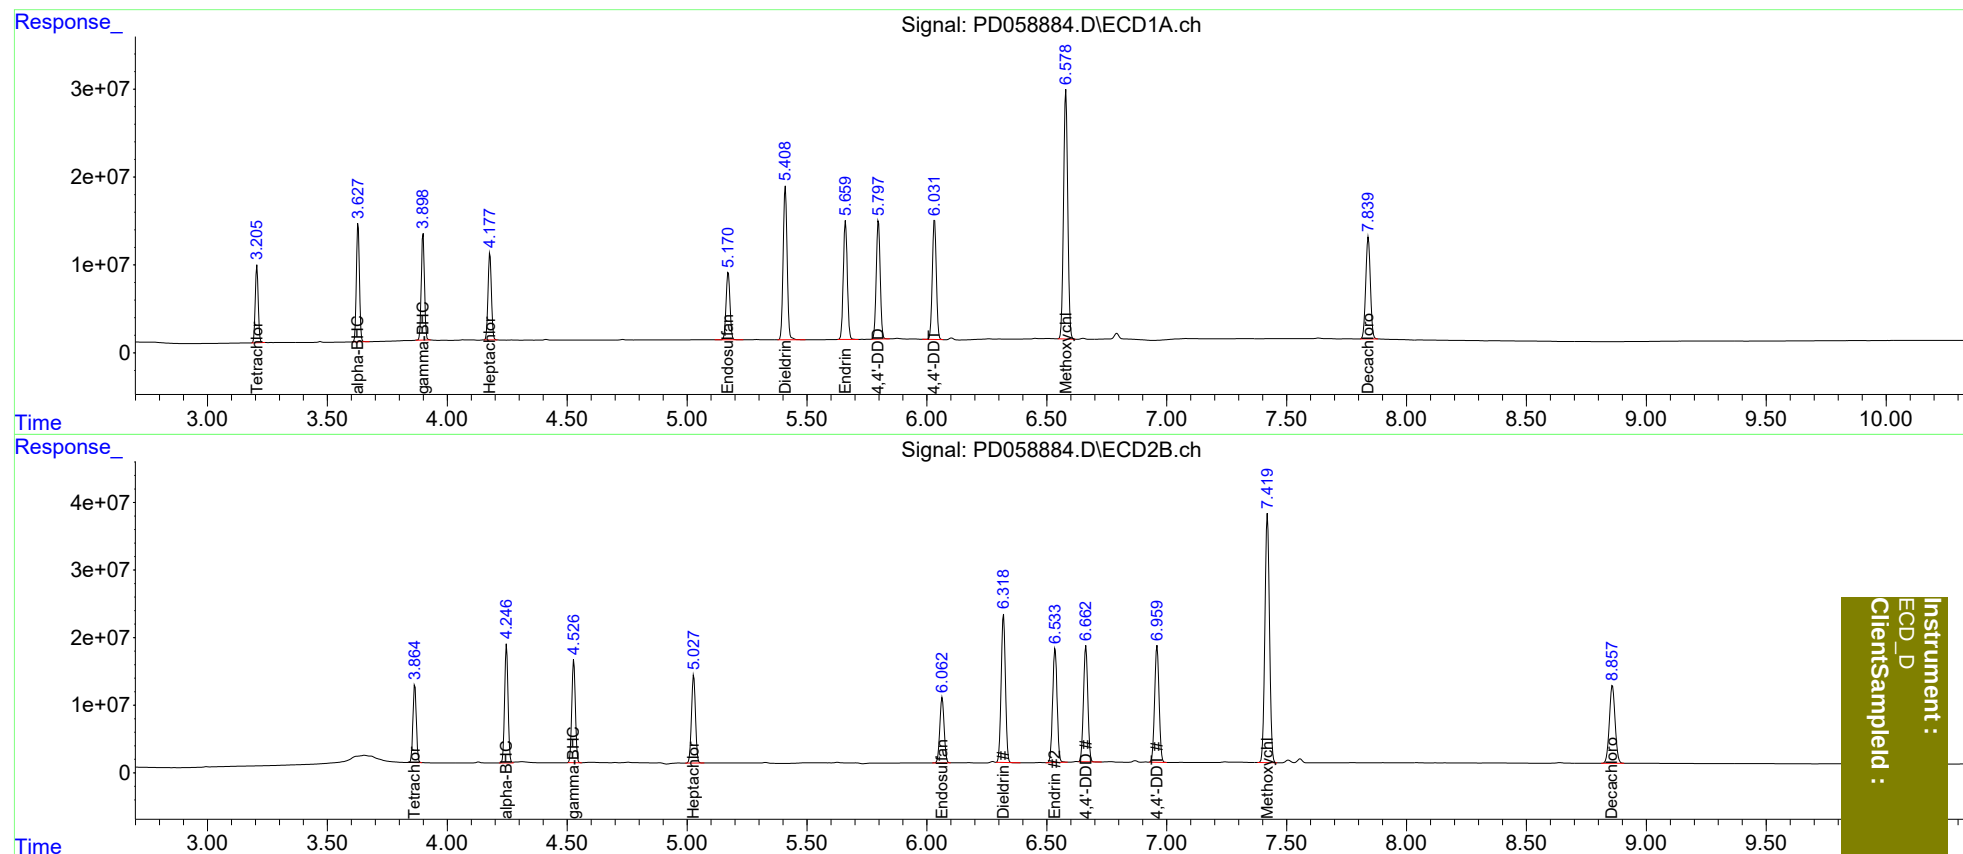


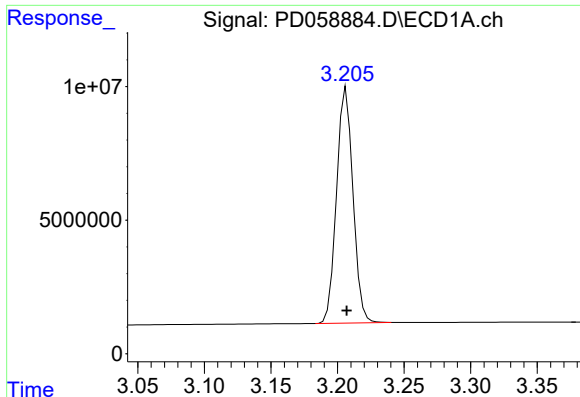

#1 Tetrachloro-m-xylene


R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 75731994
Conc: 77.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

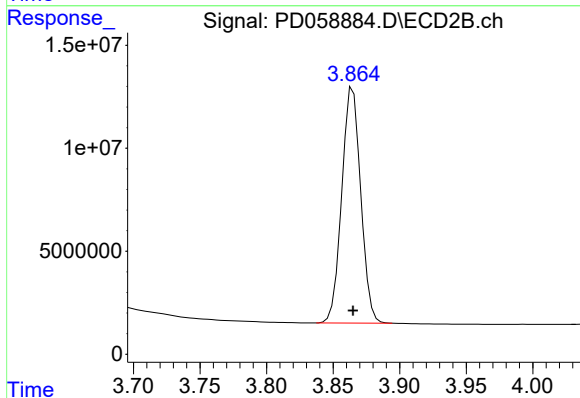


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 113524752
Conc: 76.45 ng/ml

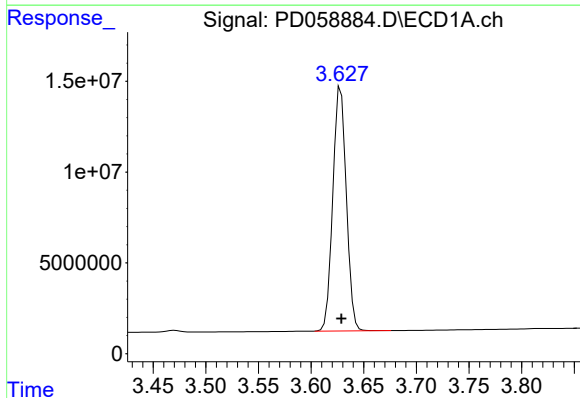


#2 alpha-BHC

R.T.: 3.628 min
Delta R.T.: 0.000 min
Response: 119707599
Conc: 84.25 ng/ml

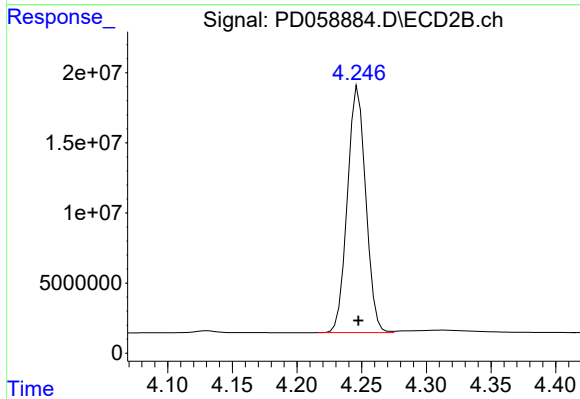

#2 alpha-BHC


R.T.: 4.247 min
Delta R.T.: 0.000 min
Response: 173140743
Conc: 82.66 ng/ml

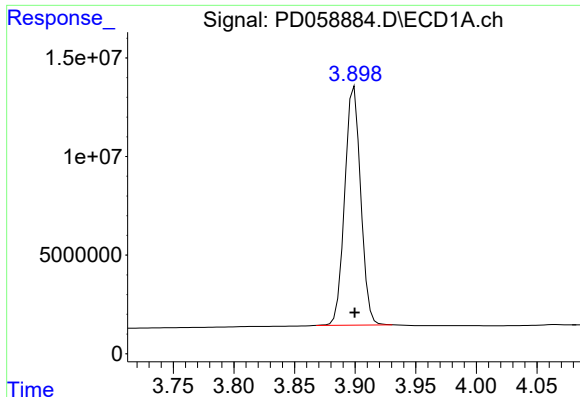

#3 gamma-BHC (Lindane)


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 110873634
Conc: 80.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

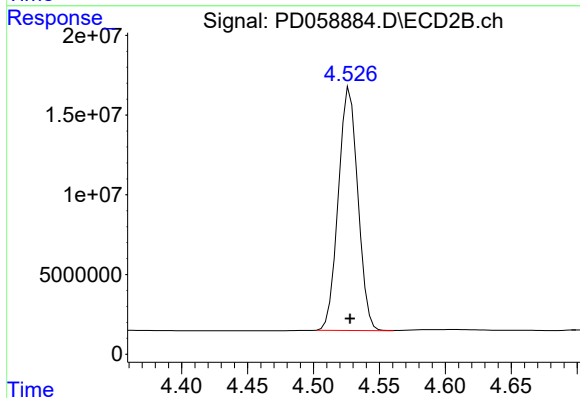


#3 gamma-BHC (Lindane)

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 157059066
Conc: 80.48 ng/ml

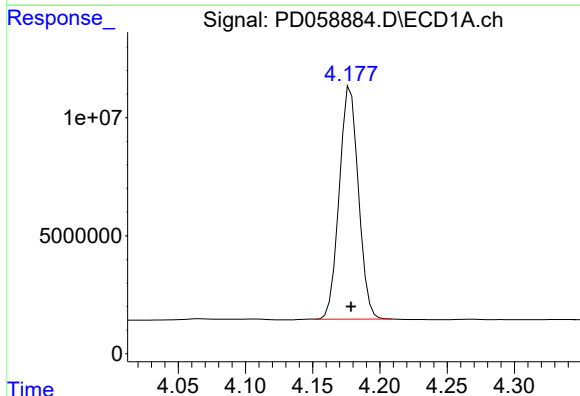


#4 Heptachlor

R.T.: 4.178 min
Delta R.T.: 0.000 min
Response: 97316502
Conc: 81.88 ng/ml

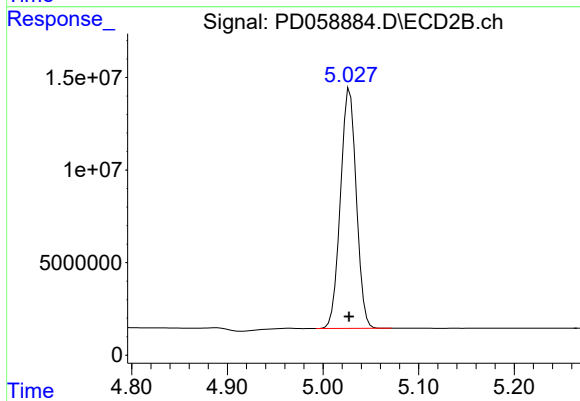

#4 Heptachlor


R.T.: 5.028 min
Delta R.T.: 0.000 min
Response: 149655928
Conc: 79.21 ng/ml

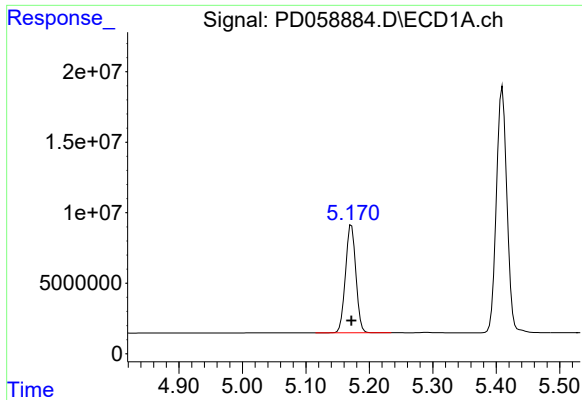

#9 Endosulfan I


R.T.: 5.172 min
Delta R.T.: 0.000 min
Response: 86805422
Conc: 79.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

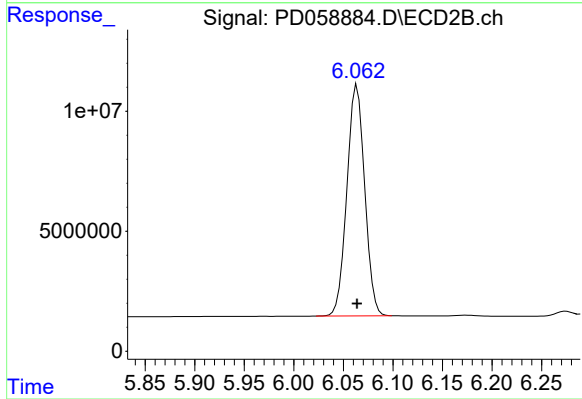


#9 Endosulfan I

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 120398063
Conc: 76.49 ng/ml

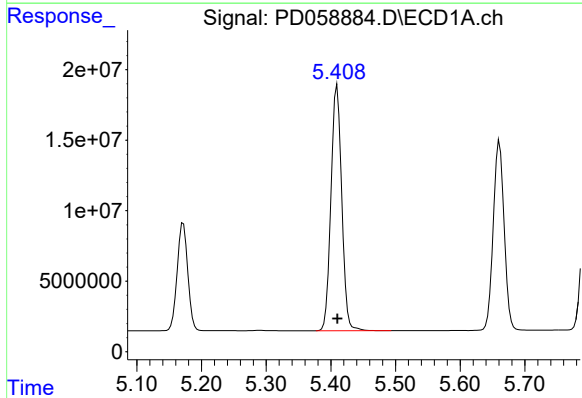


#13 Dieldrin

R.T.: 5.410 min
Delta R.T.: 0.000 min
Response: 201096832
Conc: 164.85 ng/ml

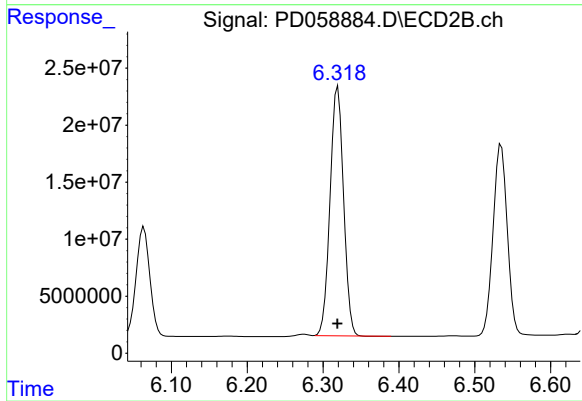

#13 Dieldrin


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 270789271
Conc: 160.39 ng/ml

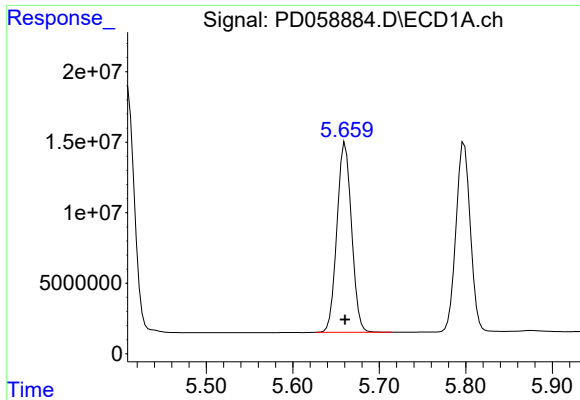

#14 Endrin


R.T.: 5.661 min
Delta R.T.: 0.000 min
Response: 156902339
Conc: 162.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

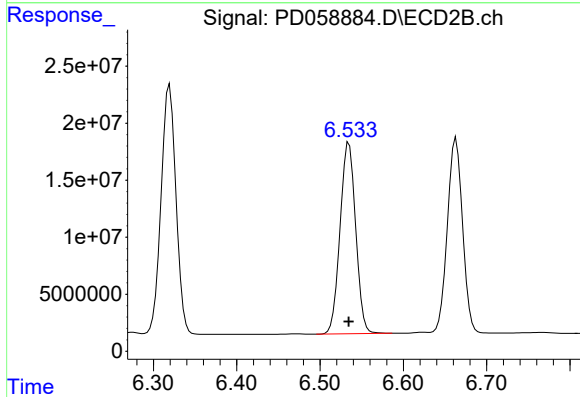


#14 Endrin

R.T.: 6.535 min
Delta R.T.: 0.000 min
Response: 218645803
Conc: 160.81 ng/ml

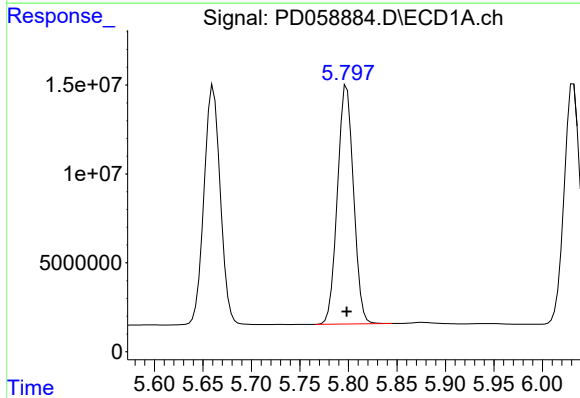


#16 4,4'-DDD

R.T.: 5.798 min
Delta R.T.: 0.000 min
Response: 154655303
Conc: 164.00 ng/ml

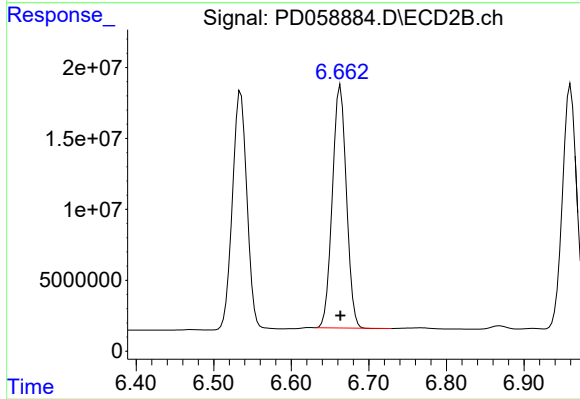

#16 4,4'-DDD


R.T.: 6.663 min
Delta R.T.: 0.000 min
Response: 215396971
Conc: 161.79 ng/ml

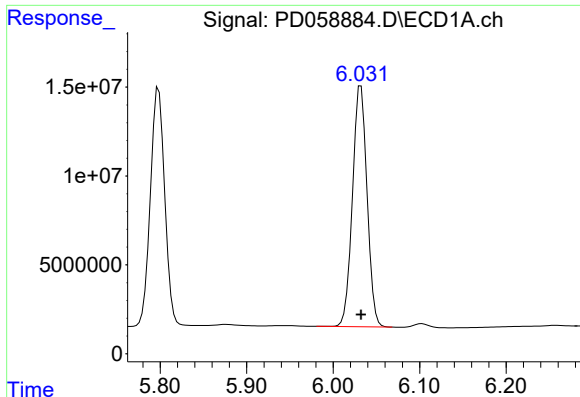

#17 4,4'-DDT


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 158604925
Conc: 175.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

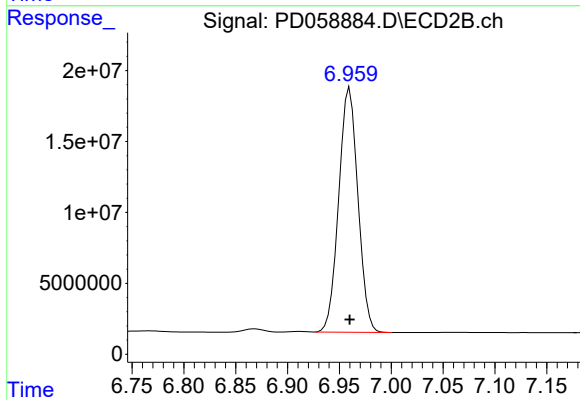


#17 4,4'-DDT

R.T.: 6.960 min
Delta R.T.: 0.000 min
Response: 222172436
Conc: 168.77 ng/ml

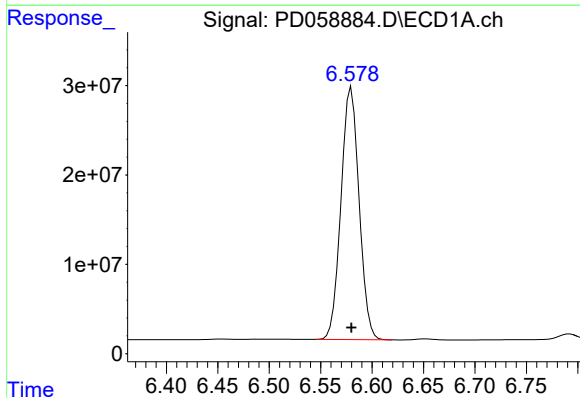


#20 Methoxychlor

R.T.: 6.580 min
Delta R.T.: 0.000 min
Response: 345788715
Conc: 764.77 ng/ml

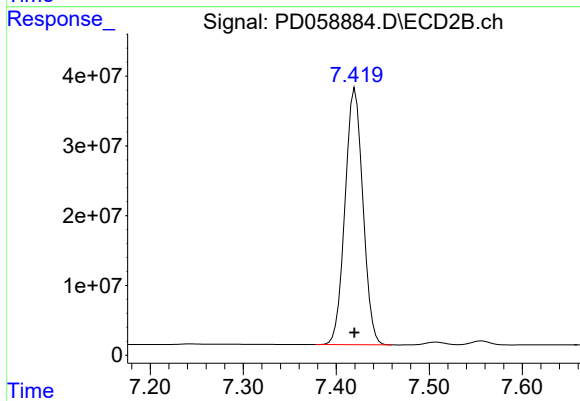

#20 Methoxychlor


R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 491615067
Conc: 708.96 ng/ml

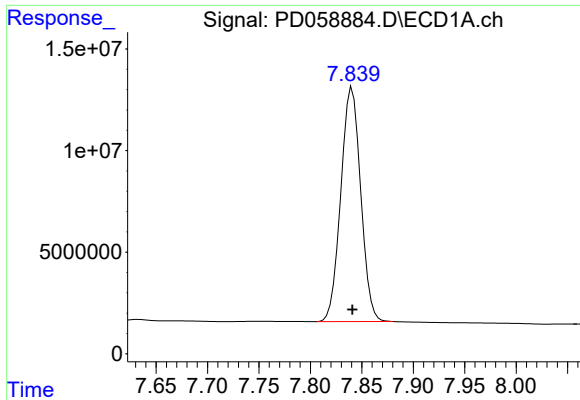

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 155061146
Conc: 145.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

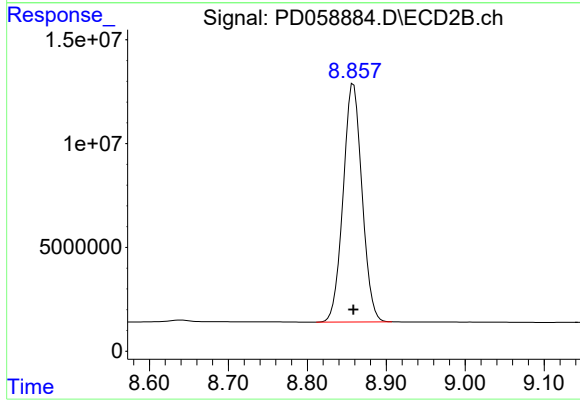

#27 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 190832780
Conc: 139.46 ng/ml