

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
 Data File : PD064797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 15:06
 Operator : AR\AJ
 Sample : M3182-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00D6

Manual Integrations
 APPROVED

mohammad
 8/9/2021 4:53:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 04:46:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.617	18713491	180.5E6	15.688	19.752m#
27)	SA Decachlor...	11.303	10.360	33634912	158.9E6	25.551	26.722
Target Compounds							
10)	B trans-Chl...	8.133	7.325	14730940	22791257	9.193	2.513m#
11)	B cis-Chlor...	8.227	7.390	1532013	13003565	0.983m	1.462m#
13)	MA Dieldrin	8.549	7.739	1358152	10530320	0.911	1.311 #
15)	B Endosulfa...	9.035	8.337	1121210	6726146	0.863m	1.165m#
16)	A 4,4'-DDD	8.949	8.176	4685680	17533611	3.817	3.044

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
Data File : PD064797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 15:06
Operator : AR\AJ
Sample : M3182-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 04:46:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

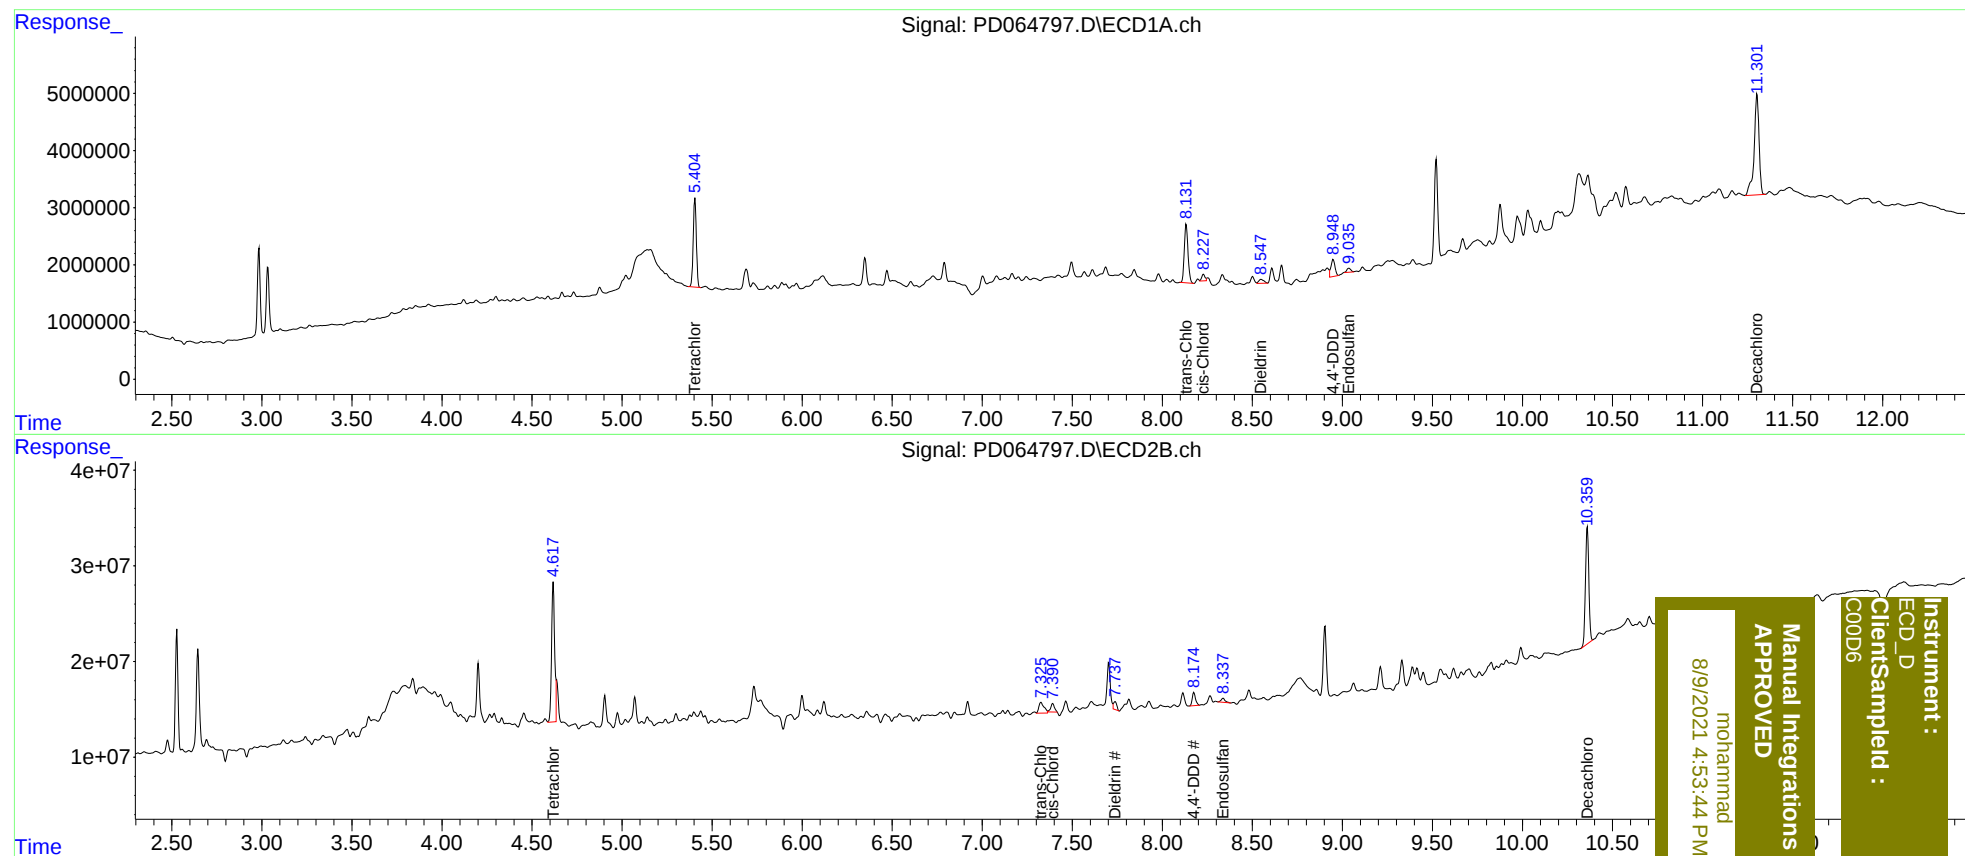

8/9/2021 4:53:44 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C00D6