

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
 Data File : PD064812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 19:13
 Operator : AR\AJ
 Sample : M3208-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00E4

Manual Integrations
 APPROVED

mohammad
 8/9/2021 4:54:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:10:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	14569385	149.9E6	12.214	16.404 #
27)	SA Decachlor...	11.306	10.359	31163647	172.3E6	23.674	28.975
Target Compounds							
15)	B Endosulfa...	9.034	8.335	2340163	38414051	1.802m	6.655m#
16)	A 4,4'-DDD	8.947	8.175	12877643	44491872	10.491m	7.725m#
17)	MA 4,4'-DDT	9.280	8.437	3815733	38413777	2.923	6.979m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
Data File : PD064812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 19:13
Operator : AR\AJ
Sample : M3208-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:10:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

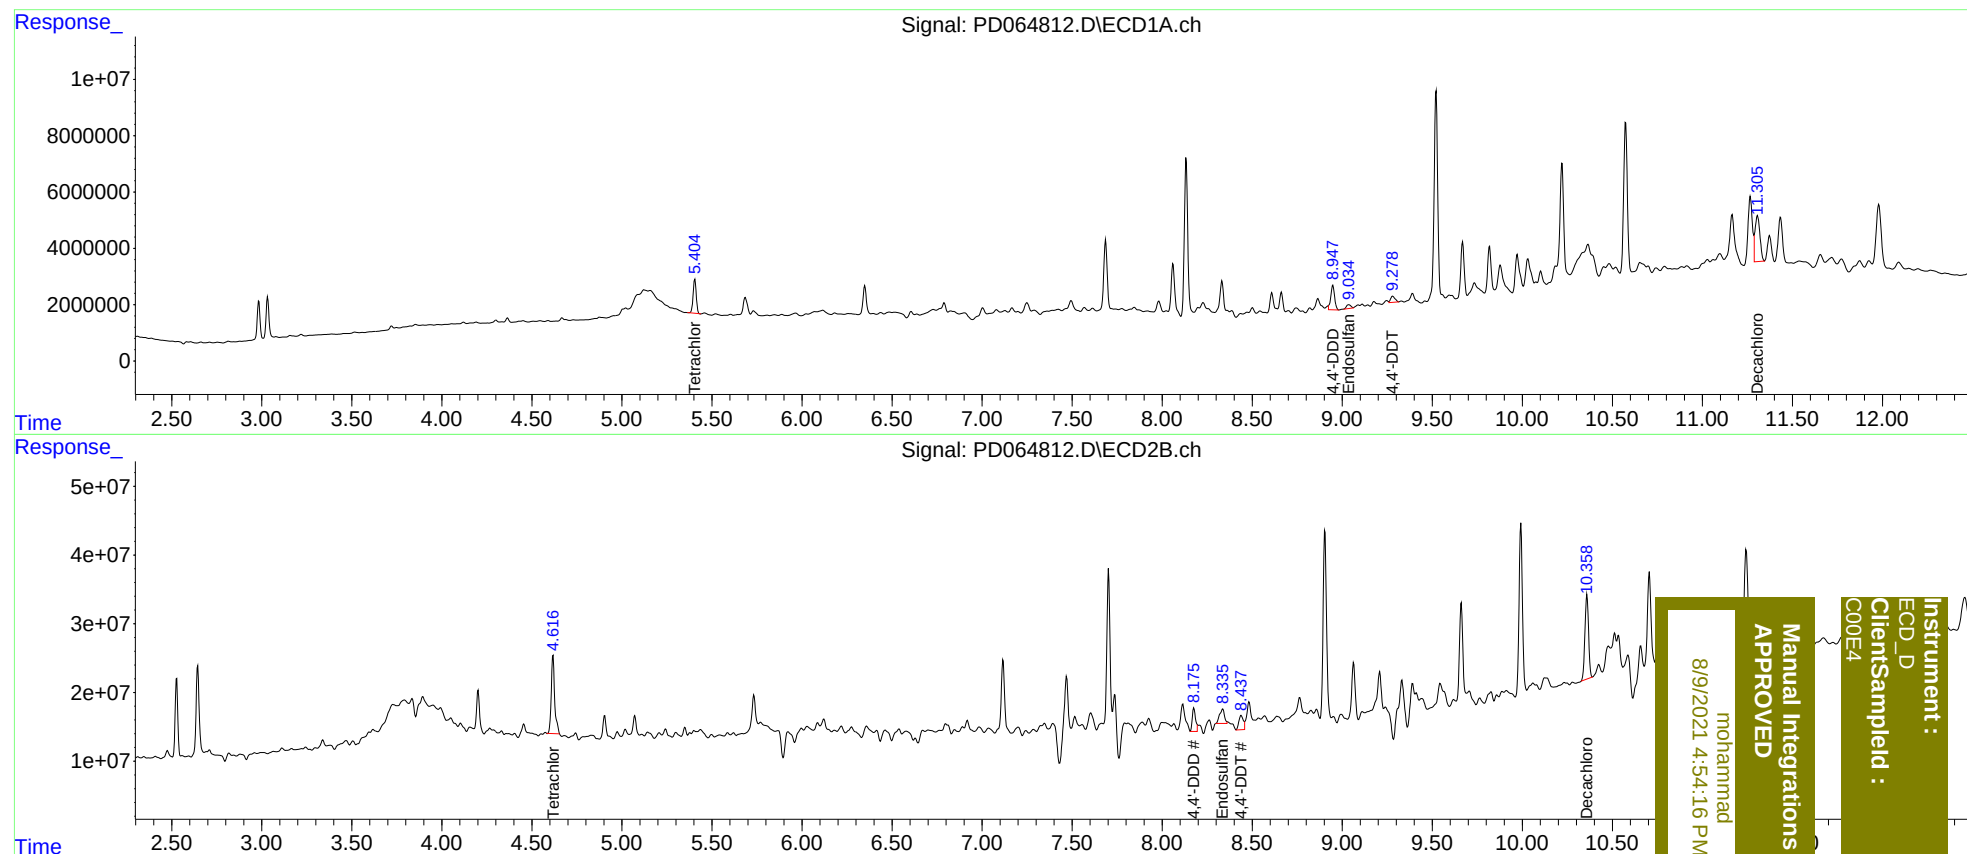

8/9/2021 4:54:16 PM

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C00E4