

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
 Data File : PD064813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 19:29
 Operator : AR\AJ
 Sample : M3208-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00E5

Manual Integrations
 APPROVED

mohammad
 8/9/2021 4:54:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 07:13:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	18898172	175.1E6	15.842	19.167
2)	SA Decachlor...	11.302	10.360	33386463	149.9E6	25.362	25.208
Target Compounds							
15)	B Endosulfa...	9.041	8.338	1137023	18659086	0.876	3.232 #
16)	A 4,4'-DDD	8.950	8.176	8789092	33357400	7.160	5.792
17)	MA 4,4'-DDT	9.278	8.442	5377715	26940193	4.119	4.894m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
Data File : PD064813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 19:29
Operator : AR\AJ
Sample : M3208-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 07:13:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

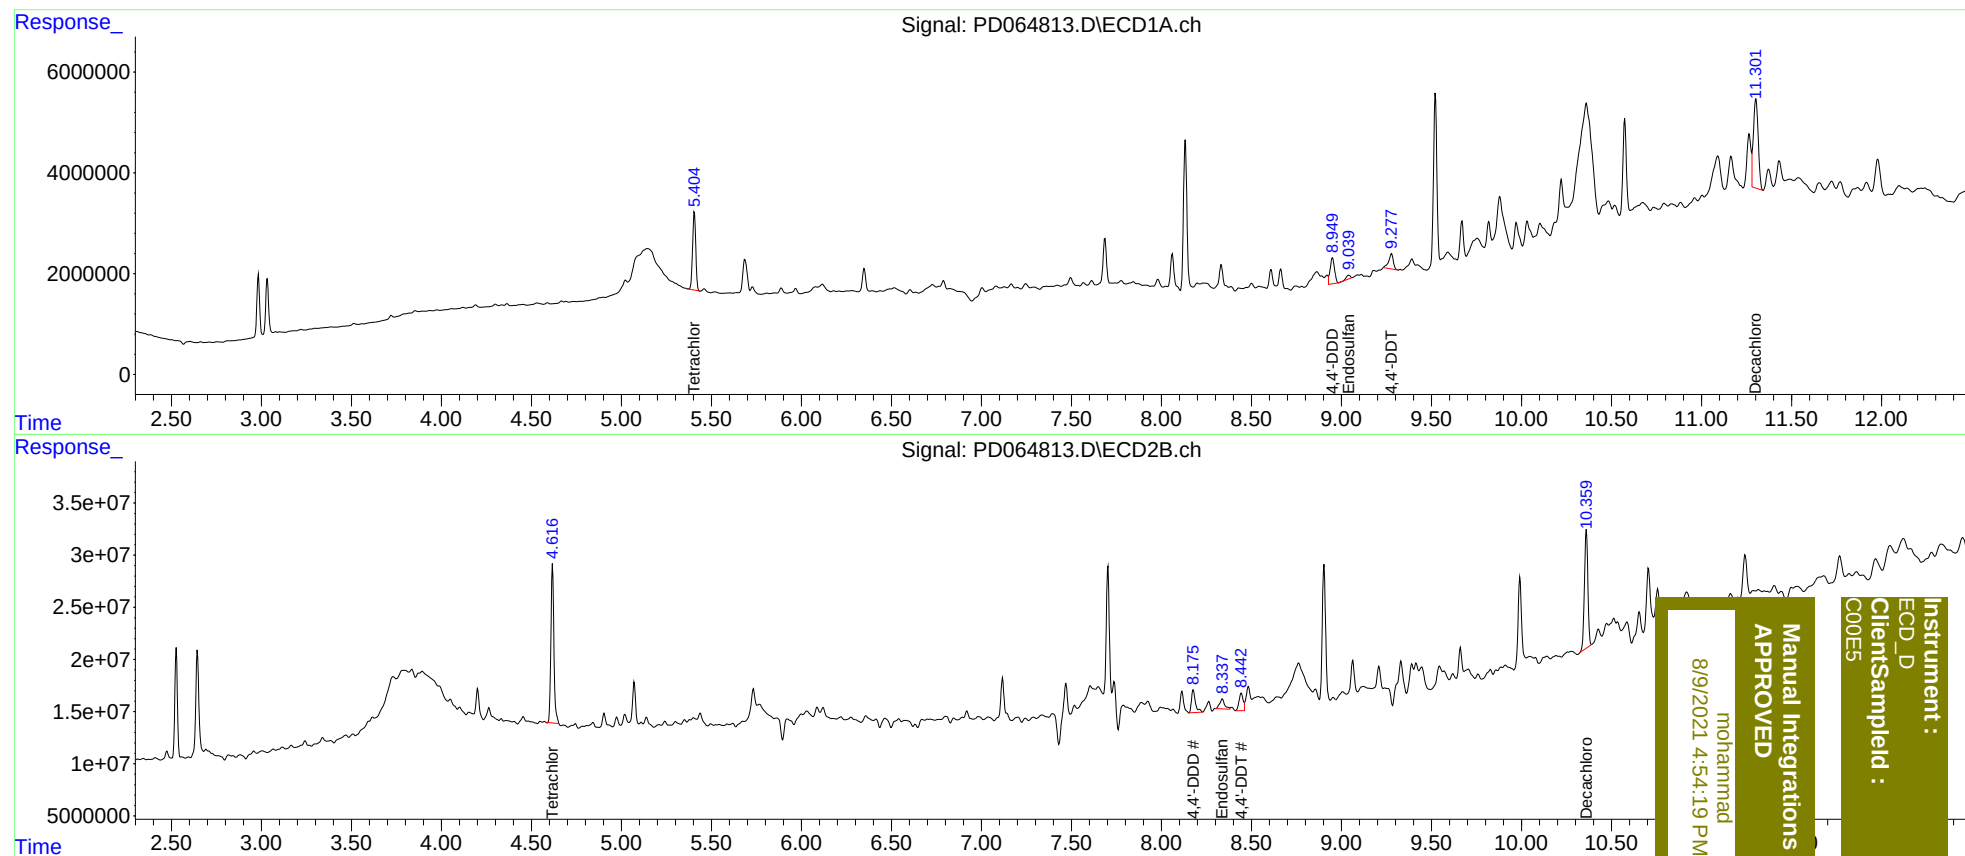

8/9/2021 4:54:19 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C00E5