

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
 Data File : PD064820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 21:21
 Operator : AR\AJ
 Sample : M3208-12MS
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C00F1MS

Manual Integrations
 APPROVED

mohammad
 8/9/2021 4:54:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:59:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	17255396	168.4E6	14.465	18.434 #
27)	SA Decachlor...	11.303	10.360	25005233	134.4E6	18.995	22.605
Target Compounds							
2)	A alpha-BHC	5.987	5.319	86048976	667.2E6	52.820	54.132
3)	MA gamma-BHC...	6.384	5.740	80643340	594.7E6	51.419	52.150
4)	MA Heptachlor	7.034	6.147	78980904	565.2E6	46.996	49.850m
5)	MB Aldrin	7.404	6.472	77525999	514.2E6	49.218	48.887
6)	B beta-BHC	6.644	6.114	35187607	239.3E6	45.103	39.446m
7)	B delta-BHC	6.909	6.377	81135789	538.3E6	46.626	49.552
8)	B Heptachlo...	7.873	7.045	73692263	420.8E6	42.923	45.456
9)	A Endosulfan I	8.278	7.447	61199223	339.3E6	43.414	44.131
10)	B trans-Chl...	8.144	7.321	96663701	423.4E6	60.322	46.675
11)	B cis-Chlor...	8.226	7.390	78806923	424.0E6	50.579	47.658
12)	B 4,4'-DDE	8.420	7.602	132.7E6	679.2E6	92.097	90.012
13)	MA Dieldrin	8.569	7.730	143.0E6	677.9E6	95.862	84.400m
14)	MA Endrin	8.807	8.022	123.6E6	557.0E6	96.515	96.954
15)	B Endosulfa...	9.043	8.332	118.9E6	500.6E6	91.582	86.723
16)	A 4,4'-DDD	8.960	8.185	121.1E6	494.1E6	98.678	85.784
17)	MA 4,4'-DDT	9.278	8.445	123.3E6	490.2E6	94.444	89.049
18)	B Endrin al...	9.178	8.518	104.8E6	384.5E6	92.521	77.909
19)	B Endosulfa...	9.417	8.748	122.2E6	451.8E6	88.632	83.821
20)	A Methoxychlor	9.770	9.037	324.6E6	1067.9E6	453.576	417.040
21)	B Endrin ke...	9.912	9.268	135.7E6	505.0E6	89.714	84.197

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
Data File : PD064820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 21:21
Operator : AR\AJ
Sample : M3208-12MS
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:59:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

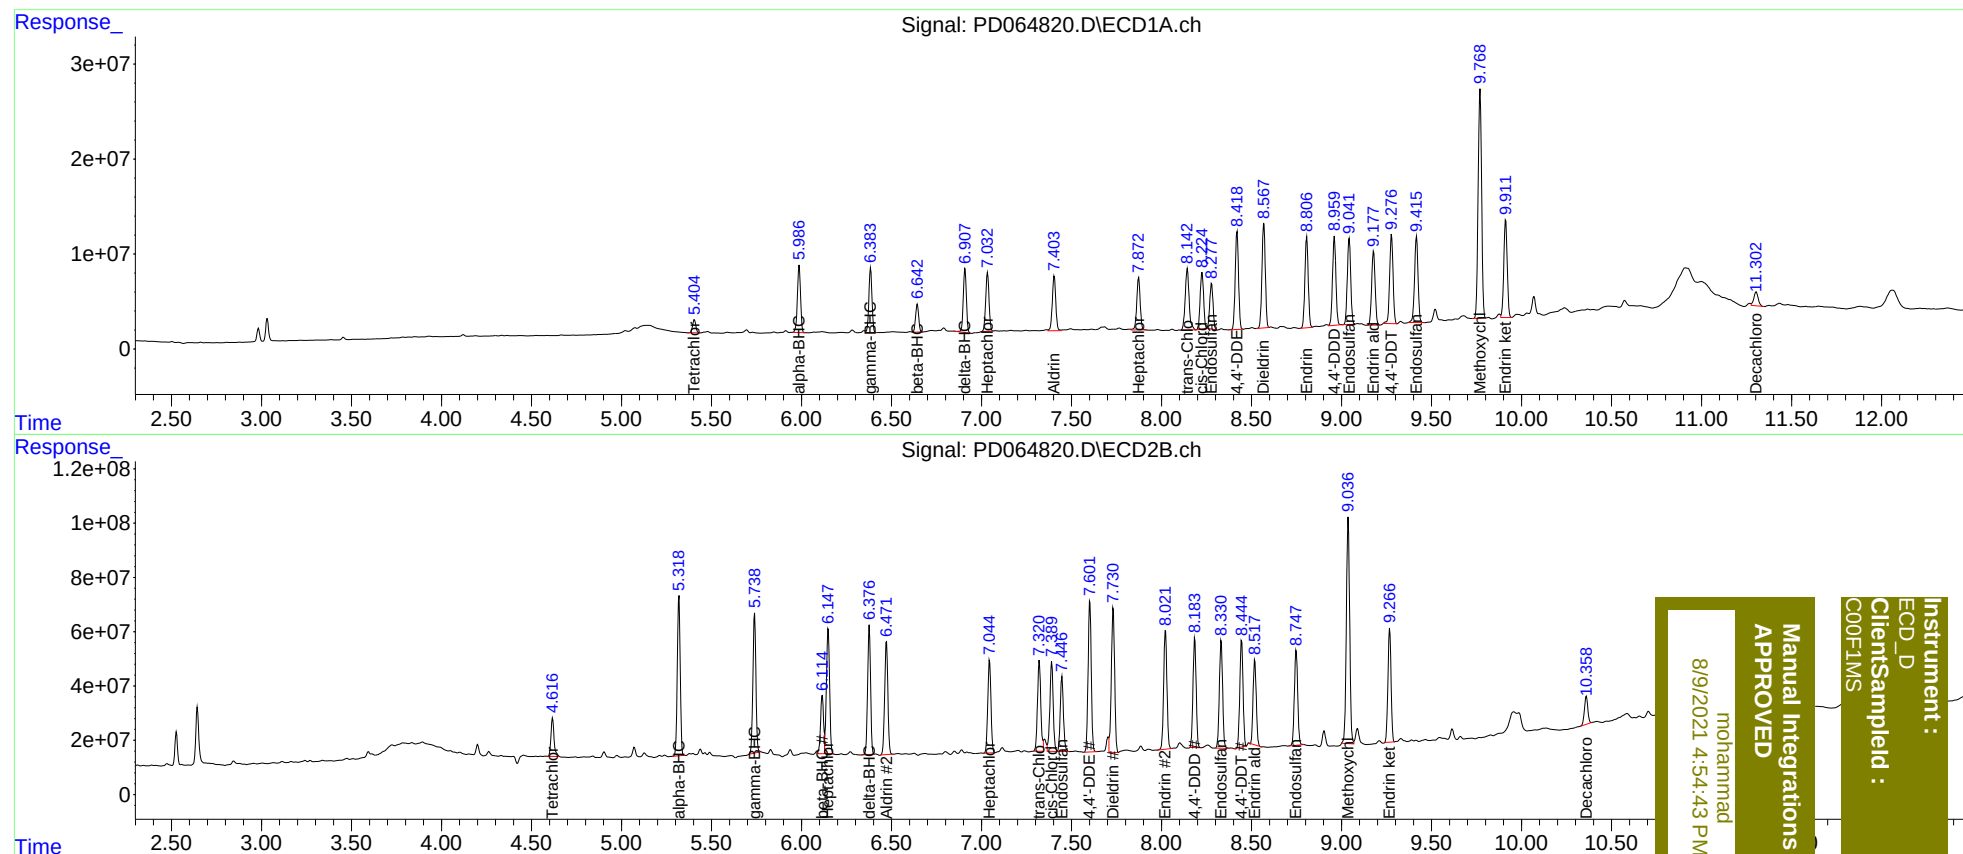

8/9/2021 4:54:43 PM

Manual Integrations
APPROVED

mohammad

Instrument :
ECD_D
ClientSampled :
C00E1MS