

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
 Data File : PD064825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2021 22:40
 Operator : AR\AJ
 Sample : M3220-03MSD
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 JCEN1MSD

Manual Integrations
 APPROVED

mohammad
 8/10/2021 4:42:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 03:00:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	21035703	187.0E6	17.634	20.465
27)	SA Decachlor...	11.302	10.360	37468273	208.5E6	28.463	35.054
Target Compounds							
2)	A alpha-BHC	5.988	5.319	96954952	739.2E6	59.515	59.975
3)	MA gamma-BHC...	6.384	5.740	90788908	663.1E6	57.888	58.153
4)	MA Heptachlor	7.034	6.147	90181354	632.8E6	53.660	55.813m
5)	MB Aldrin	7.404	6.472	85243297	578.6E6	54.117	55.005
6)	B beta-BHC	6.644	6.114	39858030	284.6E6	51.089	46.916m
7)	B delta-BHC	6.908	6.377	93932314	599.7E6	53.979	55.204
8)	B Heptachlo...	7.873	7.045	79868808	461.5E6	46.521	49.852
9)	A Endosulfan I	8.277	7.447	70415359	374.3E6	49.952	48.679
10)	B trans-Chl...	8.144	7.321	86893187	448.8E6	54.225	49.480
11)	B cis-Chlor...	8.225	7.390	76518224	423.9E6	49.110	47.648
12)	B 4,4'-DDE	8.420	7.602	155.2E6	790.5E6	107.682	104.772
13)	MA Dieldrin	8.568	7.732	164.4E6	793.0E6	110.242	98.728
14)	MA Endrin	8.807	8.022	141.6E6	637.8E6	110.626	111.034
15)	B Endosulfa...	9.043	8.331	134.9E6	568.8E6	103.897	98.541
16)	A 4,4'-DDD	8.960	8.185	137.4E6	563.1E6	111.944	97.762
17)	MA 4,4'-DDT	9.278	8.445	146.7E6	590.2E6	112.370	107.219
18)	B Endrin al...	9.178	8.518	120.4E6	462.4E6	106.237	93.683
19)	B Endosulfa...	9.416	8.749	138.4E6	510.6E6	100.390	94.722
20)	A Methoxychlor	9.769	9.038	371.3E6	1185.8E6	518.952	463.099
21)	B Endrin ke...	9.912	9.268	158.4E6	584.1E6	104.684	97.372

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080621\
Data File : PD064825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2021 22:40
Operator : AR\AJ
Sample : M3220-03MSD
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 03:00:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

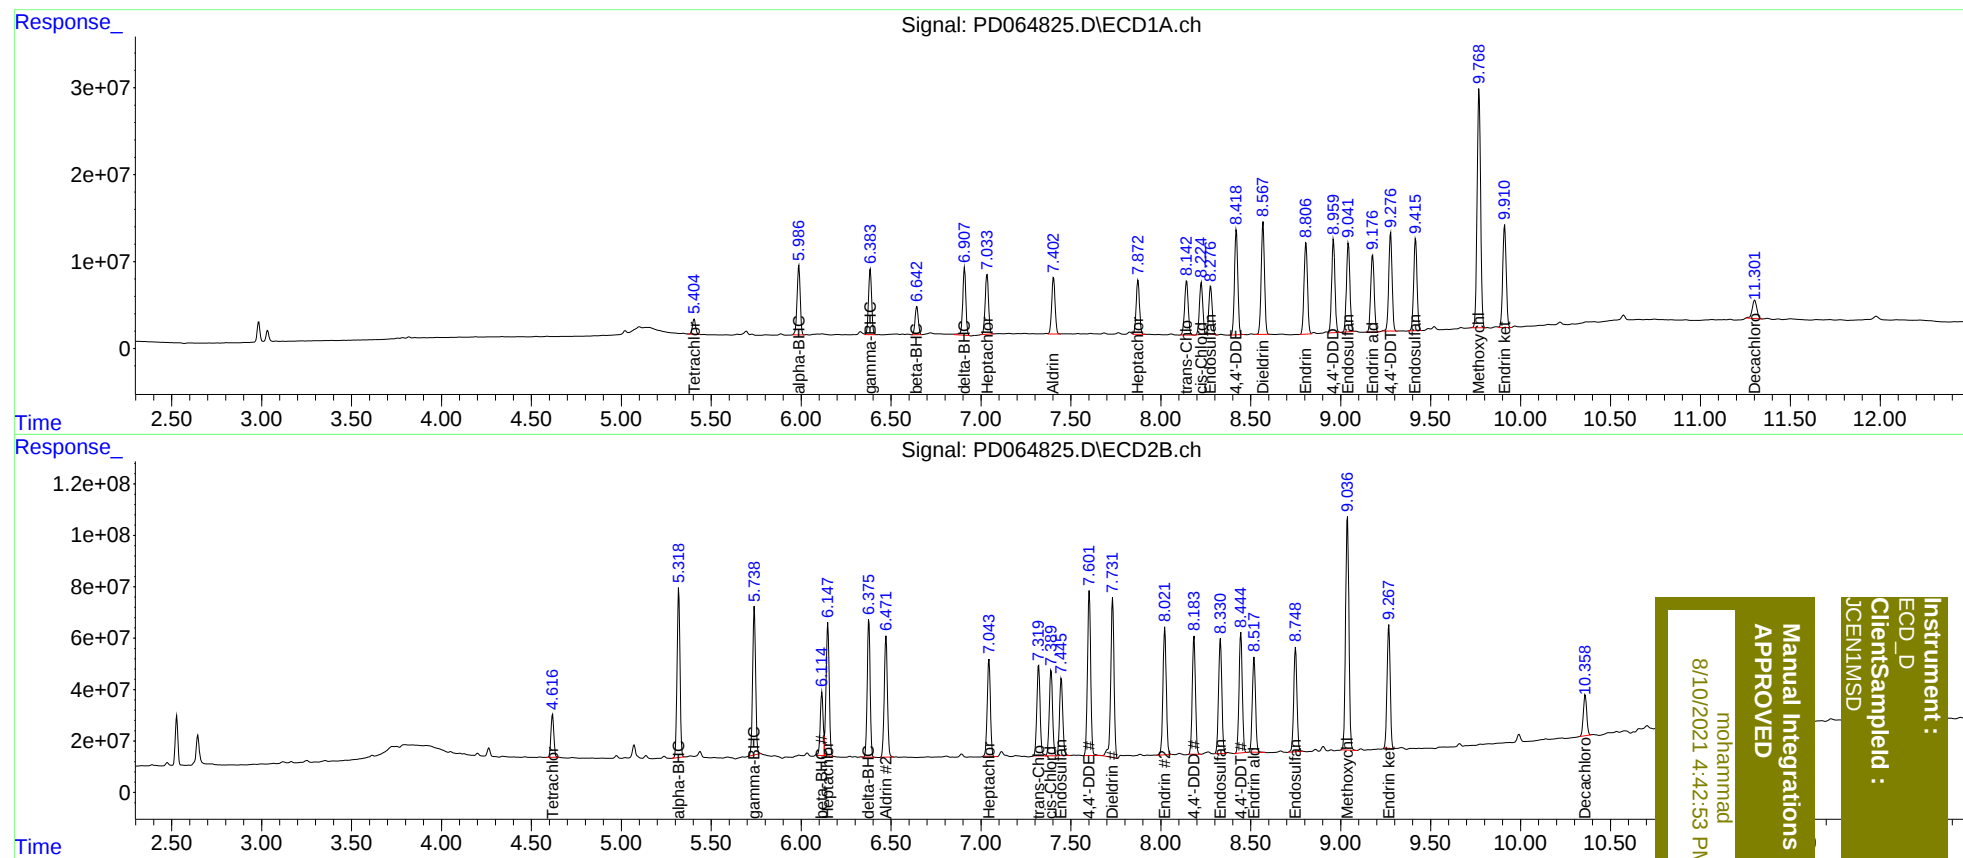

Manual Integrations
APPROVED

mohammad
8/10/2021 4:42:53 PM

Instrument :
ECD_D
Client Sampled :
JCEN1MSD