

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080624\
 Data File : PD084225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2024 13:50
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 15:57:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 16 04:22:06 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.776	0	2079	N.D.	0.000 #
28)	SA Decachlor...	0.000	7.876	0	280692	N.D.	0.044 #
Target Compounds							
2)	A alpha-BHC	0.000	3.271	0	167951	N.D.	0.019 #
3)	MA gamma-BHC...	0.000	3.593	0	510651	N.D.	0.064 #
8)	B Heptachlo...	5.718	0.000	237984	0	0.133	N.D. #
9)	A Endosulfan I	0.000	5.102f	0	497806	N.D.	0.072 #
10)	B gamma-Chl...	5.975	0.000	475964	0	0.238	N.D. #
14)	MA Endrin	0.000	5.641f	0	98320	N.D.	0.015 #
24)	Chlordane-2	5.255	4.354	65114	1436833	0.937	5.120 #
25)	Chlordane-3	5.975	0.000	475964	0	1.565	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080624\
Data File : PD084225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2024 13:50
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 15:57:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071524.M
Quant Title : GC Extractables
QLast Update : Tue Jul 16 04:22:06 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

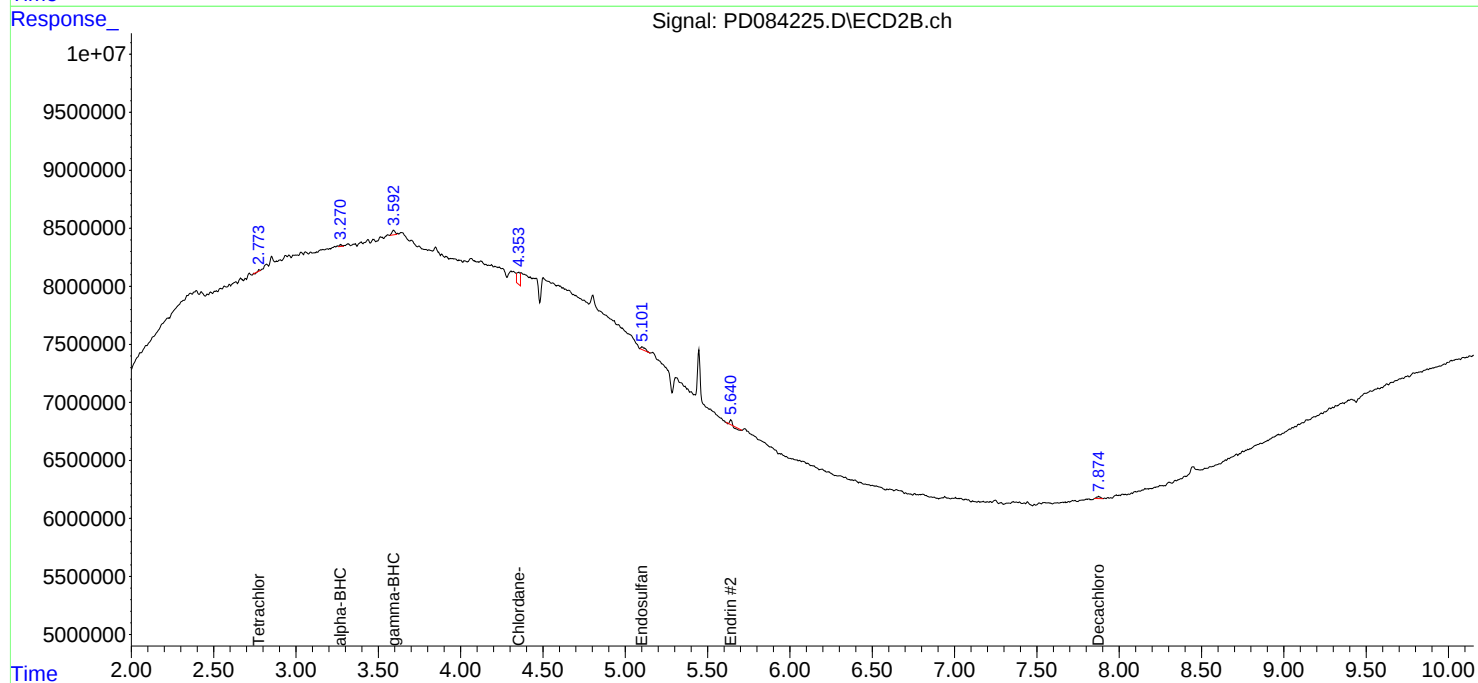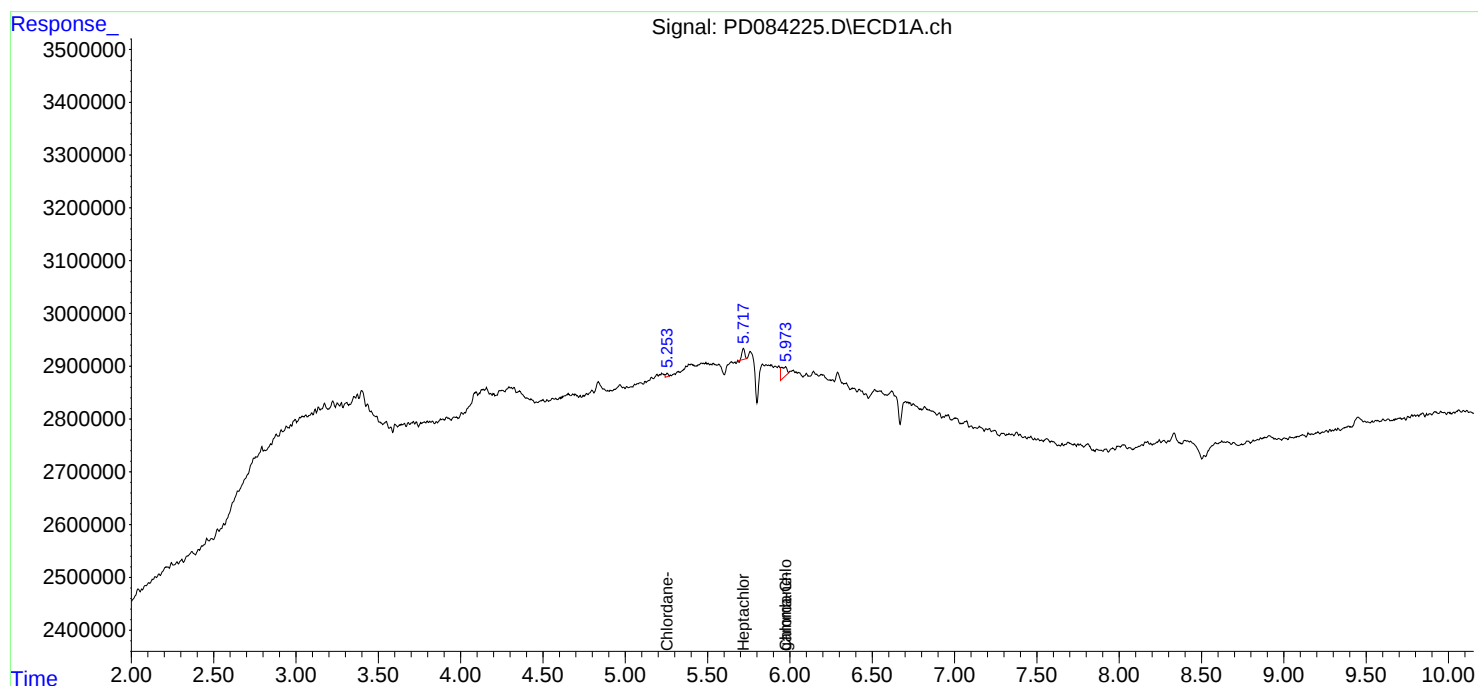


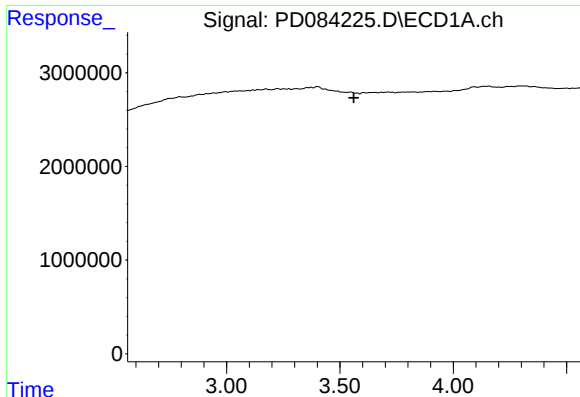

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.561 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

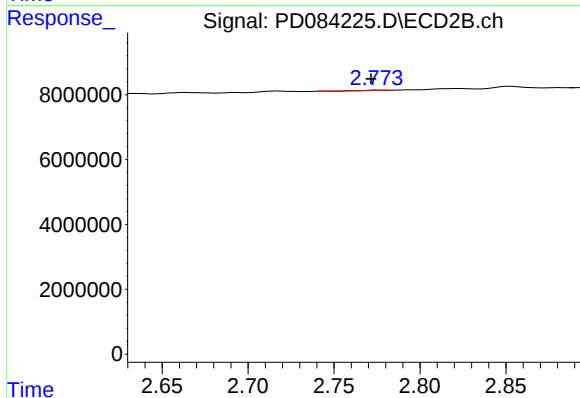


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.005 min
Response: 2079
Conc: 0.00 ng/ml

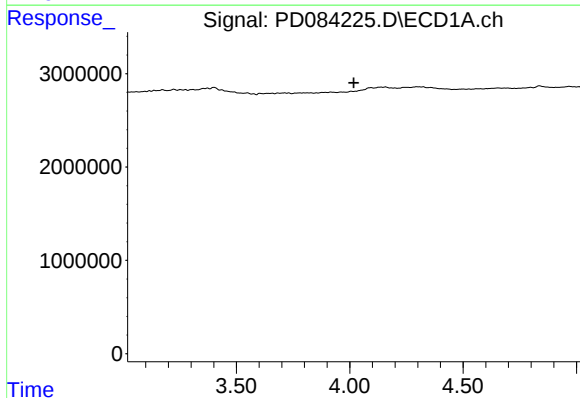


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.018 min
Response: 0
Conc: N.D.

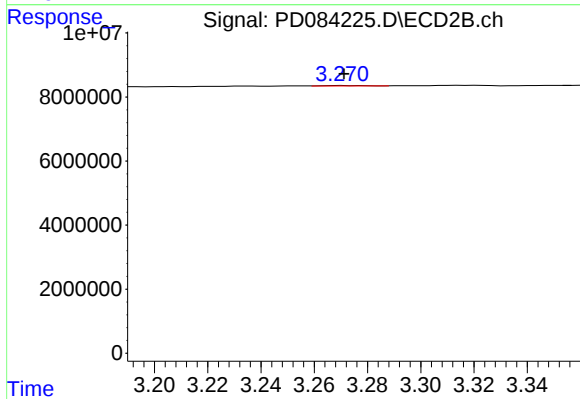

#2 alpha-BHC


R.T.: 3.271 min
Delta R.T.: 0.000 min
Response: 167951
Conc: 0.02 ng/ml

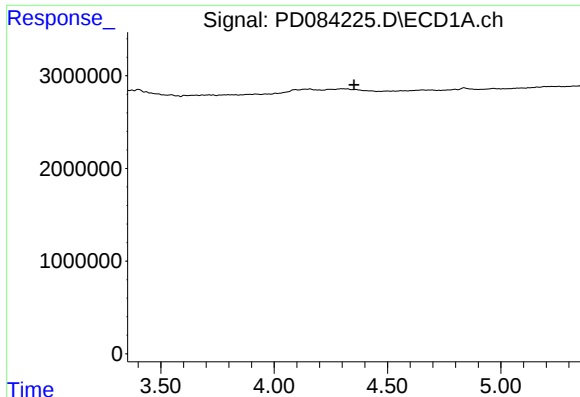

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

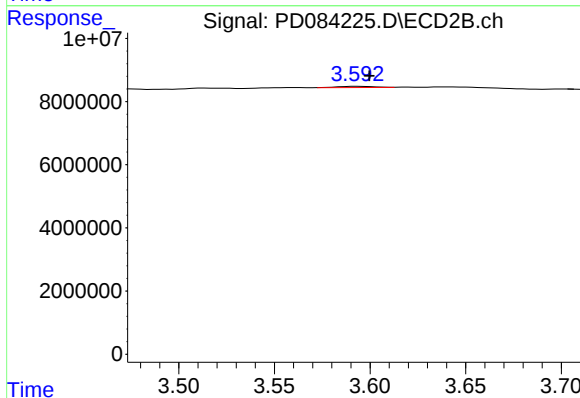


#3 gamma-BHC (Lindane)

R.T.: 3.593 min
Delta R.T.: -0.006 min
Response: 510651
Conc: 0.06 ng/ml

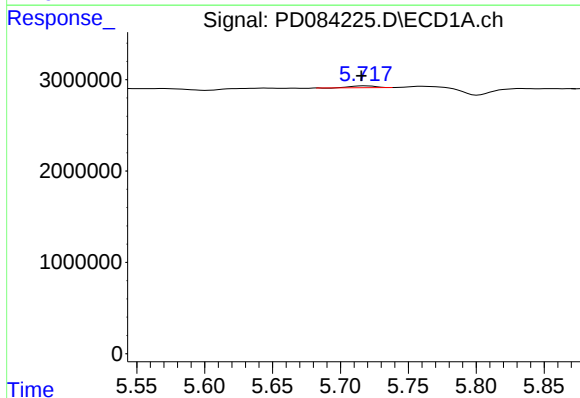


#8 Heptachlor epoxide

R.T.: 5.718 min
Delta R.T.: 0.003 min
Response: 237984
Conc: 0.13 ng/ml

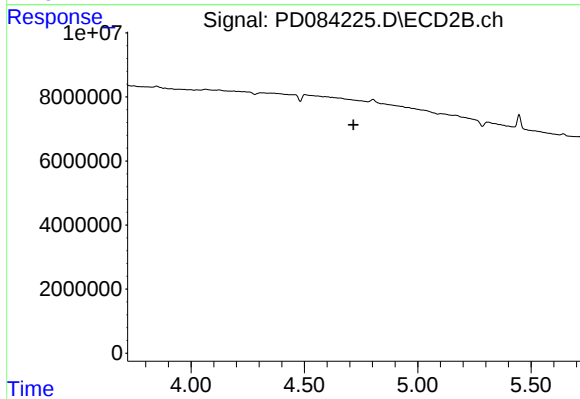

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.717 min
Response: 0
Conc: N.D.

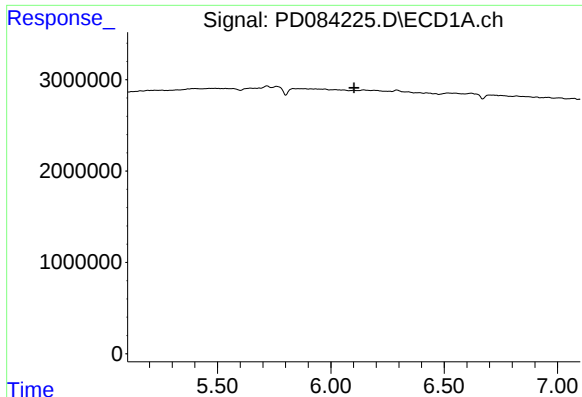

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.103 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

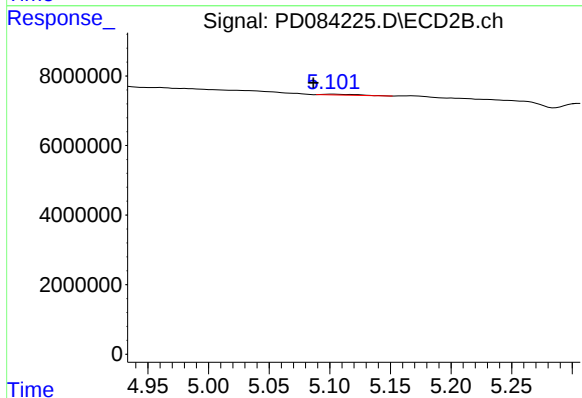


#9 Endosulfan I

R.T.: 5.102 min
Delta R.T.: 0.016 min
Response: 497806
Conc: 0.07 ng/ml

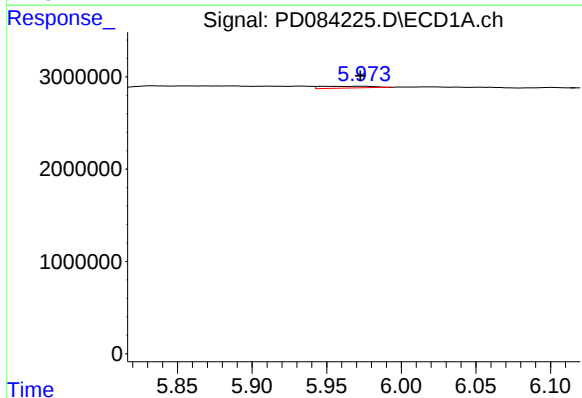


#10 gamma-Chlordane

R.T.: 5.975 min
Delta R.T.: 0.002 min
Response: 475964
Conc: 0.24 ng/ml

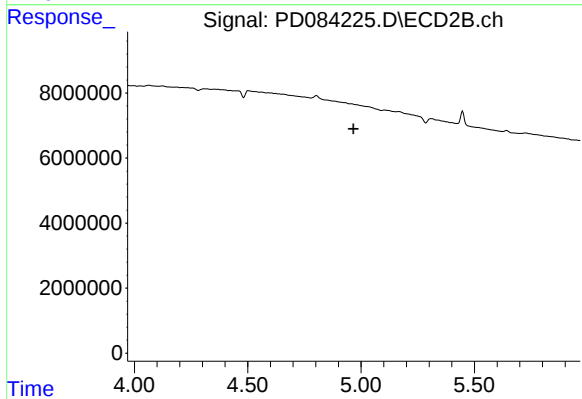

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.967 min
Response: 0
Conc: N.D.

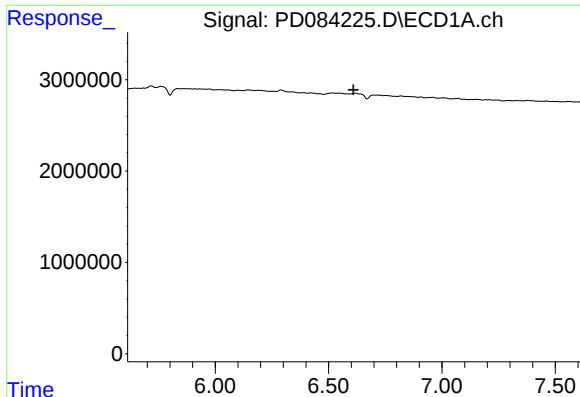

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.610 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

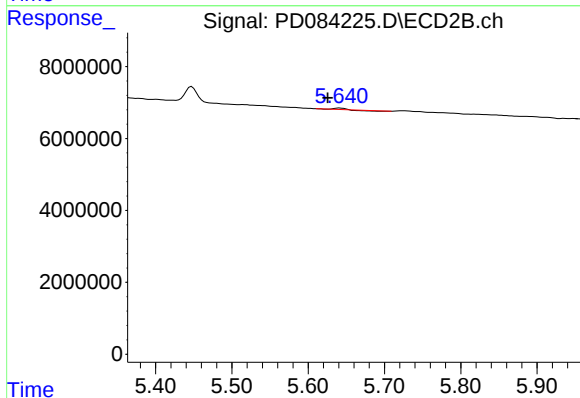


#14 Endrin

R.T.: 5.641 min
Delta R.T.: 0.016 min
Response: 98320
Conc: 0.01 ng/ml

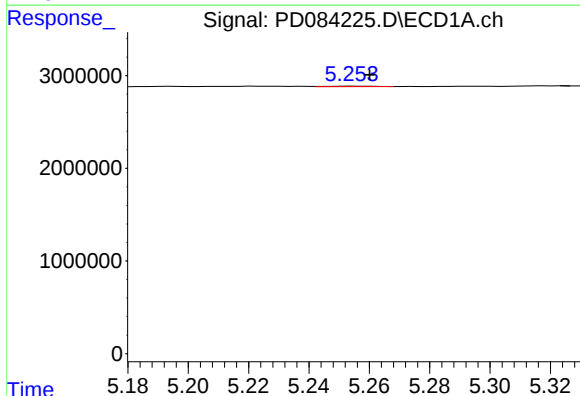


#24 Chlordane-2

R.T.: 5.255 min
Delta R.T.: -0.005 min
Response: 65114
Conc: 0.94 ng/ml

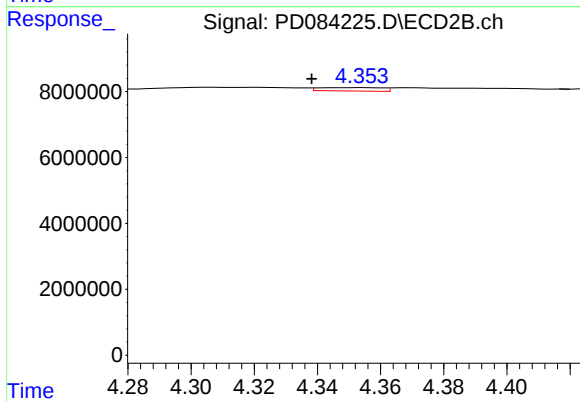

#24 Chlordane-2


R.T.: 4.354 min
Delta R.T.: 0.016 min
Response: 1436833
Conc: 5.12 ng/ml

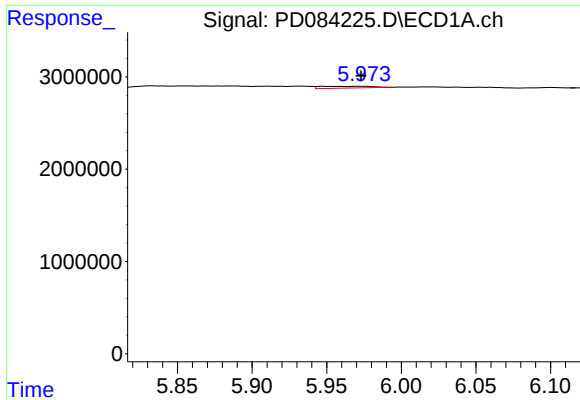

#25 Chlordane-3


R.T.: 5.975 min
Delta R.T.: 0.002 min
Response: 475964
Conc: 1.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

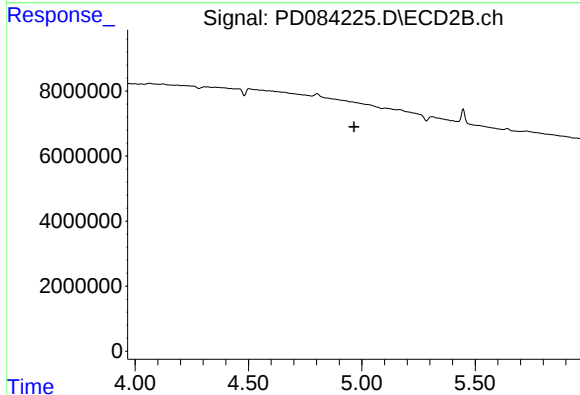


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.966 min
Response: 0
Conc: N.D.

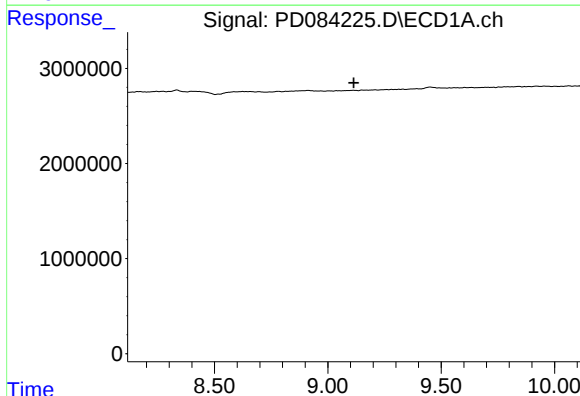

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.114 min
Response: 0
Conc: N.D.

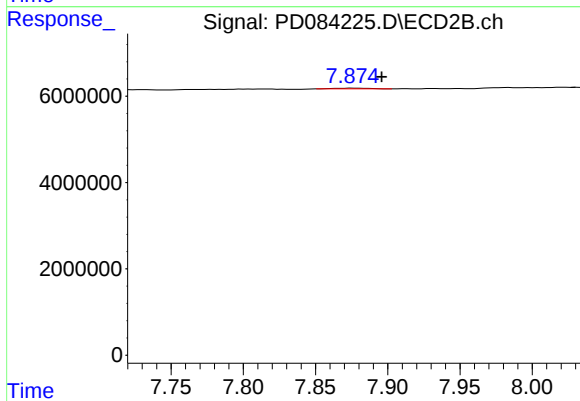

#28 Decachlorobiphenyl

R.T.: 7.876 min
Delta R.T.: -0.020 min
Response: 280692
Conc: 0.04 ng/ml