

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 18:48
 Operator : AR\AJ
 Sample : PIBLK046
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK205

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:21:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.560	2.770	22796267	143.9E6	25.460	27.578
2)	SA Decachlor...	9.111	7.892	48029239	150.9E6	25.023	26.173
Target Compounds							
3)	MA gamma-BHC...	4.308f	0.000	82432112	0	49.901	N.D. #
8)	B Heptachlo...	5.656f	0.000	855564	0	0.463	N.D. #
10)	B trans-Chl...	6.003	0.000	1398337	0	0.788	N.D. #
11)	B cis-Chlor...	6.003f	0.000	1398337	0	0.766	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 18:48
Operator : AR\AJ
Sample : PIBLK046
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:21:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

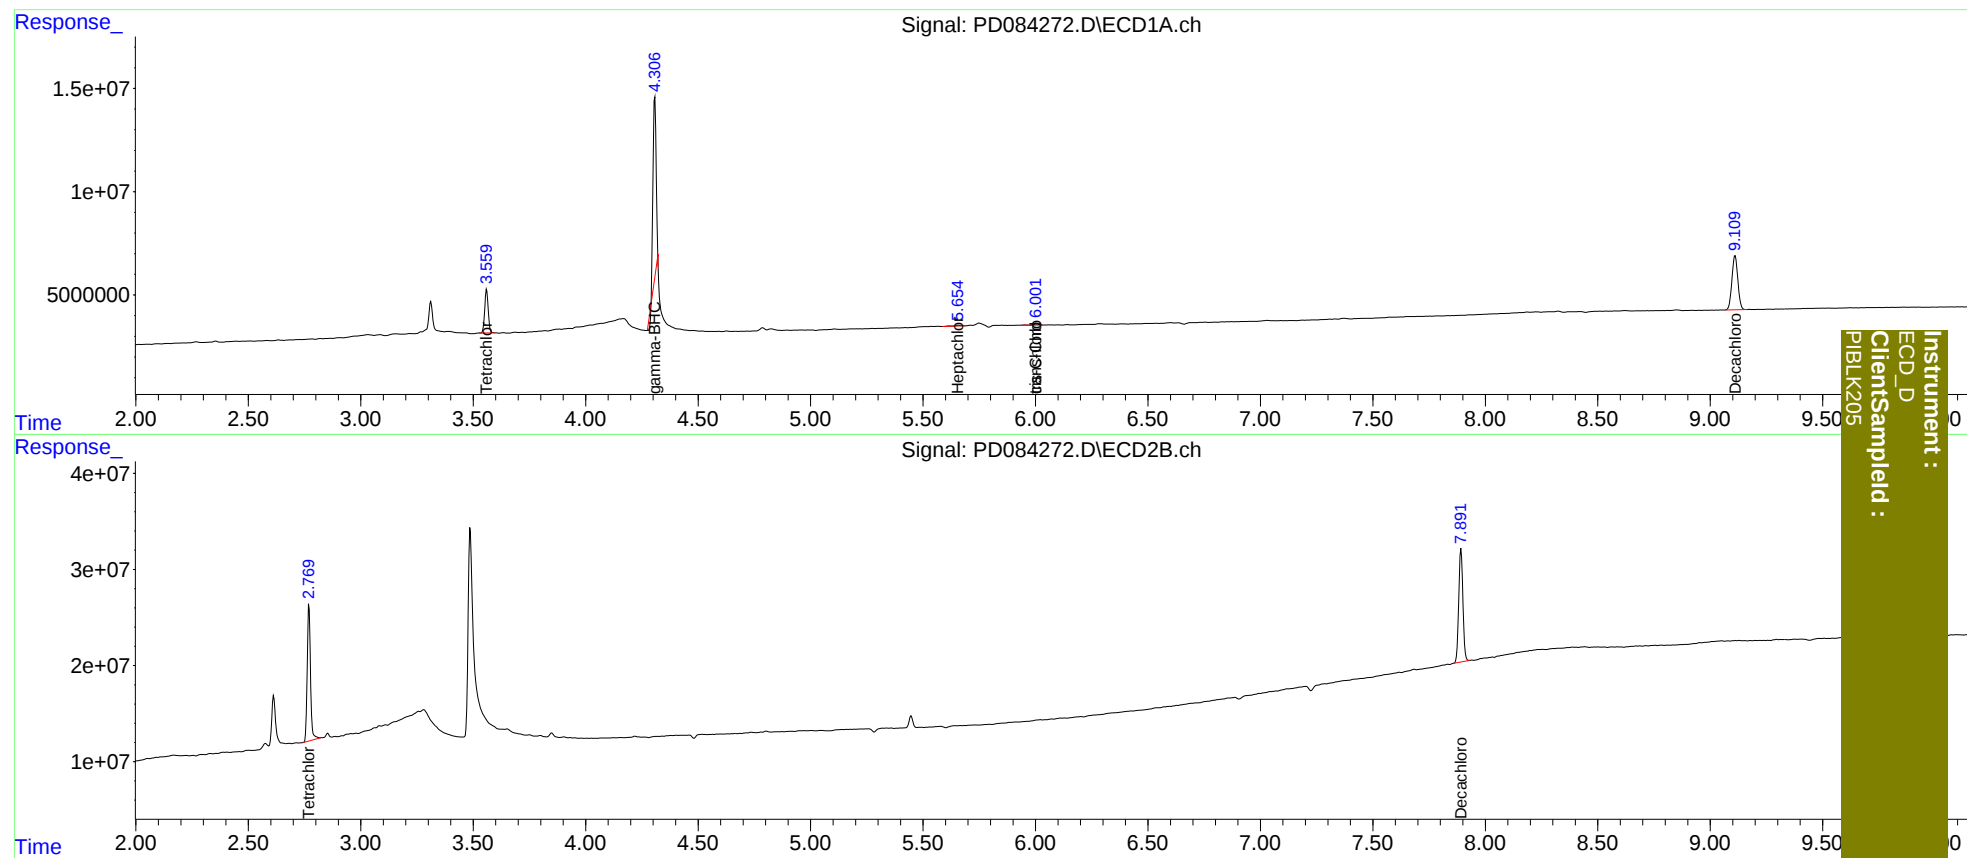


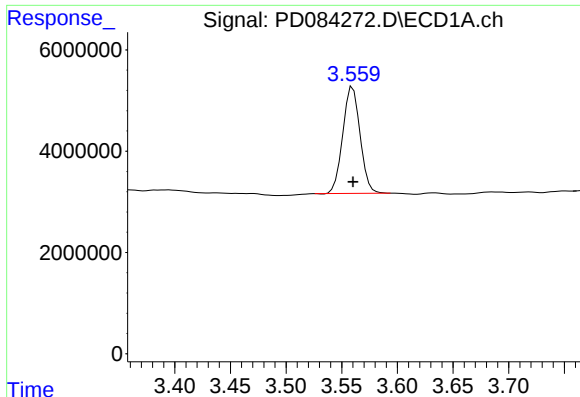

#1 Tetrachloro-m-xylene


R.T.: 3.560 min
Delta R.T.: 0.000 min
Response: 22796267
Conc: 25.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK205

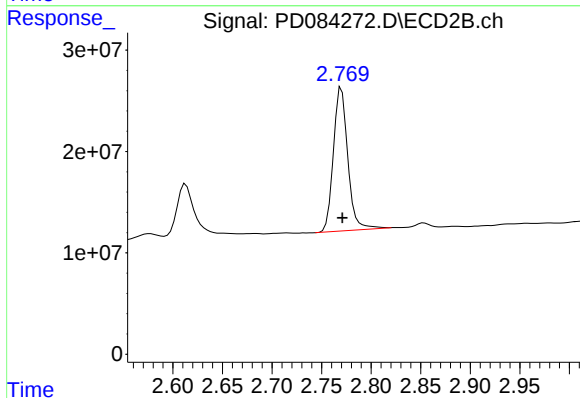


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.001 min
Response: 143857154
Conc: 27.58 ng/ml

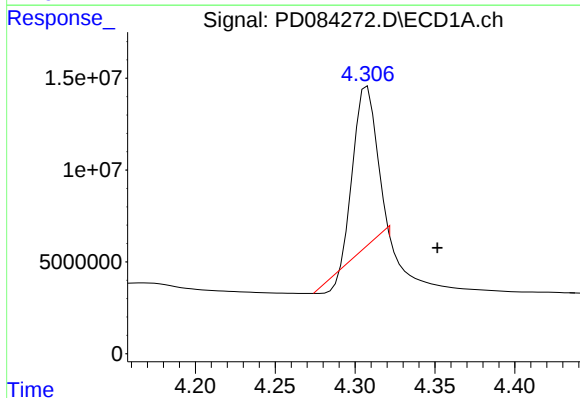


#3 gamma-BHC (Lindane)

R.T.: 4.308 min
Delta R.T.: -0.044 min
Response: 82432112
Conc: 49.90 ng/ml

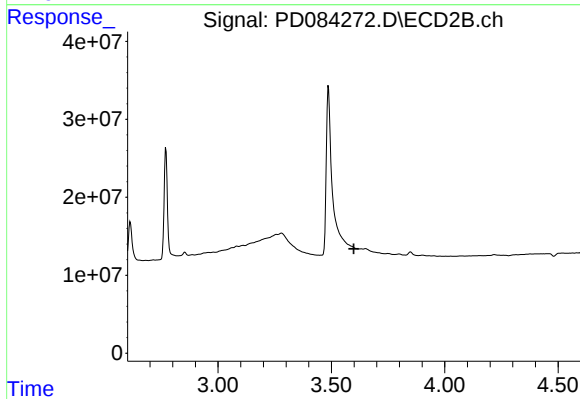

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.599 min
Response: 0
Conc: N.D.

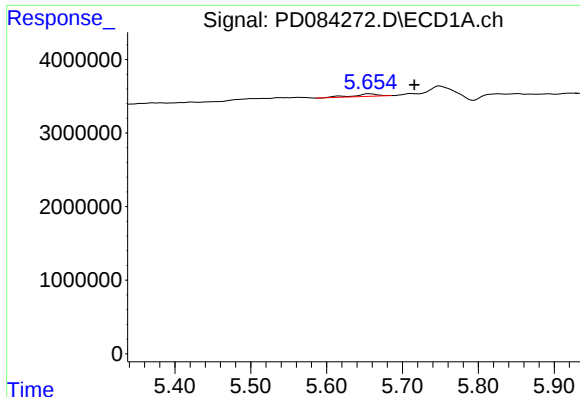

#8 Heptachlor epoxide


R.T.: 5.656 min
Delta R.T.: -0.060 min
Response: 855564
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK205

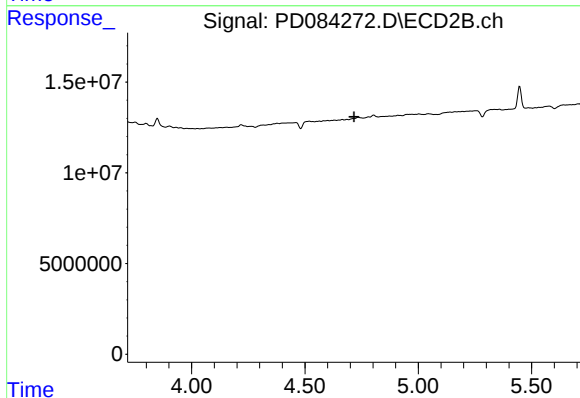


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

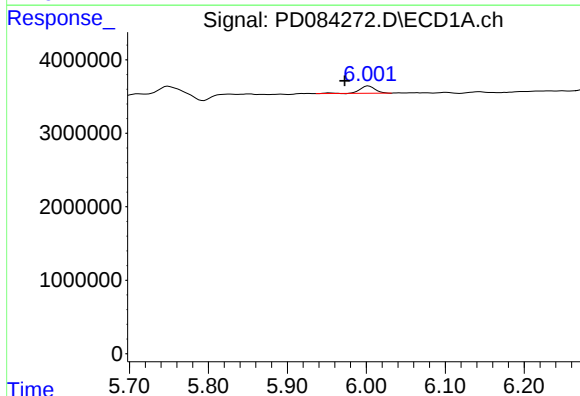


#10 trans-Chlordane

R.T.: 6.003 min
Delta R.T.: 0.030 min
Response: 1398337
Conc: 0.79 ng/ml

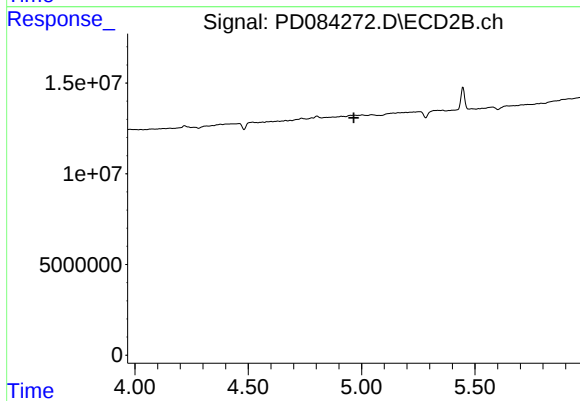

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.965 min
Response: 0
Conc: N.D.

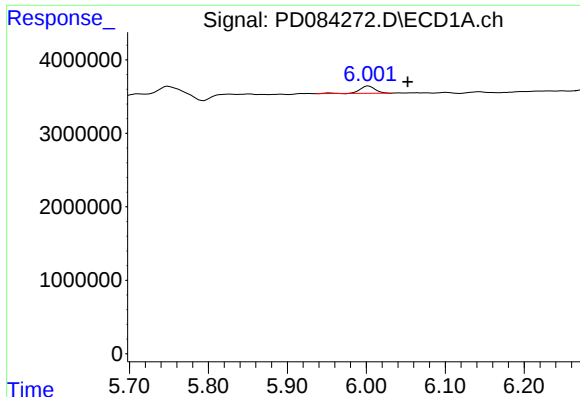

#11 cis-Chlordane


R.T.: 6.003 min
Delta R.T.: -0.049 min
Response: 1398337
Conc: 0.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK205

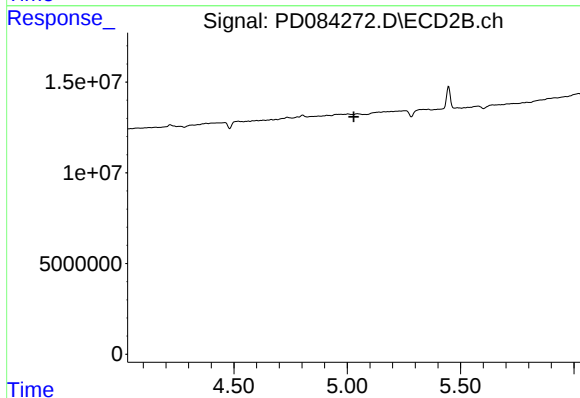


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.029 min
Response: 0
Conc: N.D.

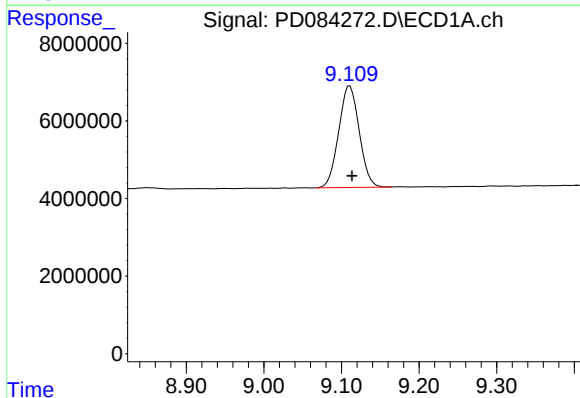

#27 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: -0.003 min
Response: 48029239
Conc: 25.02 ng/ml

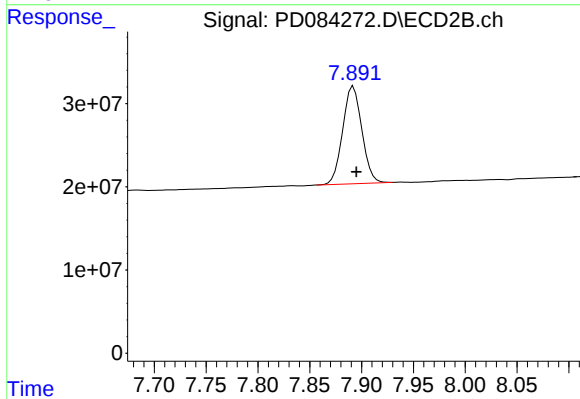

#27 Decachlorobiphenyl

R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 150882922
Conc: 26.17 ng/ml