

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084256.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 12:40
 Operator : AR\AJ
 Sample : P3171-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVX5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:16:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.558	2.774	7748321	62596486	8.654m	12.000m#
2) SA Decachlor...	9.114	7.893	26725095	79155122	13.924	13.731
Target Compounds						
2) A alpha-BHC	4.018	3.269	17832453	82437382	10.718	9.644
7) B delta-BHC	4.797	4.122	33831643	119.0E6	16.873m	13.964m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084256.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 12:40
Operator : AR\AJ
Sample : P3171-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:16:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

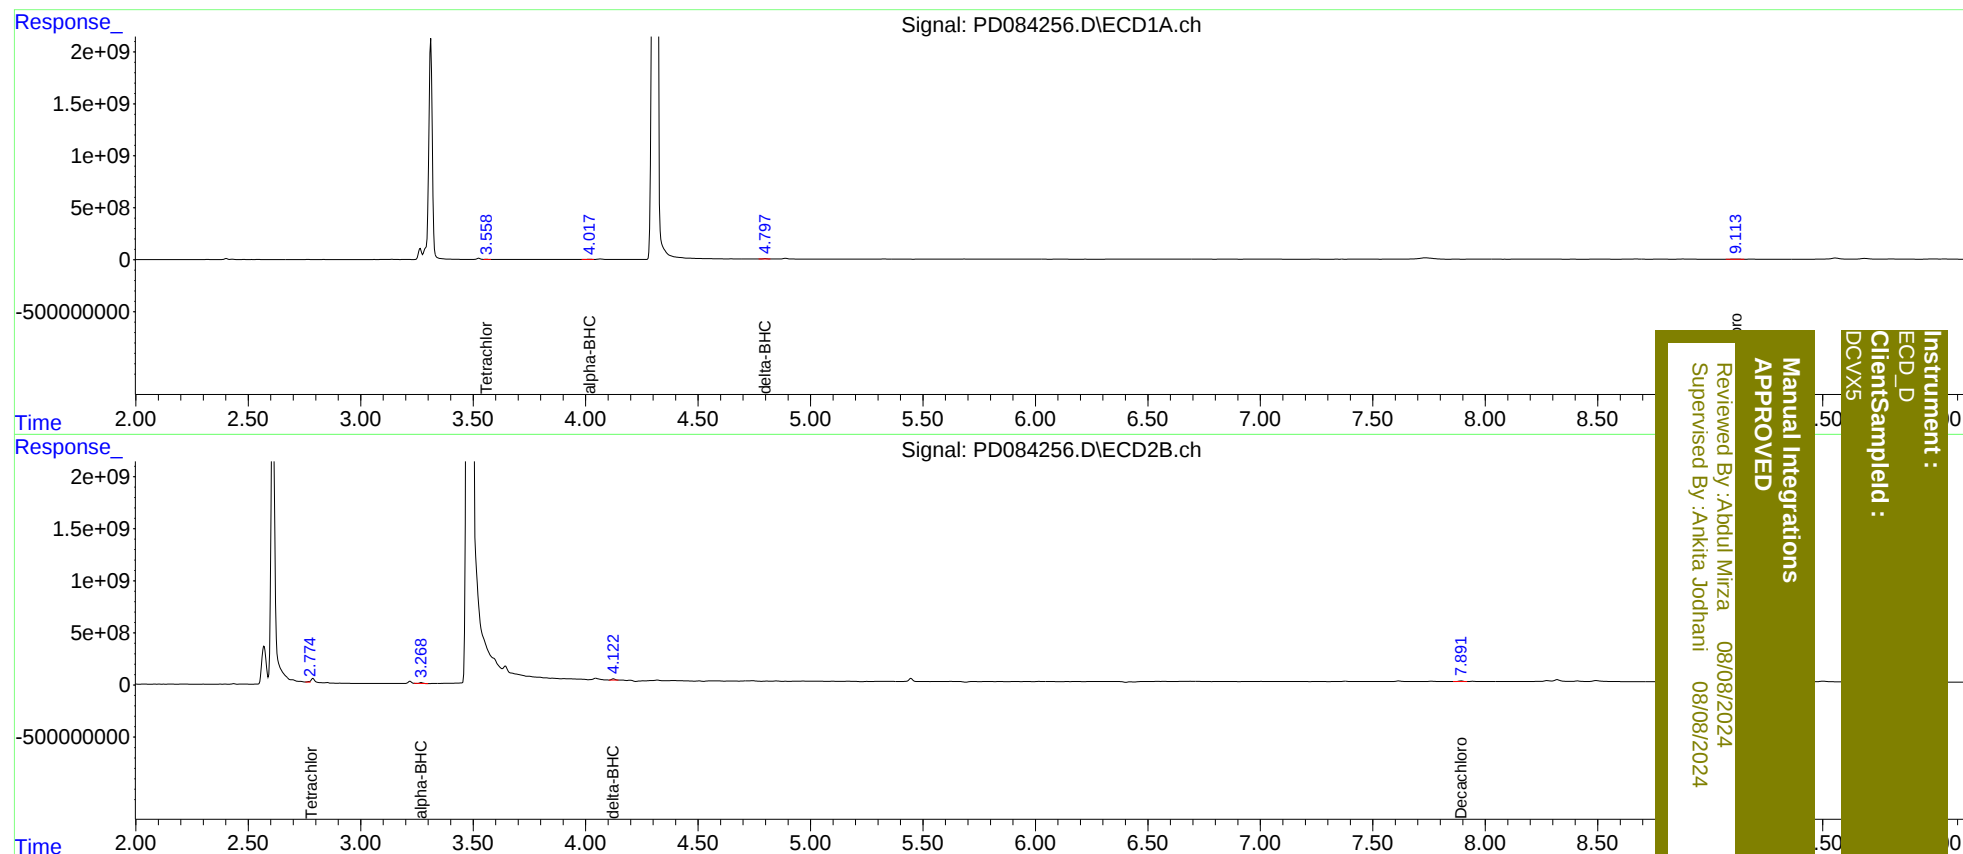

Reviewed By: Abdul Mirza 08/08/2024
Supervised By: Ankita Jodhani 08/08/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DCVX5