

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 10:26
 Operator : AR\AJ
 Sample : P3171-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVT1

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:14:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.769	18120187	108.8E6	20.237	20.860m
2)	SA Decachlor...	9.110	7.892	35594811	115.6E6	18.545m	20.061
Target Compounds							
2)	A alpha-BHC	4.018	3.268	1441.4E6	4606.5E6	866.309m	538.870m#
3)	MA gamma-BHC...	4.353	3.598	1540.7E6	5246.6E6	932.647	668.788 #
4)	MA Heptachlor	4.945	3.936	2609.5E6	7664.6E6	1420.509	988.344 #
5)	MB Aldrin	5.288	4.214	1100.4E6	3340.1E6	595.946	424.317 #
6)	B beta-BHC	4.550	3.895	619.8E6	2554.8E6	829.306	714.939
7)	B delta-BHC	4.799	4.123	789.0E6	3056.5E6	393.499	358.800
8)	B Heptachlo...	5.716	4.715	832.5E6	2805.7E6	450.372	386.833
9)	A Endosulfan I	6.103	5.084	897.5E6	2680.0E6	519.391	414.596
10)	B trans-Chl...	5.973	4.964	806.8E6	2822.4E6	454.675	398.517
11)	B cis-Chlor...	6.051	5.028	663.9E6	2368.6E6	363.871	327.642
12)	B 4,4'-DDE	6.224	5.216	2355.8E6	6953.6E6	1280.957	1012.125
13)	MA Dieldrin	6.379	5.348	2053.2E6	5830.9E6	1102.494	822.858 #
14)	MA Endrin	6.610	5.623	377.6E6	1281.6E6	236.908	210.154
15)	B Endosulfa...	6.829	5.917	1428.9E6	3895.6E6	813.204	648.851
16)	A 4,4'-DDD	6.742	5.770	1520.8E6	4659.8E6	1159.411	890.527
17)	MA 4,4'-DDT	7.057	6.020	1593.4E6	4425.4E6	1124.994	847.377
18)	B Endrin al...	6.959	6.096	244.7E6	823.3E6	195.142	186.057
19)	B Endosulfa...	7.194	6.319	357.2E6	1215.0E6	219.609	211.657
20)	A Methoxychlor	7.534	6.593	204.8E6	598.7E6	243.648	232.083
21)	B Endrin ke...	7.682	6.824	1595.7E6	4166.9E6	885.615	669.240

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 10:26
Operator : AR\AJ
Sample : P3171-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:14:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

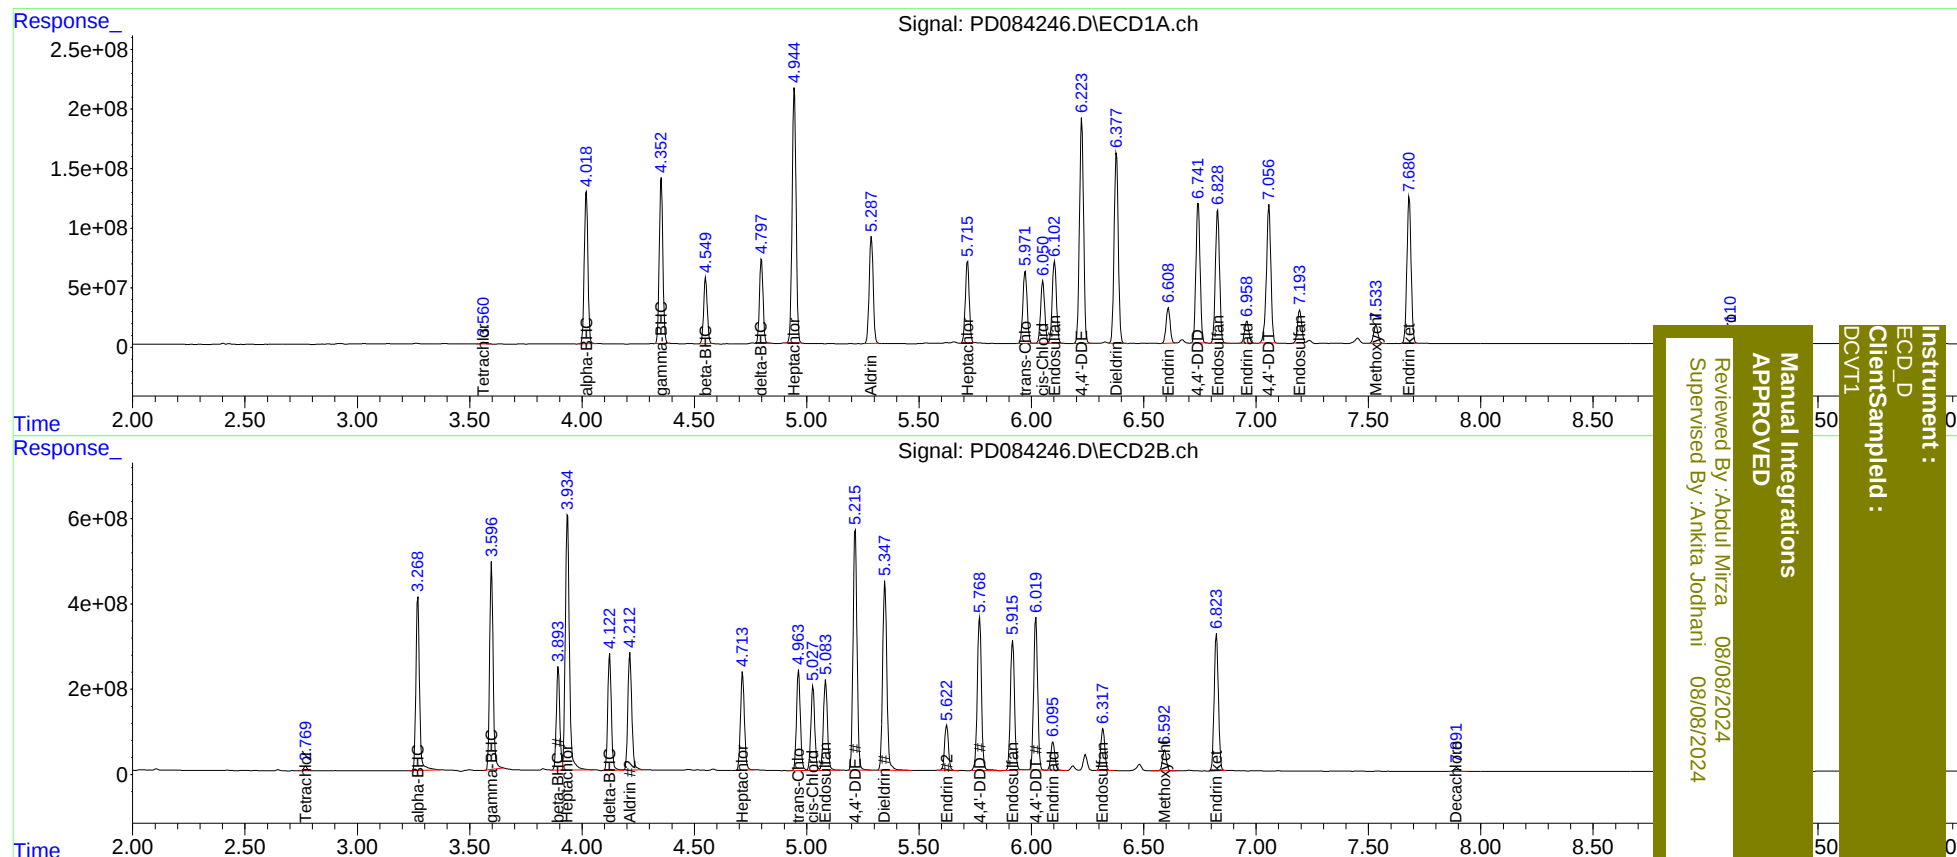

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 08/08/2024
Supervised By: Ankita Jodhani 08/08/2024

Instrument :
ECD_D
ClientSampled :
DCVT1