

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 11:46
 Operator : AR\AJ
 Sample : P3171-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVX0

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:15:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.765	6479844	6367913	7.237m	1.221m#
2) SA Decachlor...	9.112	7.889	18562868	26956566	9.671m	4.676m#
Target Compounds						
2) A alpha-BHC	4.019	3.270	57525640	218.8E6	34.574	25.598 #
7) B delta-BHC	4.799	4.124	114.6E6	414.1E6	57.141	48.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 11:46
Operator : AR\AJ
Sample : P3171-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:15:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

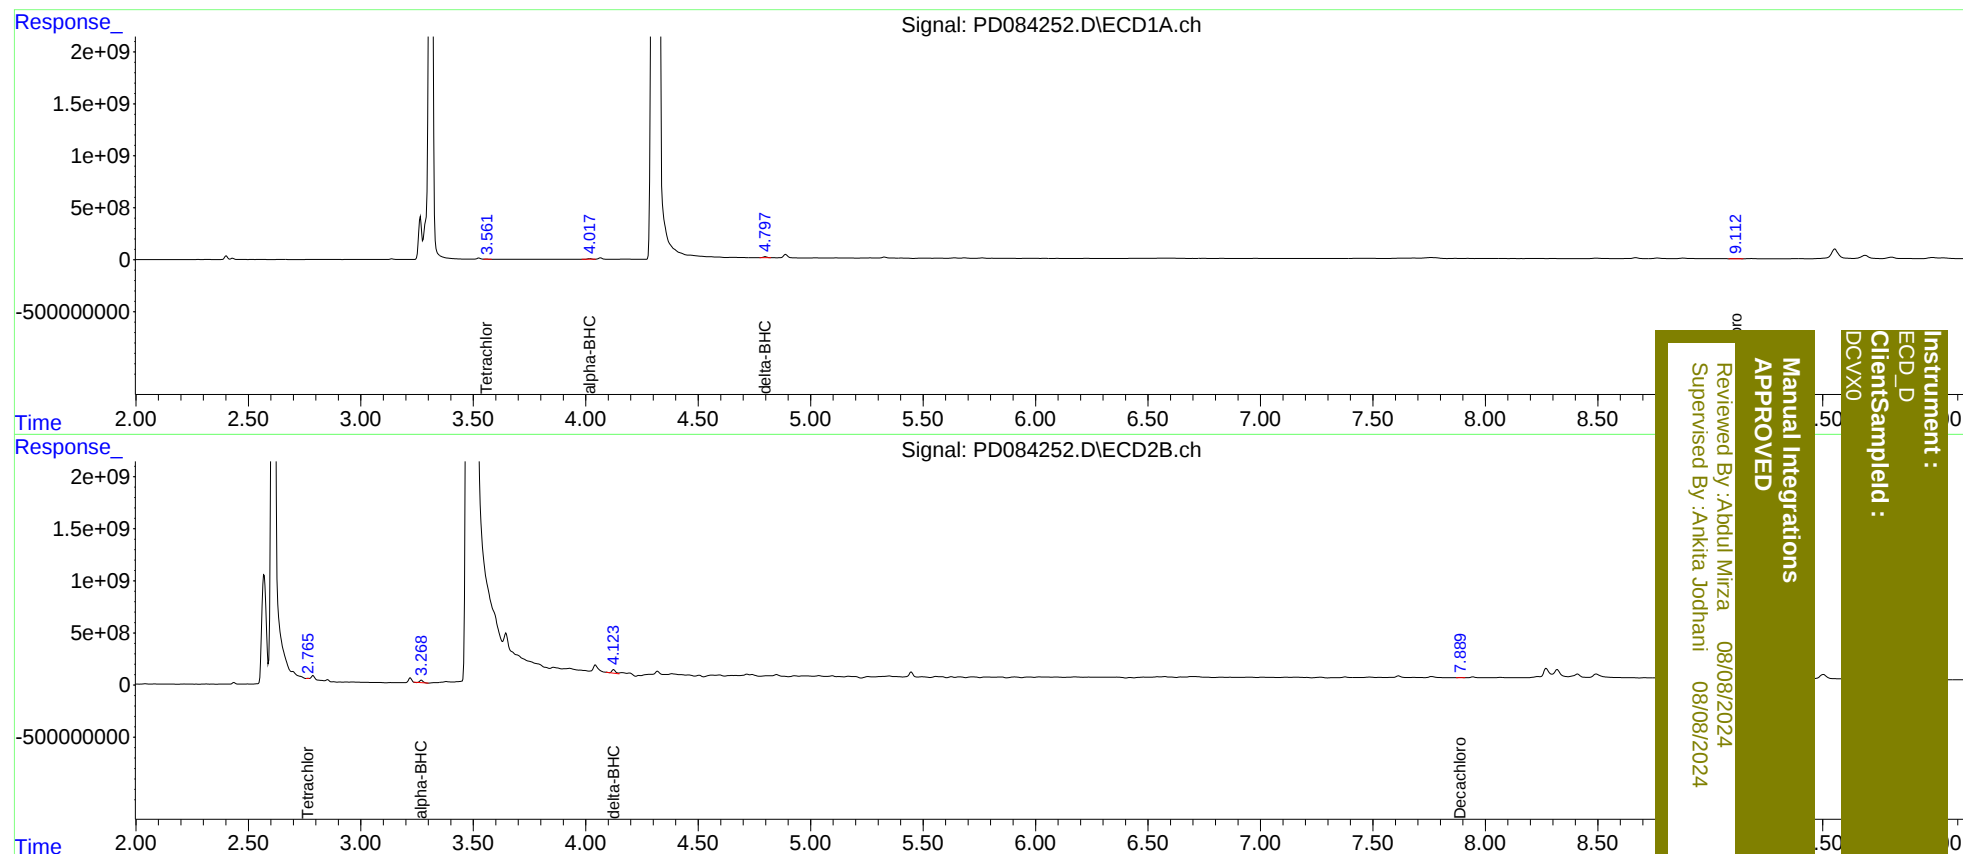

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/08/2024
Supervised By: Ankita Jodhani 08/08/2024

Instrument :
ECD_D
ClientSampled :
DCVX0