

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 12:53
 Operator : AR\AJ
 Sample : P3171-02DL 2X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVT1DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 01:17:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.559	2.769	8143110	64908127	9.095m	12.443m#
27) SA Decachlor...	9.112	7.893	17663461	58082408	9.203	10.075
Target Compounds						
2) A alpha-BHC	4.017	3.268	695.5E6	2577.9E6	418.000m	301.559m#
3) MA gamma-BHC...	4.351	3.598	747.9E6	2778.7E6	452.765m	354.203
4) MA Heptachlor	4.944	3.936	1284.0E6	4317.0E6	698.959	556.679
5) MB Aldrin	5.287	4.214	528.3E6	1854.2E6	286.098	235.547
6) B beta-BHC	4.550	3.895	303.0E6	1362.1E6	405.457	381.177
7) B delta-BHC	4.798	4.124	378.8E6	1641.0E6	188.899	192.637
8) B Heptachlo...	5.715	4.715	408.4E6	1532.3E6	220.925	211.261
9) A Endosulfan I	6.102	5.085	437.6E6	1474.3E6	253.222	228.074
10) B trans-Chl...	5.972	4.965	392.1E6	1497.7E6	220.950	211.469
11) B cis-Chlor...	6.051	5.028	322.6E6	1249.1E6	176.785	172.786
12) B 4,4'-DDE	6.224	5.216	1138.1E6	3795.2E6	618.815	552.411
13) MA Dieldrin	6.378	5.348	1007.8E6	3231.5E6	541.119	456.034
14) MA Endrin	6.609	5.624	180.6E6	683.9E6	113.331	112.137
15) B Endosulfa...	6.829	5.916	698.1E6	2152.7E6	397.273	358.549m
16) A 4,4'-DDD	6.743	5.769	729.8E6	2562.5E6	556.351	489.723m
17) MA 4,4'-DDT	7.057	6.020	765.1E6	2355.7E6	540.195	451.076
18) B Endrin al...	6.959	6.096	117.3E6	420.8E6	93.512	95.094
19) B Endosulfa...	7.194	6.319	177.6E6	641.1E6	109.164	111.690
20) A Methoxychlor	7.534	6.594	95845917	318.0E6	114.042	123.263
21) B Endrin ke...	7.681	6.824	751.6E6	2307.9E6	417.144	370.662

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 12:53
Operator : AR\AJ
Sample : P3171-02DL 2X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 01:17:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

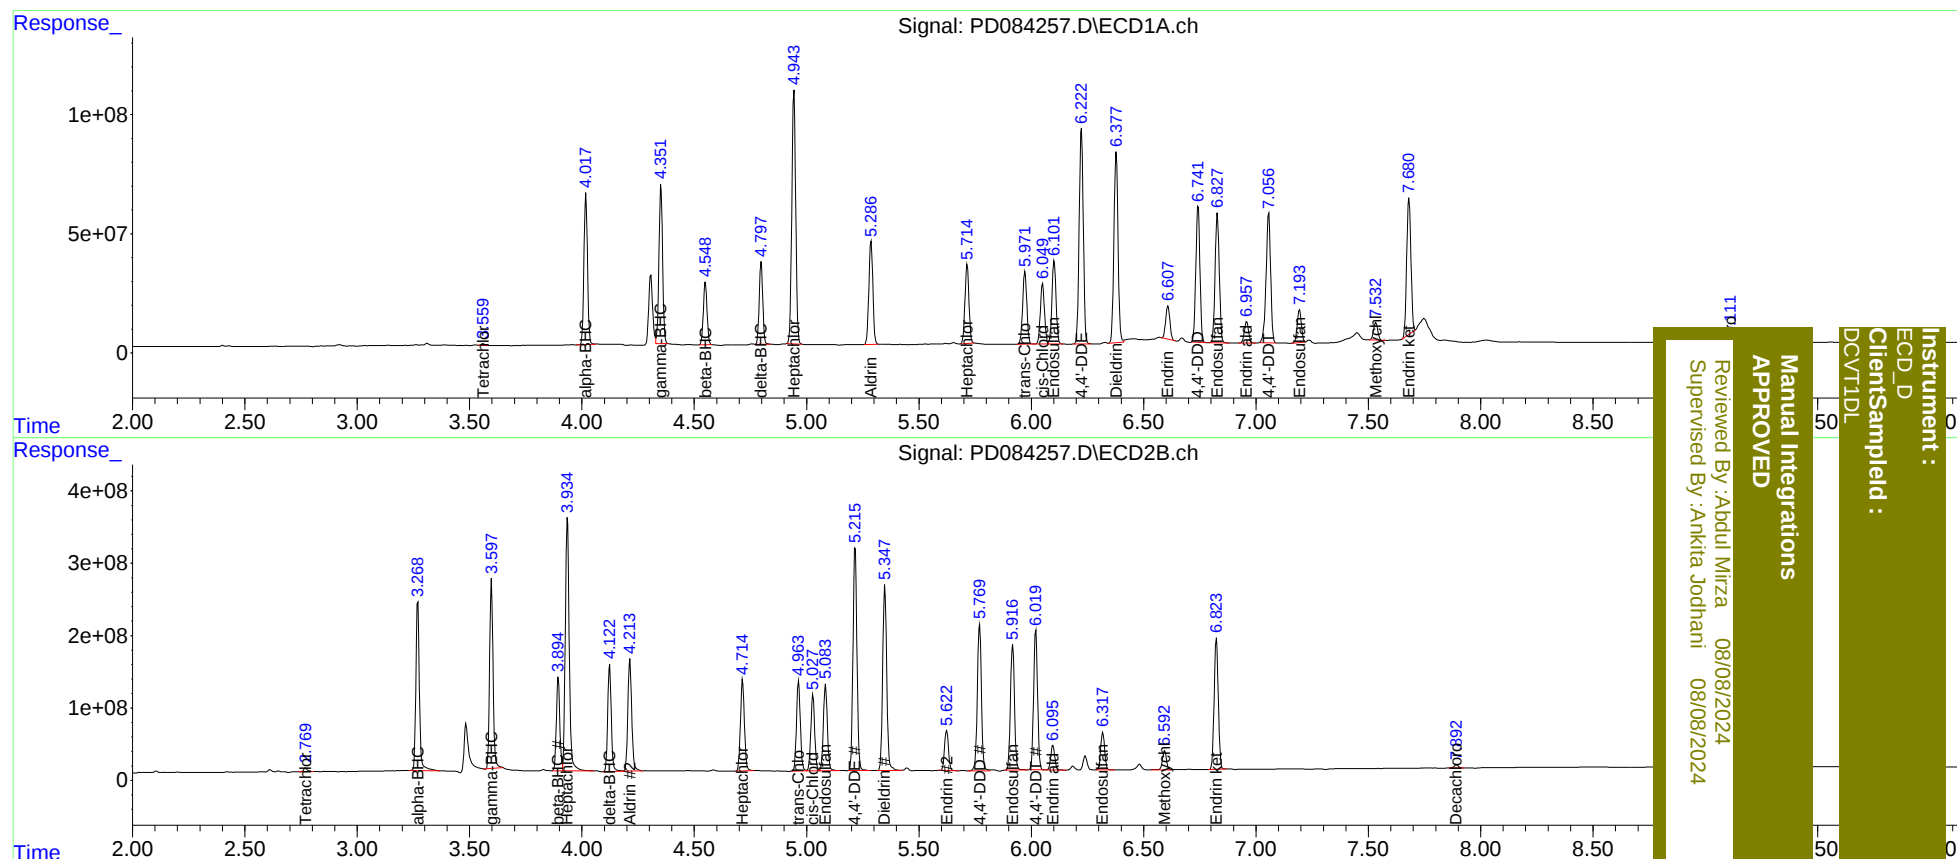

Instrument :
ECD_D
Client Sampled :
DCVTIDL

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 08/08/2024
Supervised By: Ankita Jodhani 08/08/2024