

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
 Data File : PD084270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Aug 2024 18:21
 Operator : AR\AJ
 Sample : P3439-03MSD
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVW9MSD

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 08/08/2024
 Supervised By :Ankita Jodhani 08/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 07 14:26:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 25 11:17:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.787	3316686	3049.6E6	3.704m	584.624m#
27)	SA Decachlor...	9.111	7.891	22605856	68008052	11.778m	11.797m
Target Compounds							
2)	A alpha-BHC	4.018	3.270	276.7E6	949.2E6	166.297	111.039 #
3)	MA gamma-BHC...	4.291f	3.593	75578.0E6	16576.3E6	45751.659m	2113.001m#
4)	MA Heptachlor	4.943	3.933	71436145	292.8E6	38.888m	37.761m
5)	MB Aldrin	5.288	4.214	79883654	768.3E6	43.263	97.608 #
6)	B beta-BHC	4.546	3.896	35543307	223.2E6	47.556m	62.462m#
7)	B delta-BHC	4.799	4.124	358.0E6	1109.9E6	178.527	130.285 #
8)	B Heptachlo...	5.715	4.715	69056632	379.1E6	37.359	52.263 #
9)	A Endosulfan I	6.102	5.093	85436504	615.7E6	49.443	95.258 #
10)	B trans-Chl...	5.977	4.965	229.9E6	226.4E6	129.564	31.964 #
11)	B cis-Chlor...	6.051	5.028	98734251	271.8E6	54.112	37.600 #
12)	B 4,4'-DDE	6.223	5.215	197.5E6	598.7E6	107.398	87.143
13)	MA Dieldrin	6.378	5.349	221.1E6	934.4E6	118.718	131.863
14)	MA Endrin	6.608	5.622	154.2E6	443.6E6	96.716	72.736m
15)	B Endosulfa...	6.829	5.916	158.8E6	554.7E6	90.399	92.392
16)	A 4,4'-DDD	6.741	5.768	137.3E6	451.7E6	104.708	86.327m
17)	MA 4,4'-DDT	7.057	6.019	140.5E6	436.1E6	99.168	83.497m
18)	B Endrin al...	6.959	6.095	145.2E6	392.1E6	115.793	88.618m
19)	B Endosulfa...	7.194	6.318	172.4E6	492.1E6	105.996	85.731
20)	A Methoxychlor	7.533	6.594	377.6E6	878.1E6	449.271	340.386
21)	B Endrin ke...	7.681	6.824	191.2E6	546.4E6	106.136	87.748

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080724\
Data File : PD084270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Aug 2024 18:21
Operator : AR\AJ
Sample : P3439-03MSD
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 07 14:26:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072424CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jul 25 11:17:53 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

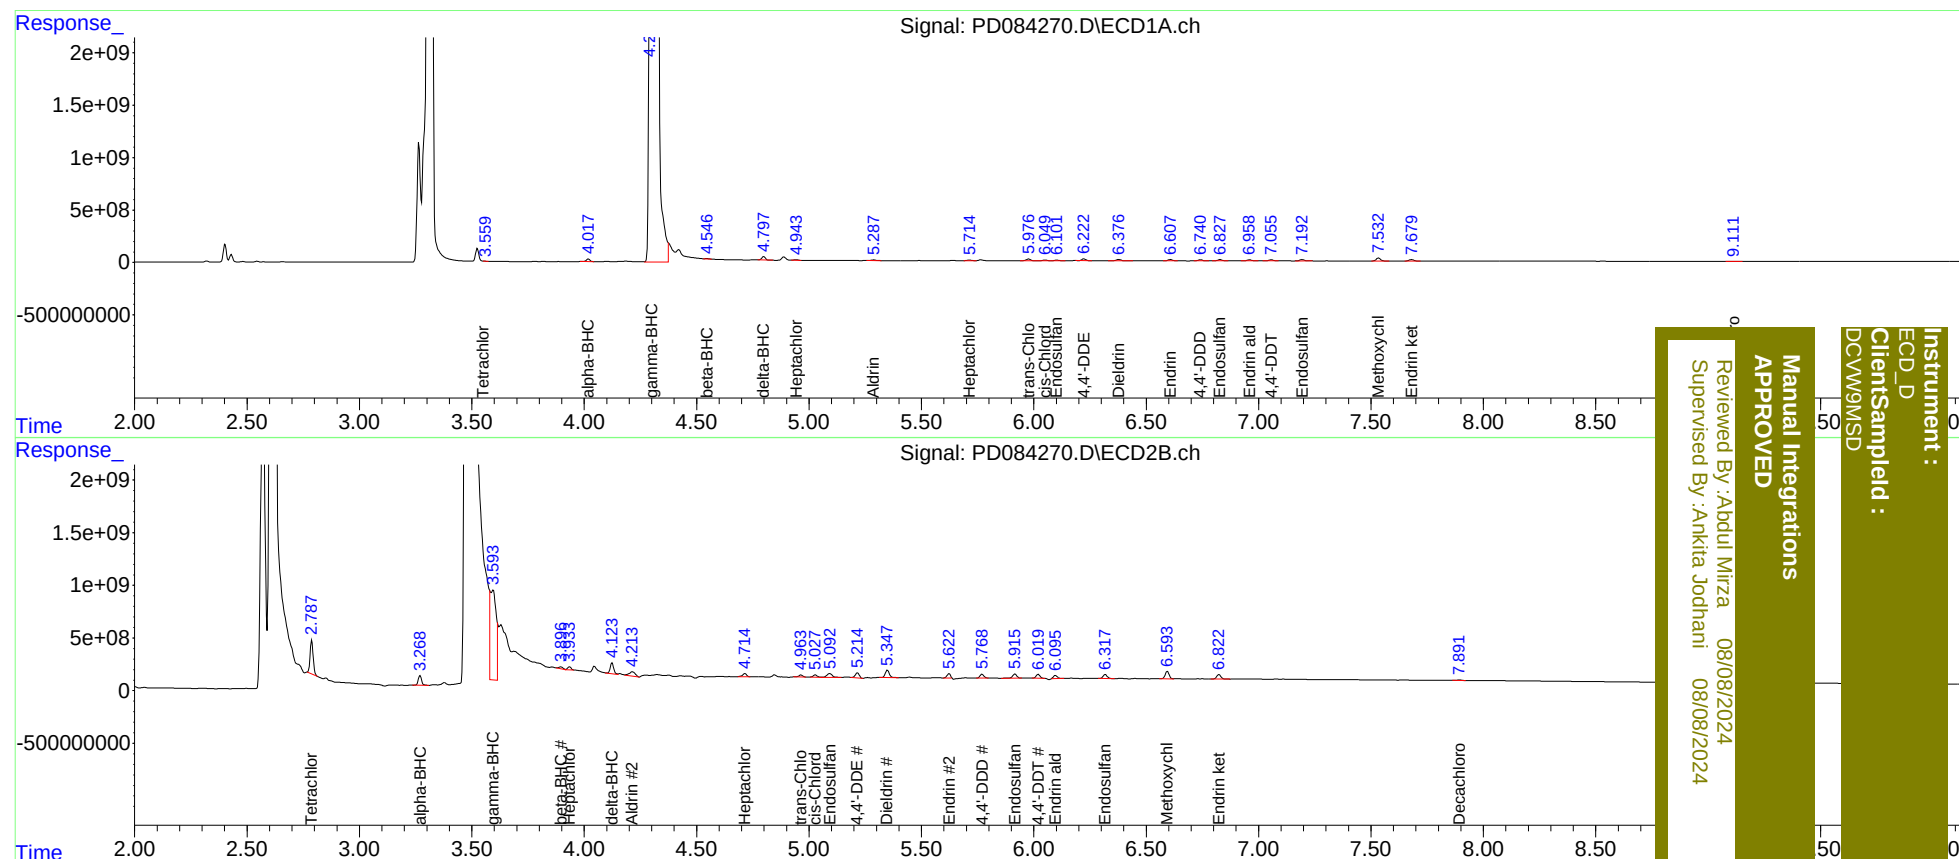

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/08/2024
Supervised By: Ankita Jodhani 08/08/2024

Instrument :
ECD_D
Client Sampled :
DCW/MSD