

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
 Data File : PD071389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 11:09
 Operator : AR\AJ
 Sample : N4023-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP3-1-6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/09/2022
 Supervised By :Ankita Jodhani 08/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 08 11:50:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.814	3.574	36637385	478.7E6	12.919m	17.005 #
28) SA Decachlor...	8.014	9.102	50819563	224.2E6	18.323	21.659

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
Data File : PD071389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 11:09
Operator : AR\AJ
Sample : N4023-08
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP3-1-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/09/2022
Supervised By :Ankita Jodhani 08/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 08 11:50:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

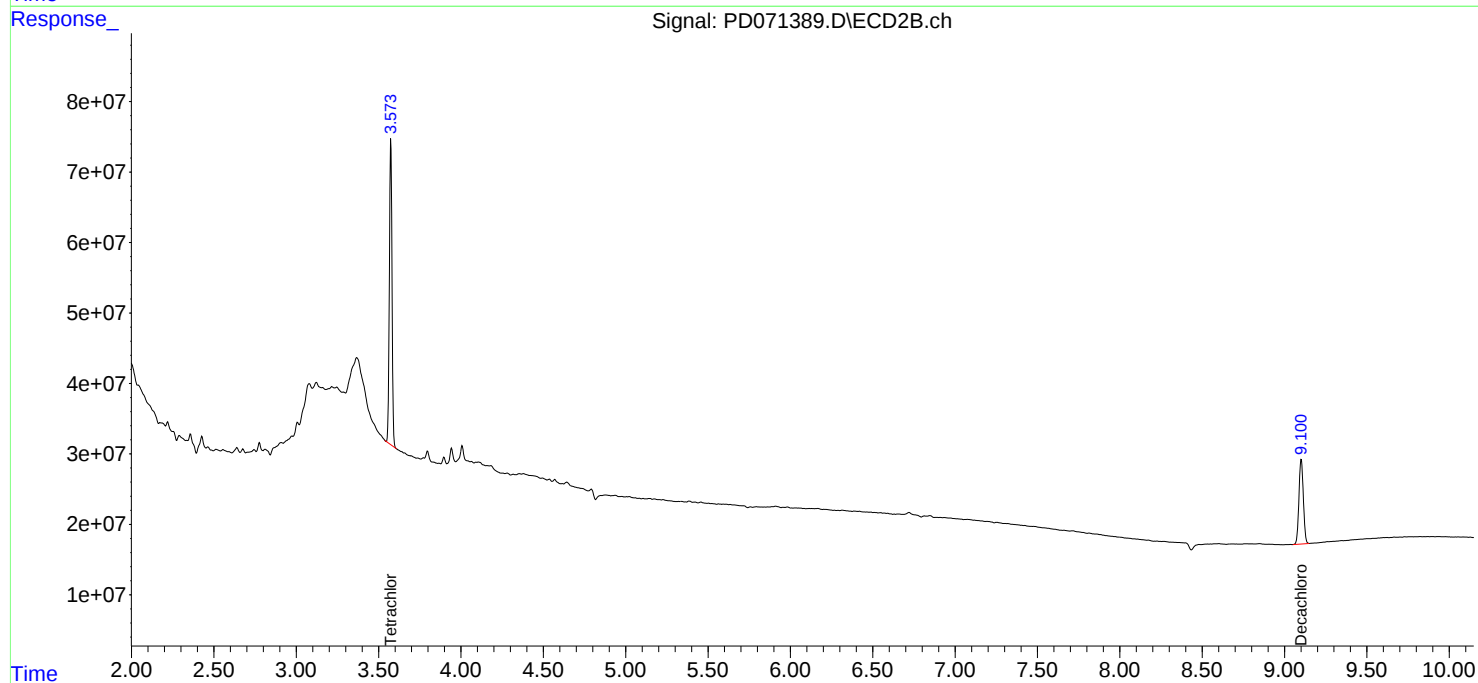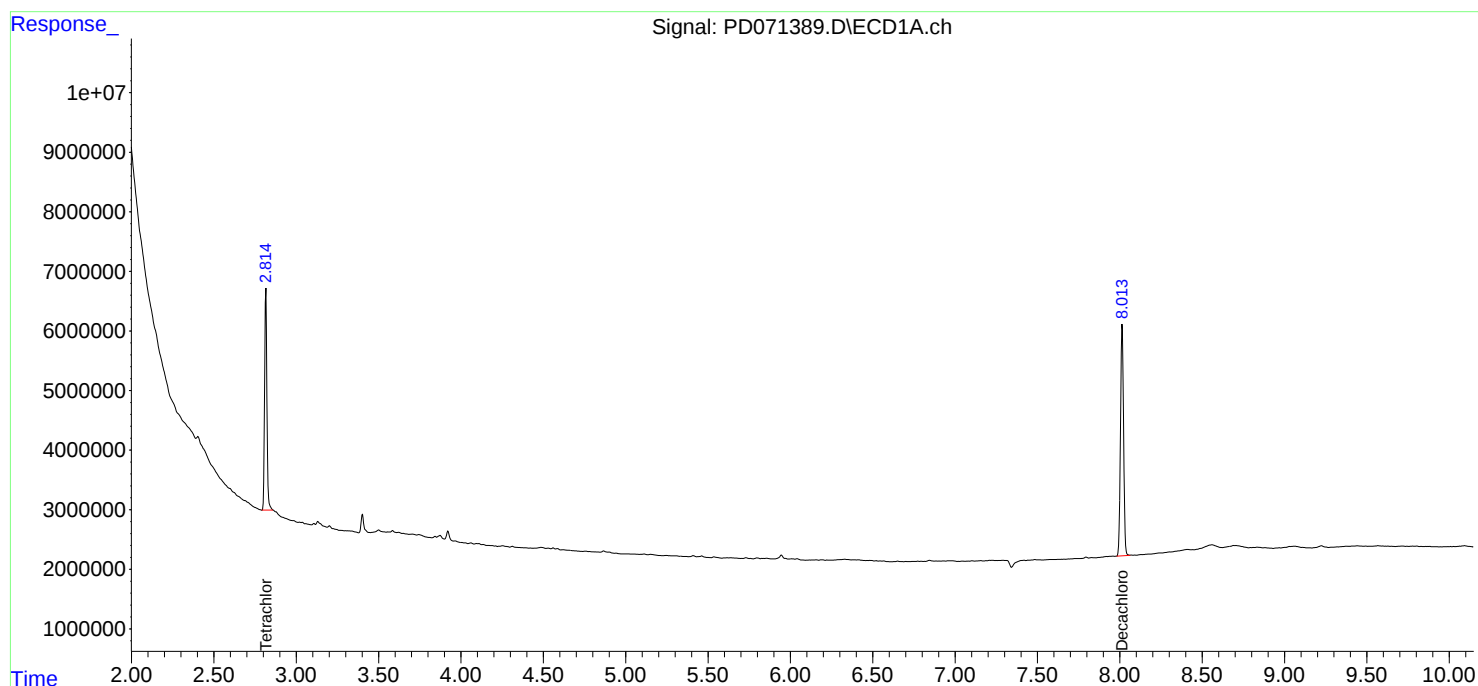

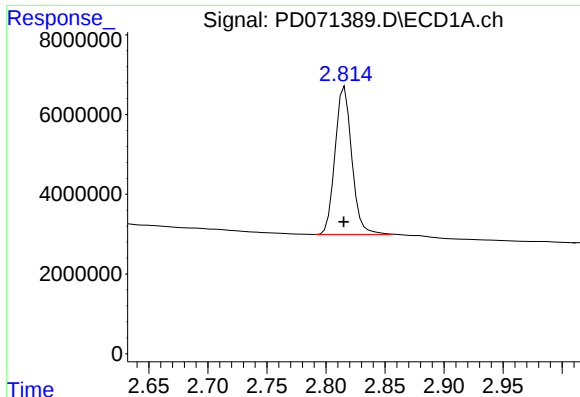


#1 Tetrachloro-m-xylene

R.T.: 2.814 min
Delta R.T.: 0.000 min
Response: 36637385
Conc: 12.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP3-1-6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/09/2022
Supervised By :Ankita Jodhani 08/09/2022

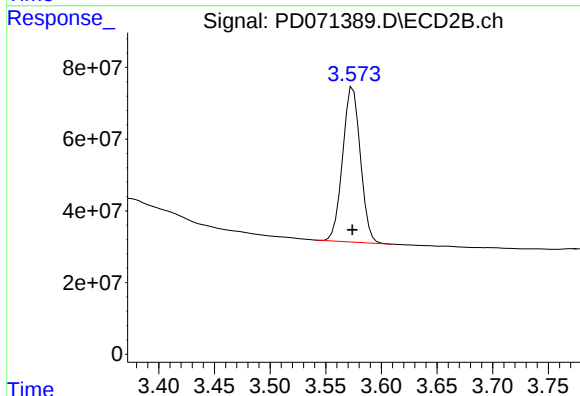


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 478680170
Conc: 17.00 ng/ml

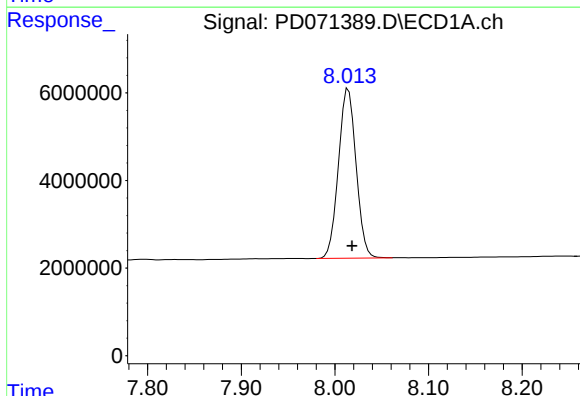

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.004 min
Response: 50819563
Conc: 18.32 ng/ml

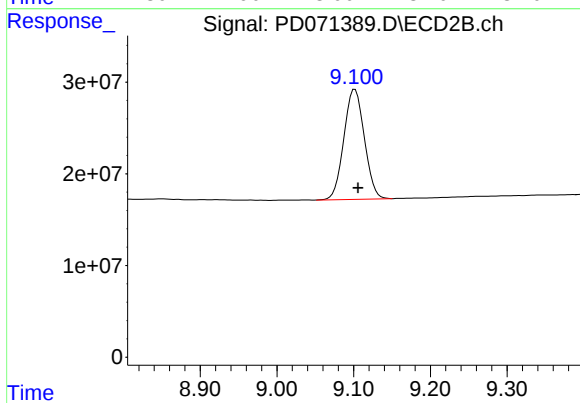

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.004 min
Response: 224230070
Conc: 21.66 ng/ml