

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
 Data File : PD071407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 15:12
 Operator : AR\AJ
 Sample : N4046-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BEACONPOINT-BACKFILL-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 01:23:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.815	3.574	49085639	574.1E6	17.308	20.394
28)	SA Decachlor...	8.016	9.106	47248305	208.3E6	17.036	20.118

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
Data File : PD071407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 15:12
Operator : AR\AJ
Sample : N4046-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BEACONPOINT-BACKFILL-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 01:23:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

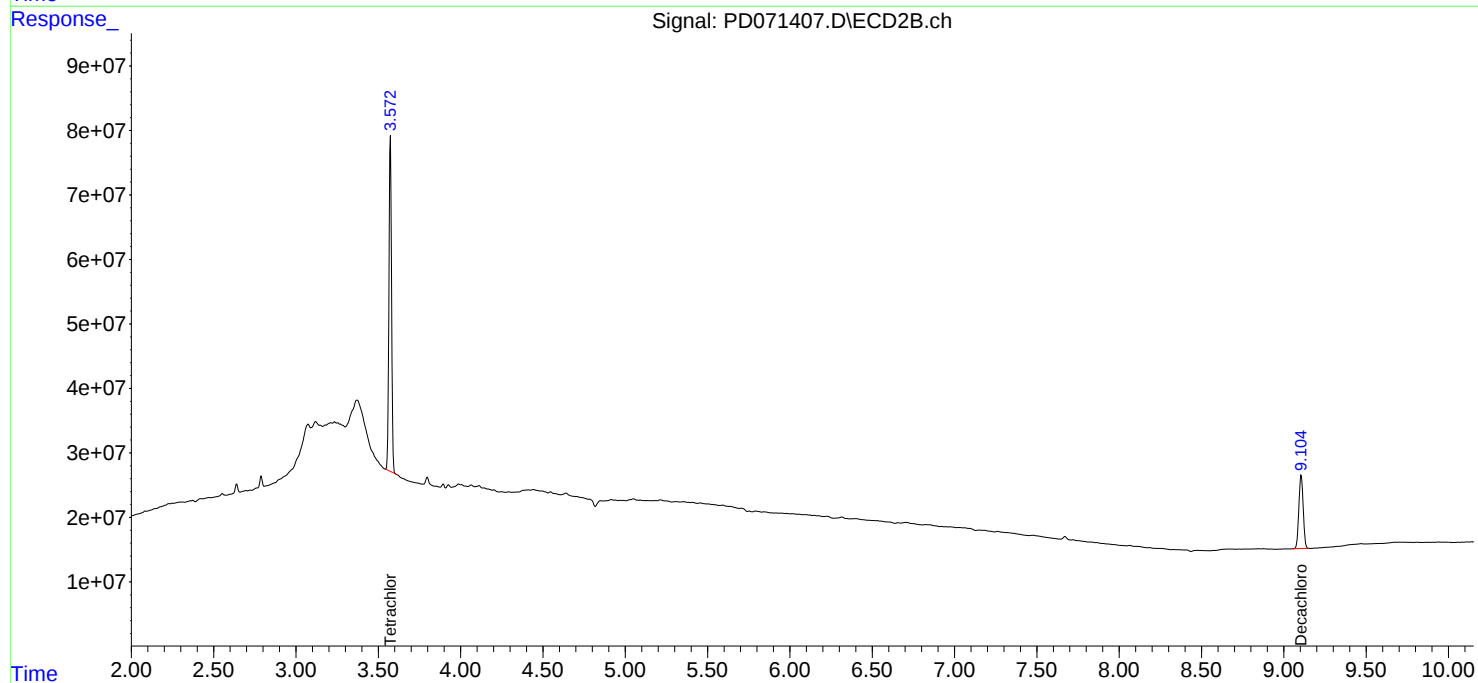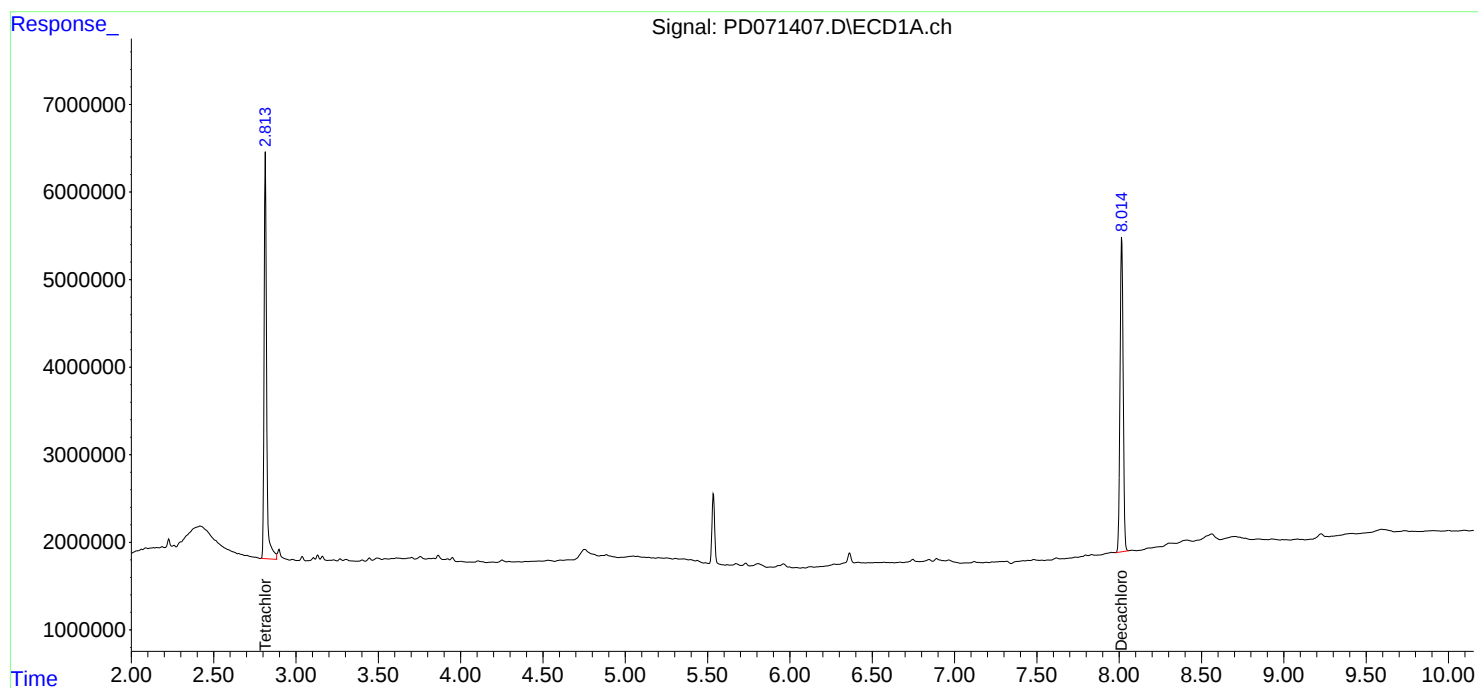


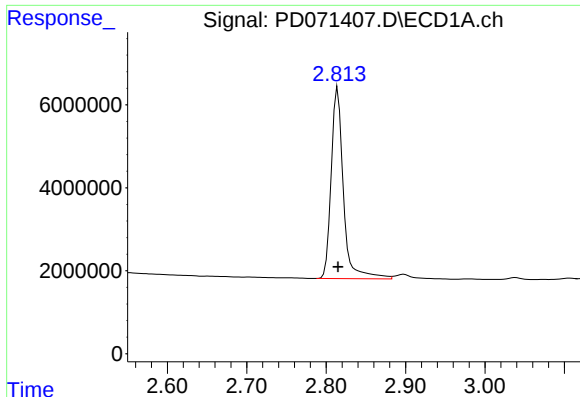

#1 Tetrachloro-m-xylene


R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 49085639
Conc: 17.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEACONPOINT-BACKFILL-01

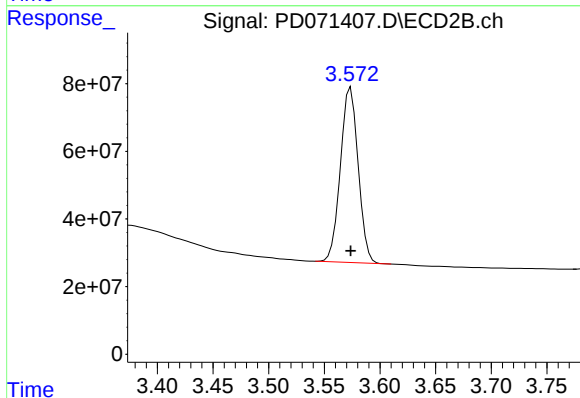


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 574082632
Conc: 20.39 ng/ml

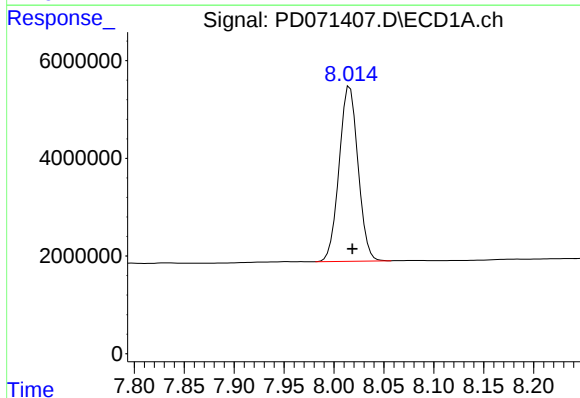

#28 Decachlorobiphenyl

R.T.: 8.016 min
Delta R.T.: -0.003 min
Response: 47248305
Conc: 17.04 ng/ml

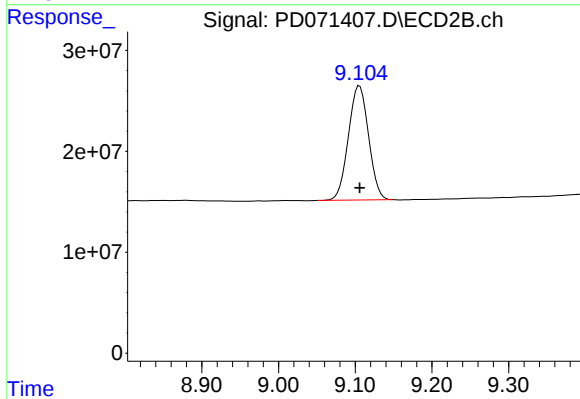

#28 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: 0.000 min
Response: 208272037
Conc: 20.12 ng/ml