

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
 Data File : PD071443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2022 23:59
 Operator : AR\AJ
 Sample : N4046-21
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BEACONPOINT-BACKFILL-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 02:40:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.814	3.573	51775225	602.7E6	18.257	21.409
28)	SA Decachlor...	8.013	9.102	48182051	197.9E6	17.372	19.112

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080822\
Data File : PD071443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2022 23:59
Operator : AR\AJ
Sample : N4046-21
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
BEACONPOINT-BACKFILL-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 02:40:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

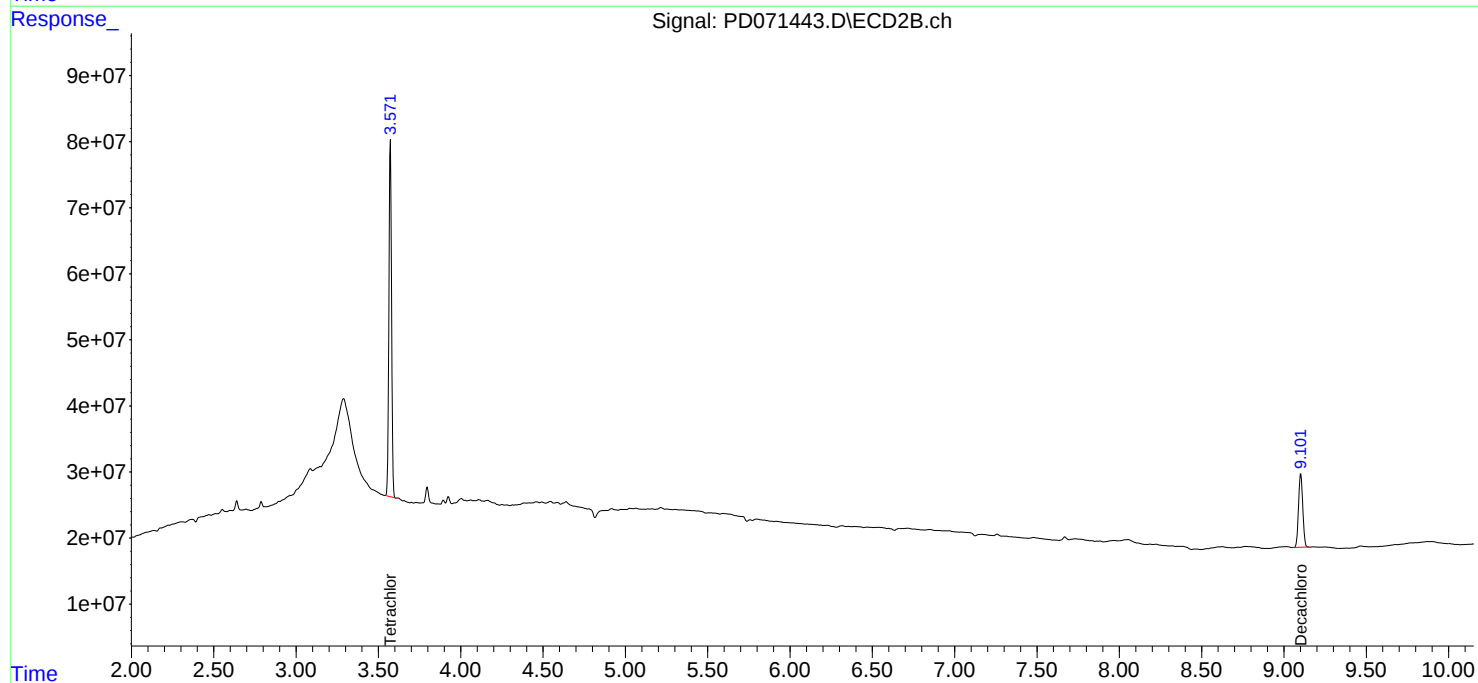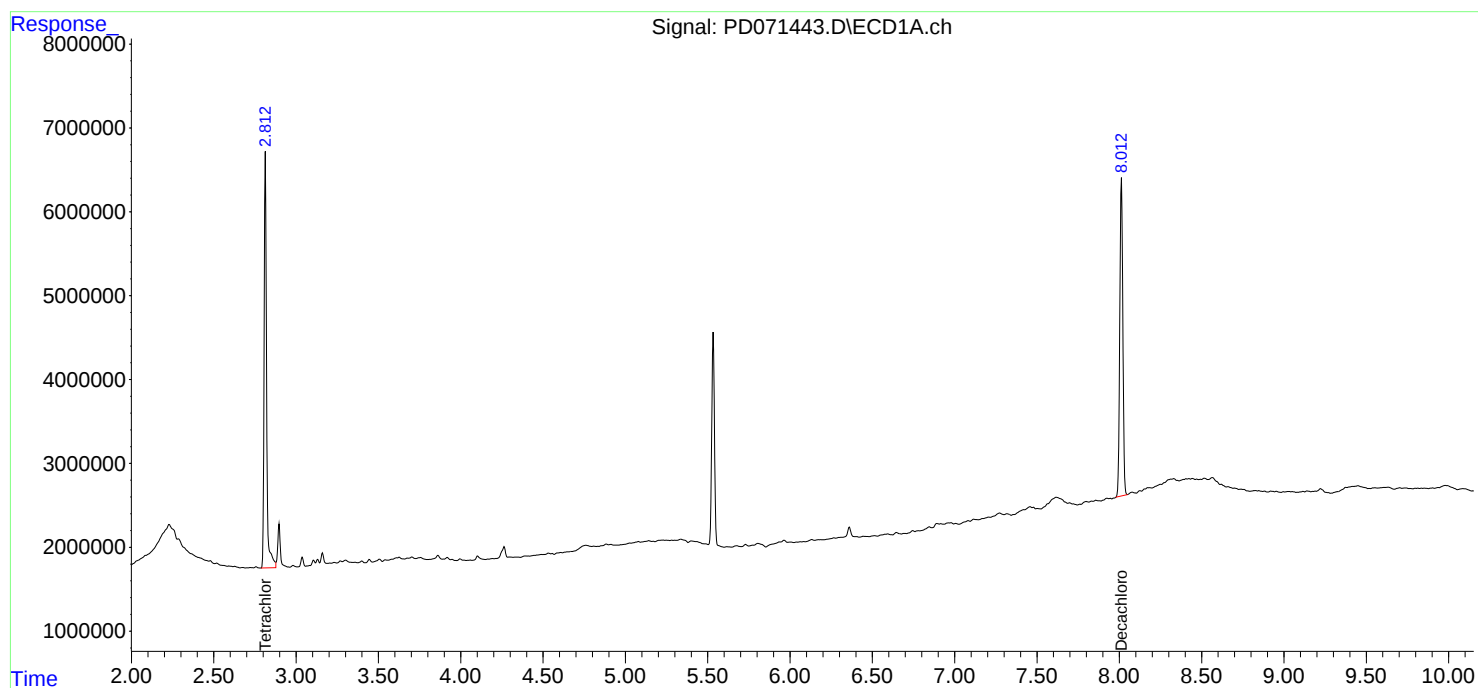


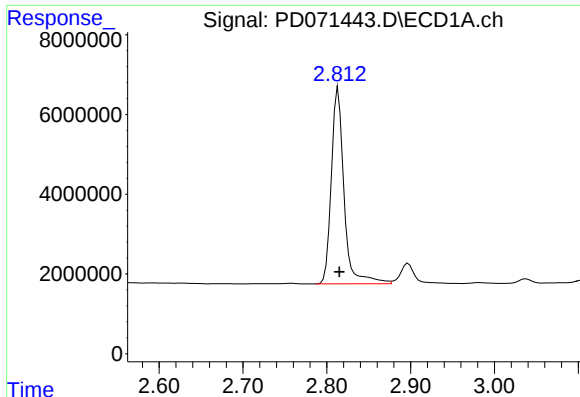

#1 Tetrachloro-m-xylene


R.T.: 2.814 min
Delta R.T.: -0.001 min
Response: 51775225
Conc: 18.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
BEACONPOINT-BACKFILL-11

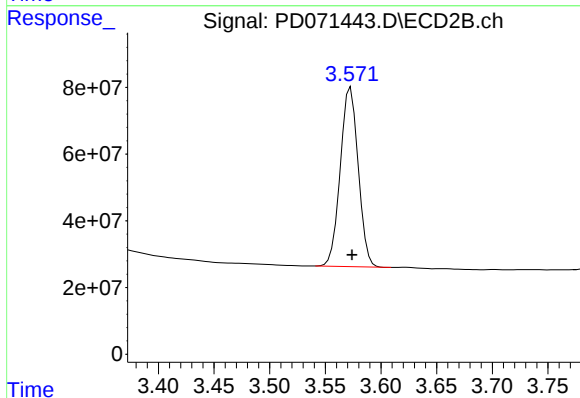


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: -0.001 min
Response: 602662783
Conc: 21.41 ng/ml

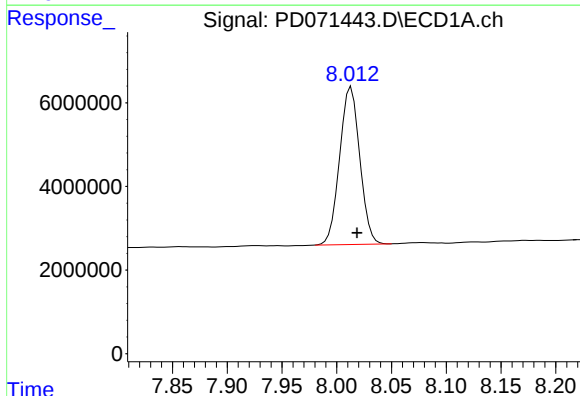

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: -0.005 min
Response: 48182051
Conc: 17.37 ng/ml

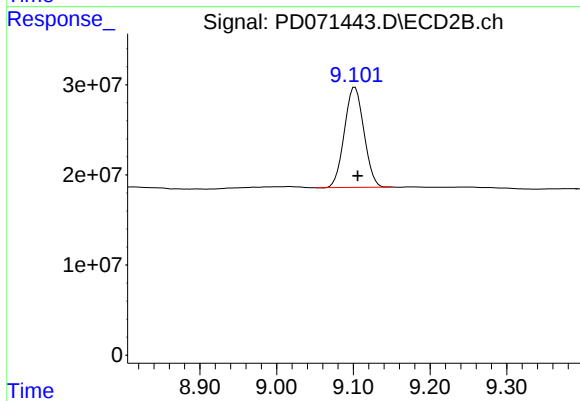

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.004 min
Response: 197862603
Conc: 19.11 ng/ml