

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080823\
 Data File : PD077017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2023 09:01
 Operator : AR\AJ
 Sample : PIBLK225
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 09 00:00:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 14:58:34 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.763	36899319	20488867	17.345	19.195
27)	SA Decachlor...	9.092	7.907	101.4E6	49849389	41.740	46.502
Target Compounds							
3)	MA gamma-BHC...	0.000	3.631f	0	245356	N.D.	0.164
4)	MA Heptachlor	0.000	3.899f	0	248236	N.D.	0.166
5)	MB Aldrin	0.000	4.222	0	379866	N.D.	0.252
6)	B beta-BHC	0.000	3.899	0	248236	N.D.	0.347
7)	B delta-BHC	4.776	0.000	5157562	0	1.538	N.D. #
8)	B Heptachlo...	0.000	4.740	0	245063	N.D.	0.174
10)	B trans-Chl...	5.990	0.000	1558049	0	0.507	N.D. #
11)	B cis-Chlor...	5.990f	0.000	1558049	0	0.491	N.D. #
15)	B Endosulfa...	0.000	5.881f	0	329087	N.D.	0.274
18)	B Endrin al...	0.000	6.115	0	256354	N.D.	0.306


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080823\
Data File : PD077017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2023 09:01
Operator : AR\AJ
Sample : PIBLK225
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 09 00:00:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071423CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 14:58:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

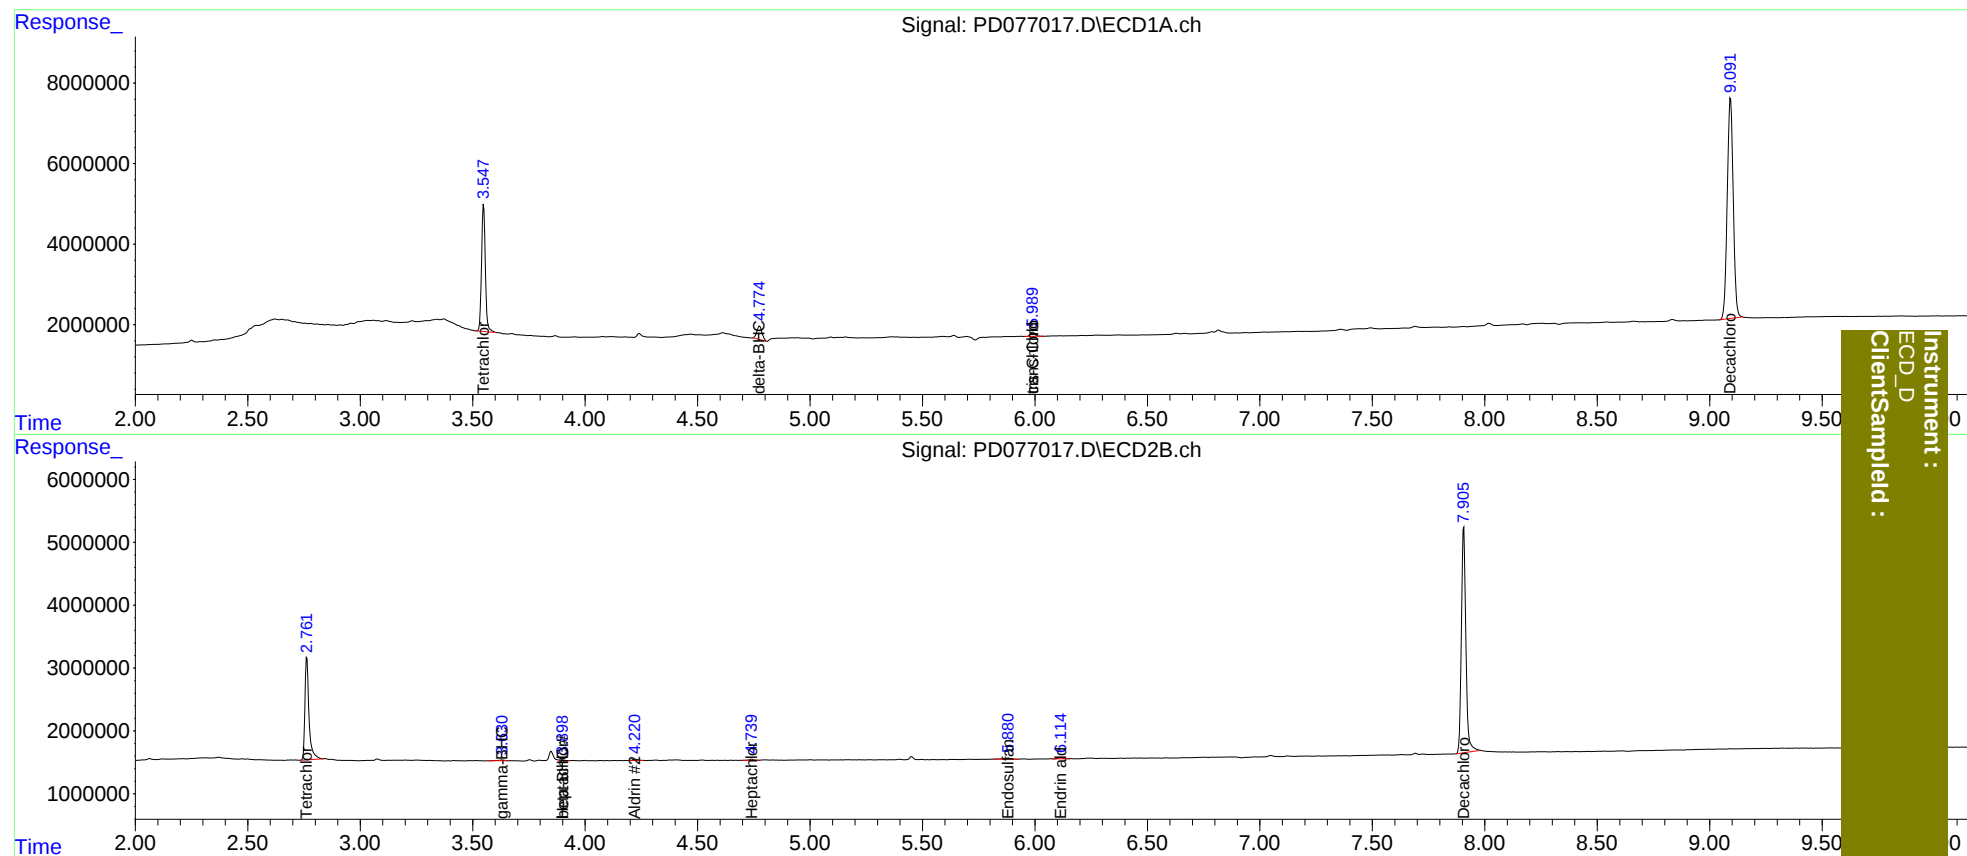


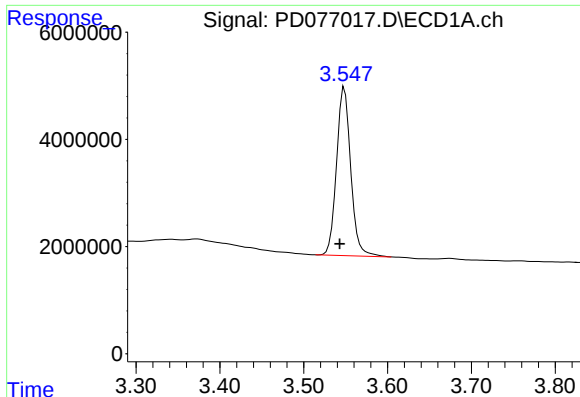

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.006 min
Response: 36899319
Conc: 17.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

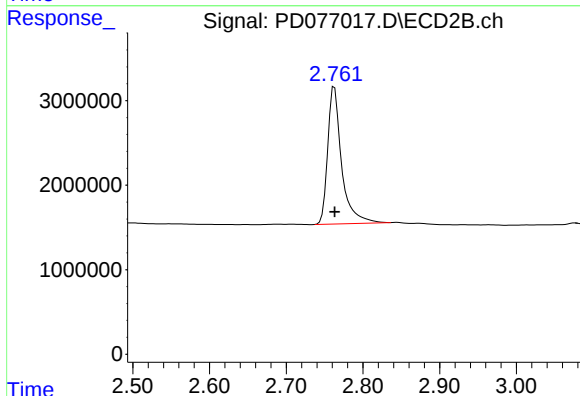


#1 Tetrachloro-m-xylene

R.T.: 2.763 min
Delta R.T.: 0.000 min
Response: 20488867
Conc: 19.19 ng/ml

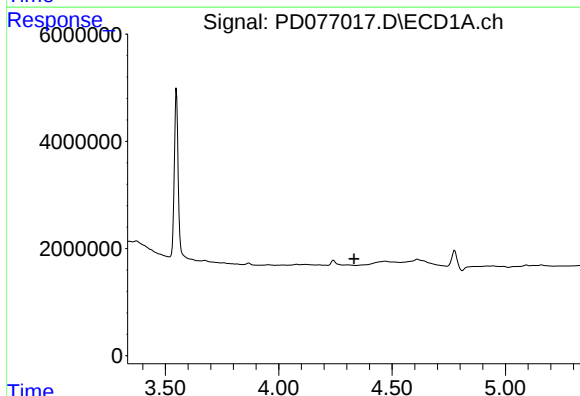


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.333 min
Response: 0
Conc: N.D.

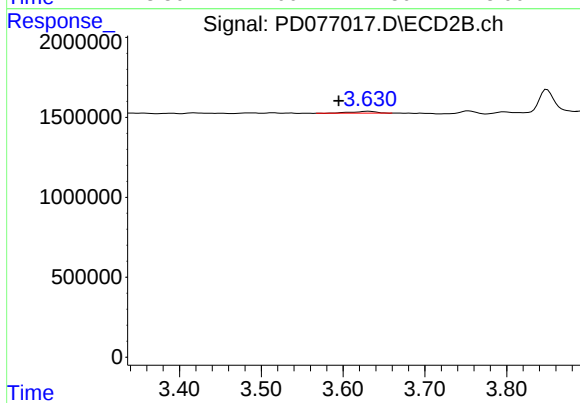

#3 gamma-BHC (Lindane)


R.T.: 3.631 min
Delta R.T.: 0.036 min
Response: 245356
Conc: 0.16 ng/ml

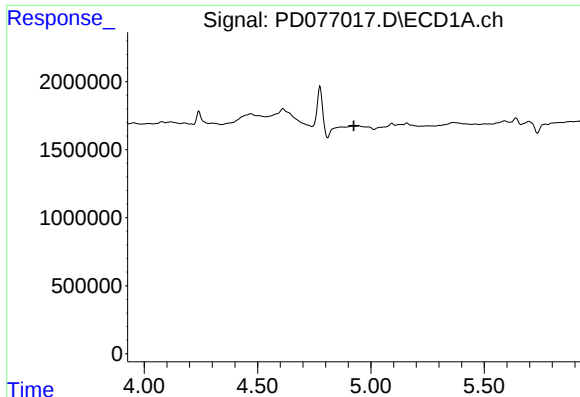

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.924 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

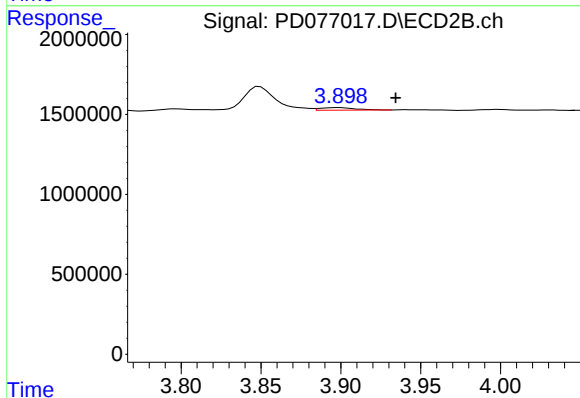


#4 Heptachlor

R.T.: 3.899 min
Delta R.T.: -0.035 min
Response: 248236
Conc: 0.17 ng/ml

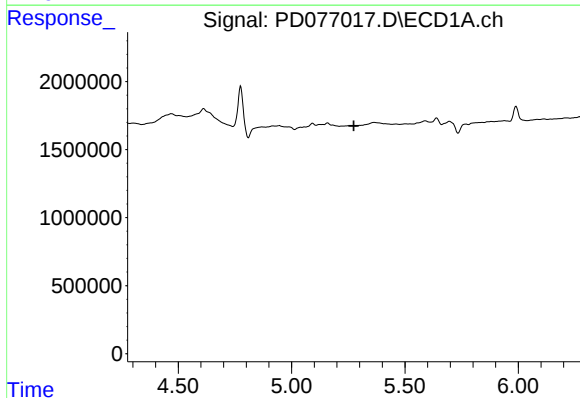


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

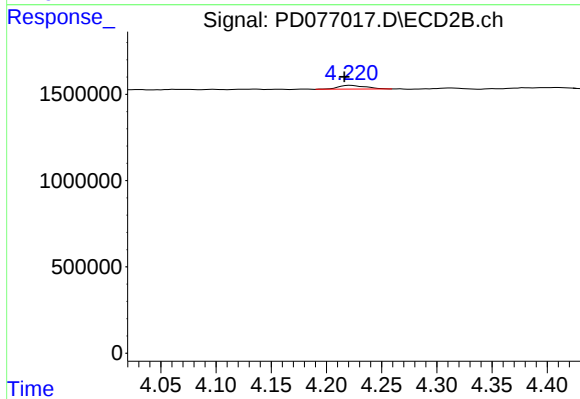

#5 Aldrin


R.T.: 4.222 min
Delta R.T.: 0.005 min
Response: 379866
Conc: 0.25 ng/ml

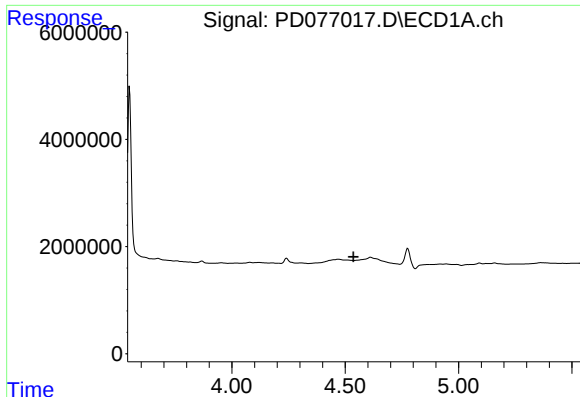

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

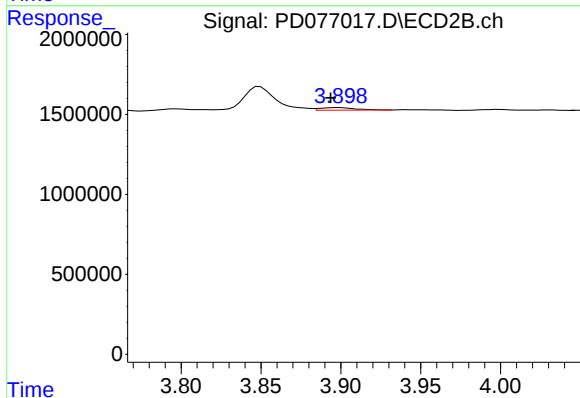


#6 beta-BHC

R.T.: 3.899 min
Delta R.T.: 0.006 min
Response: 248236
Conc: 0.35 ng/ml

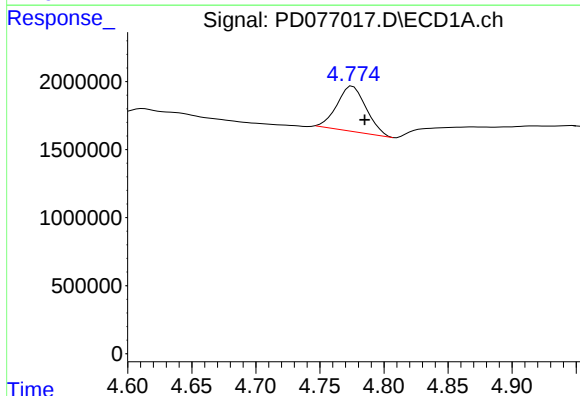


#7 delta-BHC

R.T.: 4.776 min
Delta R.T.: -0.009 min
Response: 5157562
Conc: 1.54 ng/ml

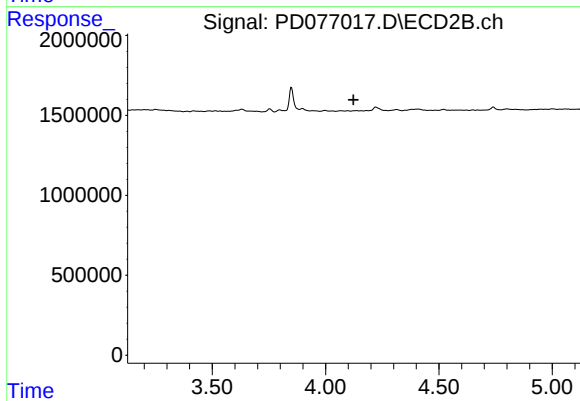

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.123 min
Response: 0
Conc: N.D.

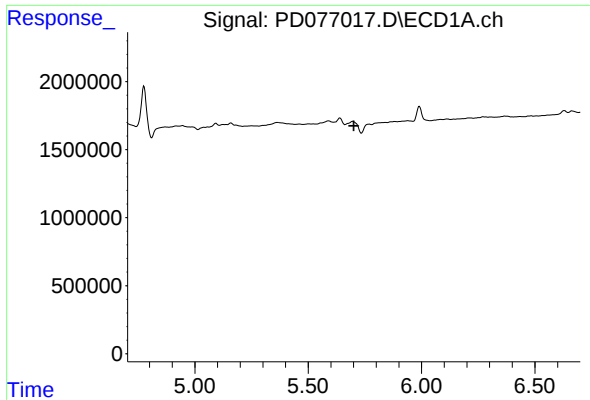

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

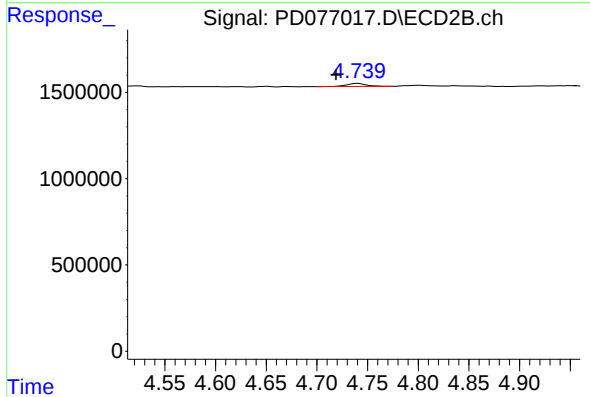


#8 Heptachlor epoxide

R.T.: 4.740 min
Delta R.T.: 0.021 min
Response: 245063
Conc: 0.17 ng/ml

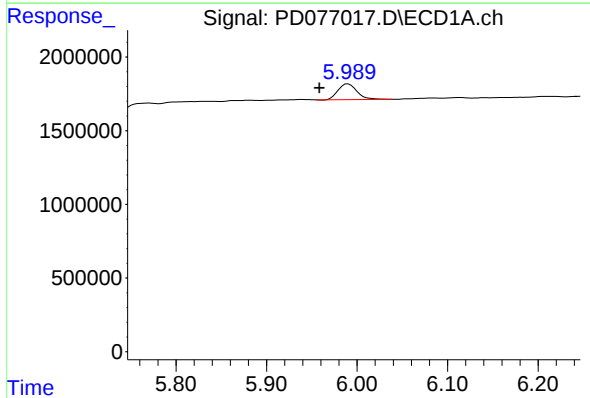


#10 trans-Chlordane

R.T.: 5.990 min
Delta R.T.: 0.032 min
Response: 1558049
Conc: 0.51 ng/ml

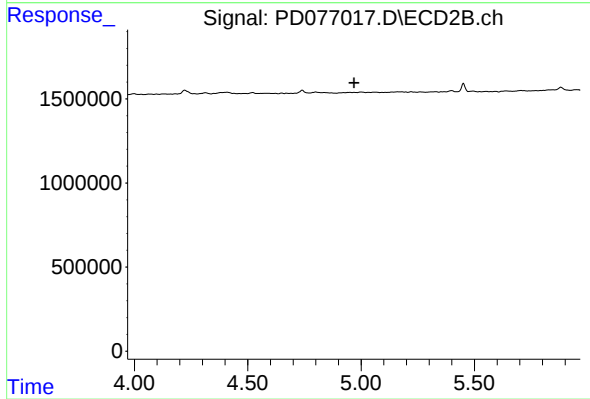

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.969 min
Response: 0
Conc: N.D.

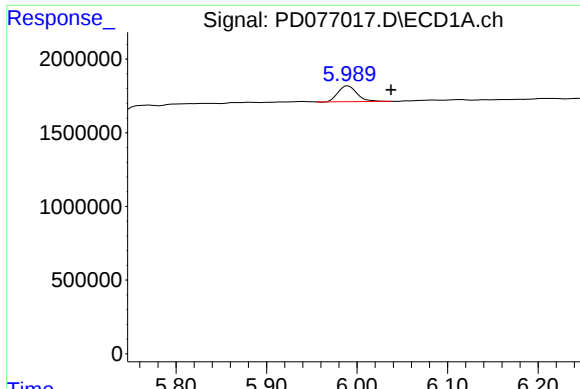

#11 cis-Chlordane


R.T.: 5.990 min
Delta R.T.: -0.048 min
Response: 1558049
Conc: 0.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

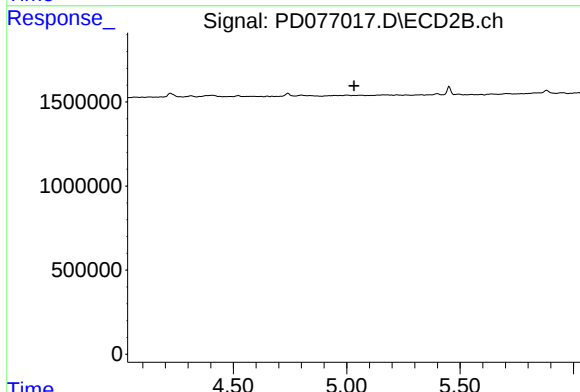


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.033 min
Response: 0
Conc: N.D.

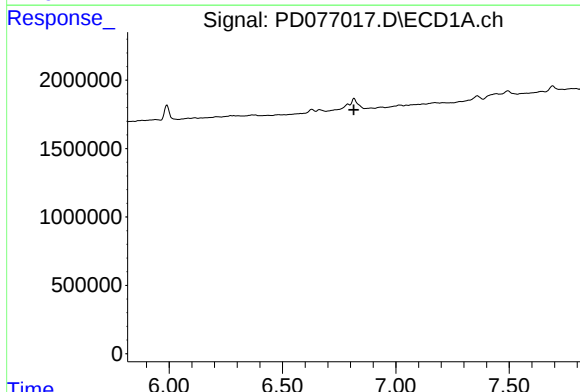


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

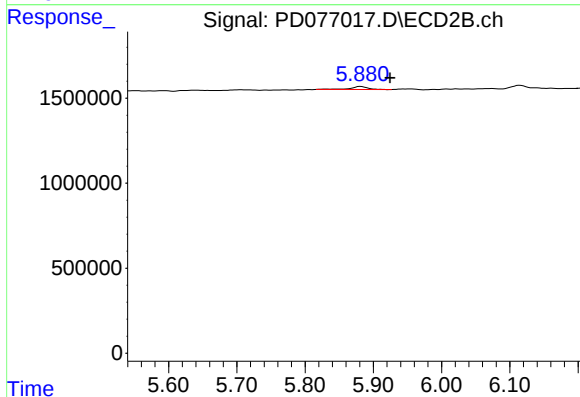

#15 Endosulfan II


R.T.: 5.881 min
Delta R.T.: -0.043 min
Response: 329087
Conc: 0.27 ng/ml

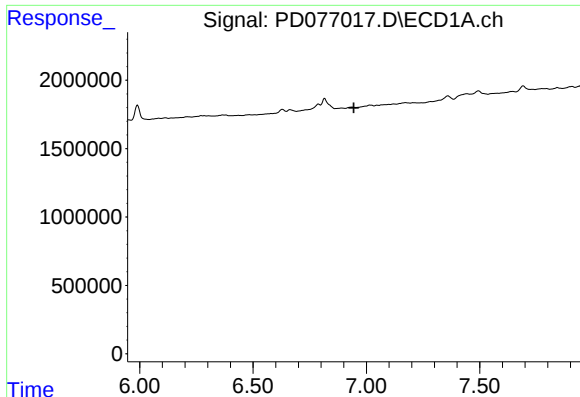

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.945 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

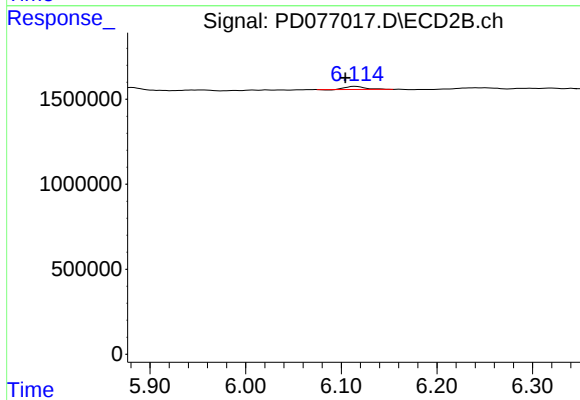


#18 Endrin aldehyde

R.T.: 6.115 min
Delta R.T.: 0.011 min
Response: 256354
Conc: 0.31 ng/ml

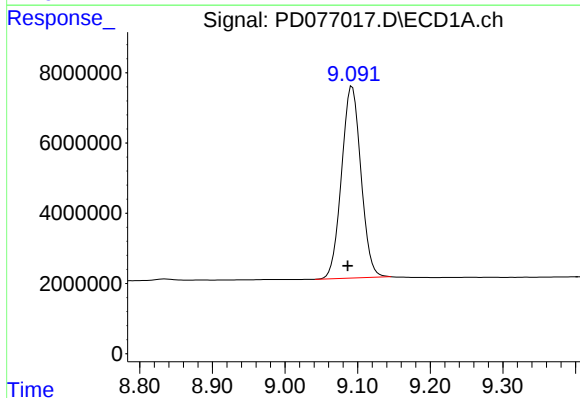

#27 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.006 min
Response: 101405661
Conc: 41.74 ng/ml

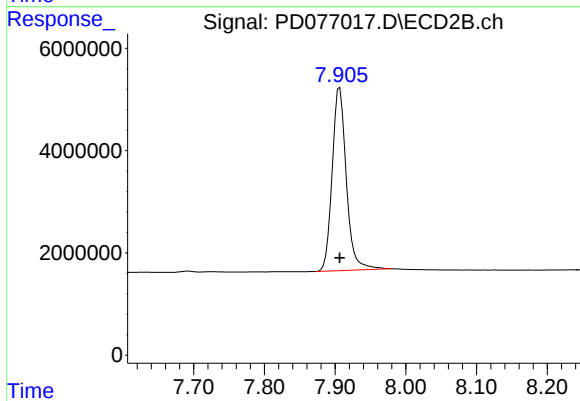

#27 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: 0.000 min
Response: 49849389
Conc: 46.50 ng/ml