

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080919\
 Data File : PD054214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2019 12:22
 Operator : SM\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:20:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 05:49:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:33:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	33925250	43408837	58.945	49.831
28)	SA Decachlor...	8.007	9.026	33218691	45356620	49.346	48.926
Target Compounds							
2)	A alpha-BHC	3.742	4.370	51783998	64216104	59.790	50.907
3)	MA gamma-BHC...	4.019	4.653	48320352	61161564	58.906	49.866
4)	MA Heptachlor	4.307	5.160	43507869	62287084	59.704	49.722
5)	MB Aldrin	4.548	5.465	46429013	61228559	58.425	49.797
6)	B beta-BHC	4.268	4.819	20456383	27788268	58.078	49.631
7)	B delta-BHC	4.466	5.036	49728878	64054067	59.312	49.486
8)	B Heptachlor...	4.986	5.848	43400363	59489904	57.209	49.195
9)	A Endosulfan I	5.318	6.203	41340991	56921161	55.643	49.017
10)	B gamma-Chl...	5.209	6.081	45463095	63520009	55.893	48.221
11)	B alpha-Chl...	5.266	6.153	44911601	62791206	55.437	48.360
12)	B 4,4'-DDE	5.435	6.309	41531857	59691925	52.413	48.581
13)	MA Dieldrin	5.559	6.459	45024813	62441902	55.441	49.693
14)	MA Endrin	5.813	6.676	41305587	52250676	55.156	49.852
15)	B Endosulfa...	6.086	6.883	40343656	56851856	53.918	49.165
16)	A 4,4'-DDD	5.947	6.796	30651685	48005640	51.215	47.517
17)	MA 4,4'-DDT	6.183	7.094	30269550	48798737	52.561	49.535
18)	B Endrin al...	6.255	7.006	33166349	48099581	52.216	48.364
19)	B Endosulfa...	6.467	7.228	36408795	52569049	51.794	48.377
20)	A Methoxychlor	6.731	7.550	13776587	24925639	48.208m	46.455
21)	B Endrin ke...	6.951	7.697	42769459	59798426	53.367m	49.182
22)	Mirex	7.129	8.153	33581165	44798769	51.619	48.605

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080919\
Data File : PD054214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2019 12:22
Operator : SM\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_D
Client Sampled :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 05:49:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:33:23 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

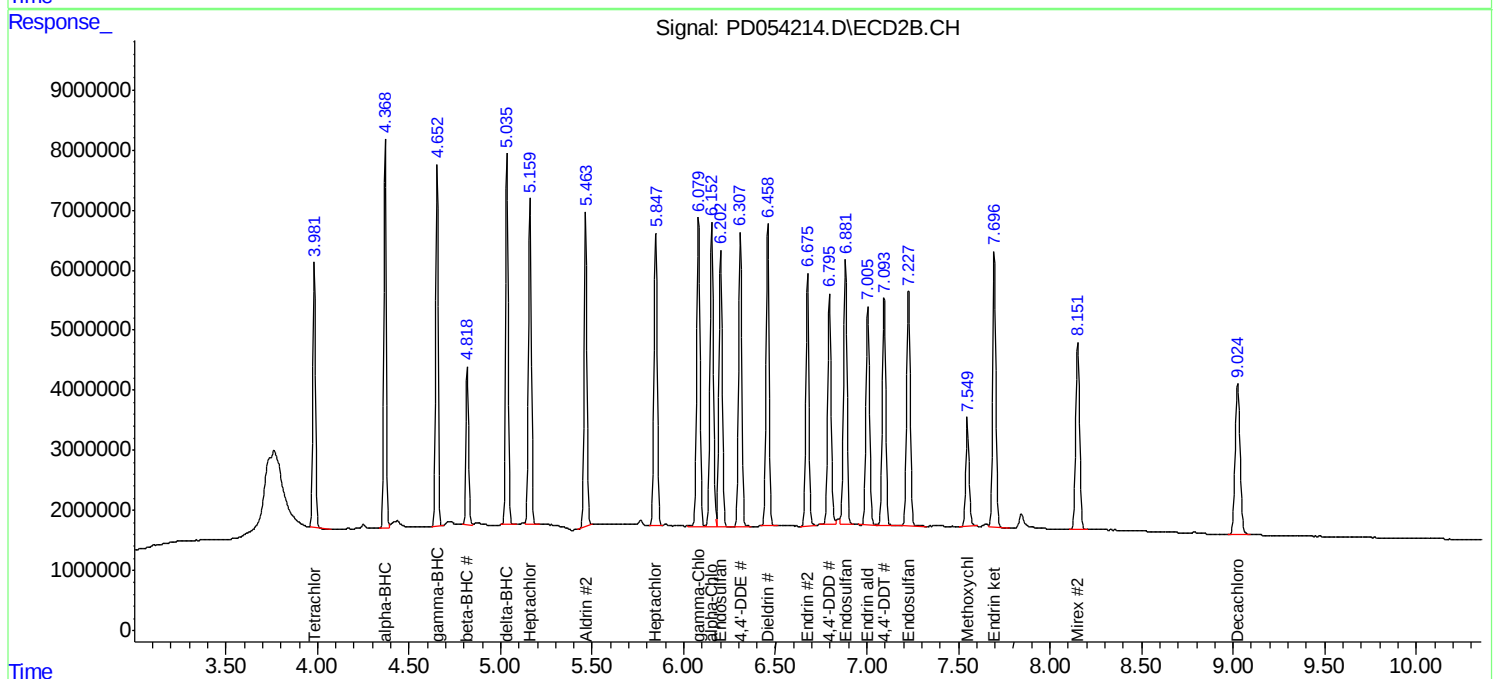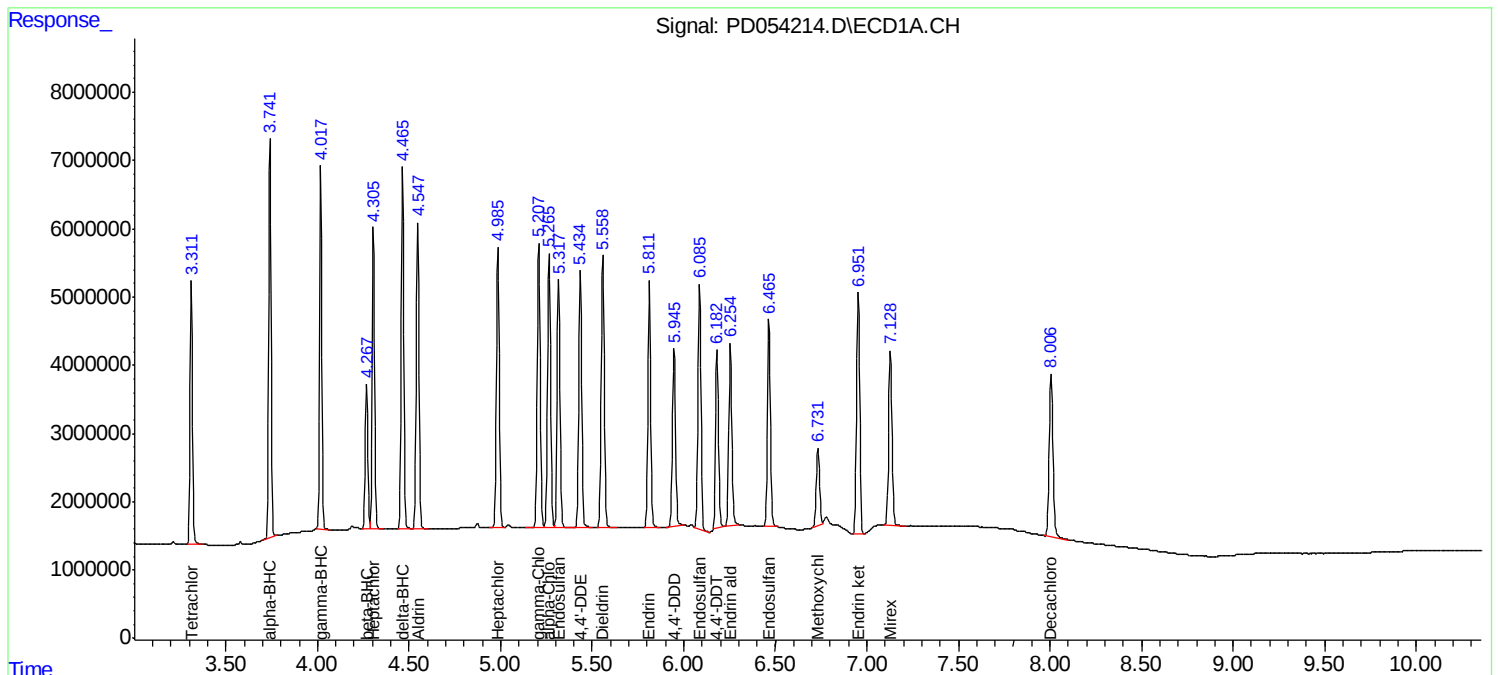

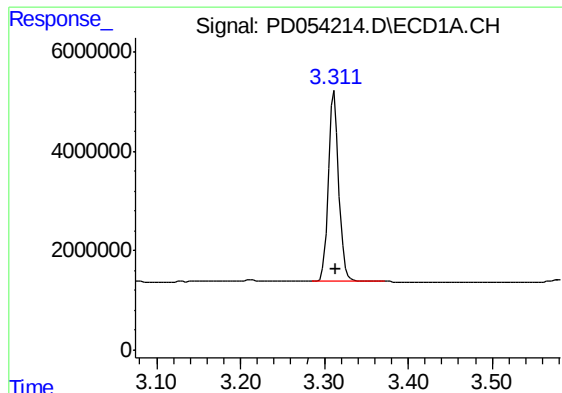


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 33925250
Conc: 58.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM

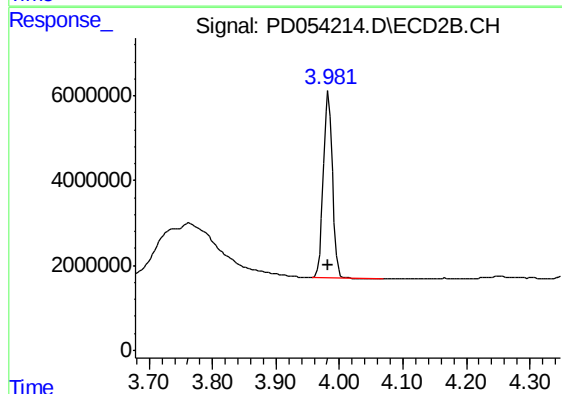


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 43408837
Conc: 49.83 ng/ml




#2 alpha-BHC

R.T.: 3.742 min
Delta R.T.: 0.000 min
Response: 51783998
Conc: 59.79 ng/ml

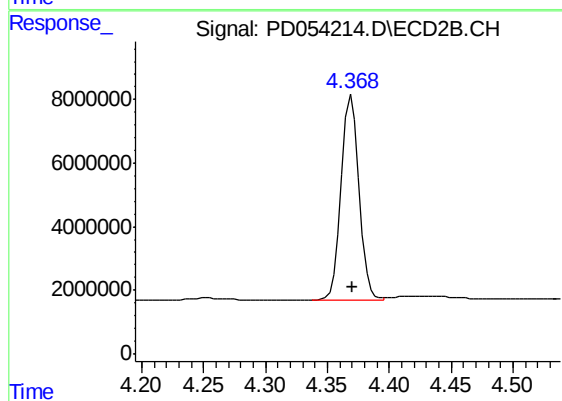

#2 alpha-BHC

R.T.: 4.370 min
Delta R.T.: 0.000 min
Response: 64216104
Conc: 50.91 ng/ml




#3 gamma-BHC (Lindane)

R.T.: 4.019 min
Delta R.T.: 0.000 min
Response: 48320352
Conc: 58.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#3 gamma-BHC (Lindane)

R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 61161564
Conc: 49.87 ng/ml

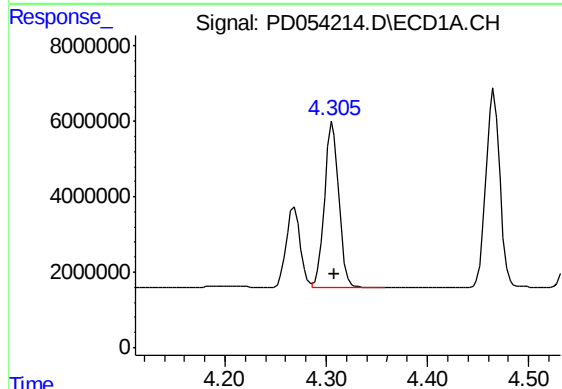


#4 Heptachlor

R.T.: 4.307 min
Delta R.T.: 0.000 min
Response: 43507869
Conc: 59.70 ng/ml

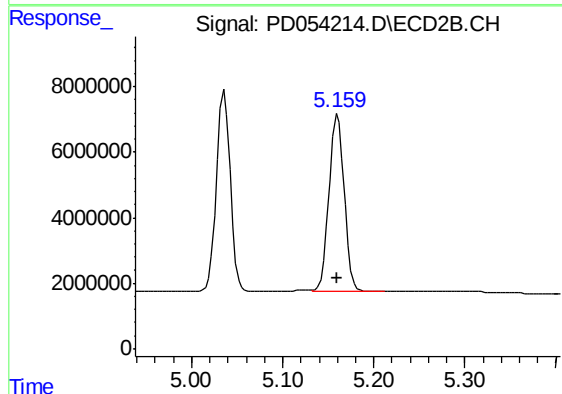

#4 Heptachlor

R.T.: 5.160 min
Delta R.T.: 0.000 min
Response: 62287084
Conc: 49.72 ng/ml




#5 Aldrin

R.T.: 4.548 min
Delta R.T.: 0.000 min
Response: 46429013
Conc: 58.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#5 Aldrin

R.T.: 5.465 min
Delta R.T.: 0.000 min
Response: 61228559
Conc: 49.80 ng/ml

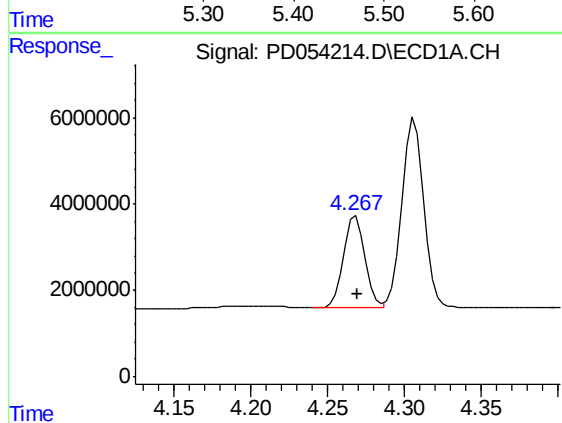


#6 beta-BHC

R.T.: 4.268 min
Delta R.T.: 0.000 min
Response: 20456383
Conc: 58.08 ng/ml

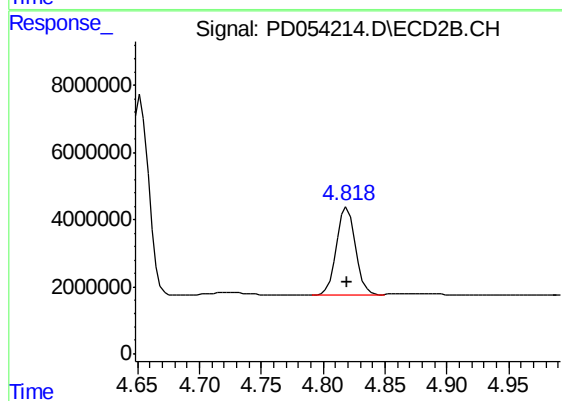

#6 beta-BHC

R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 27788268
Conc: 49.63 ng/ml




#7 delta-BHC

R.T.: 4.466 min
Delta R.T.: 0.000 min
Response: 49728878
Conc: 59.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#7 delta-BHC

R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 64054067
Conc: 49.49 ng/ml




#8 Heptachlor epoxide

R.T.: 4.986 min
Delta R.T.: 0.000 min
Response: 43400363
Conc: 57.21 ng/ml

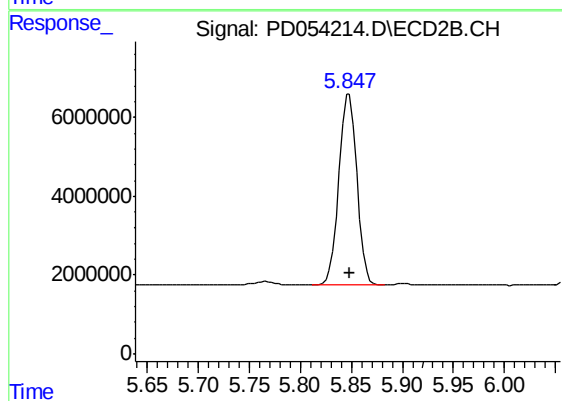

#8 Heptachlor epoxide

R.T.: 5.848 min
Delta R.T.: 0.000 min
Response: 59489904
Conc: 49.20 ng/ml




#9 Endosulfan I

R.T.: 5.318 min
Delta R.T.: -0.001 min
Response: 41340991
Conc: 55.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#9 Endosulfan I

R.T.: 6.203 min
Delta R.T.: 0.000 min
Response: 56921161
Conc: 49.02 ng/ml




#10 gamma-Chlordane

R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 45463095
Conc: 55.89 ng/ml

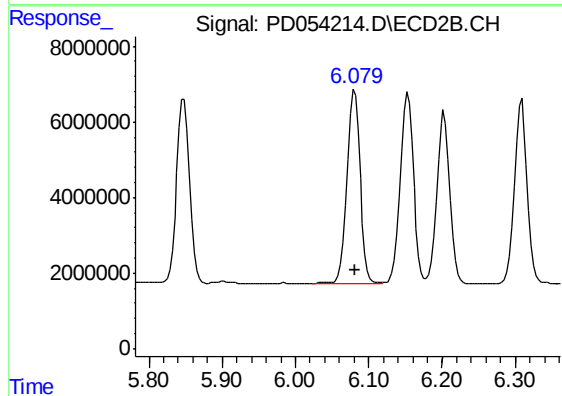

#10 gamma-Chlordane

R.T.: 6.081 min
Delta R.T.: 0.000 min
Response: 63520009
Conc: 48.22 ng/ml




#11 alpha-Chlordane

R.T.: 5.266 min
Delta R.T.: 0.000 min
Response: 44911601
Conc: 55.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#11 alpha-Chlordane

R.T.: 6.153 min
Delta R.T.: 0.000 min
Response: 62791206
Conc: 48.36 ng/ml




#12 4,4'-DDE

R.T.: 5.435 min
Delta R.T.: -0.001 min
Response: 41531857
Conc: 52.41 ng/ml

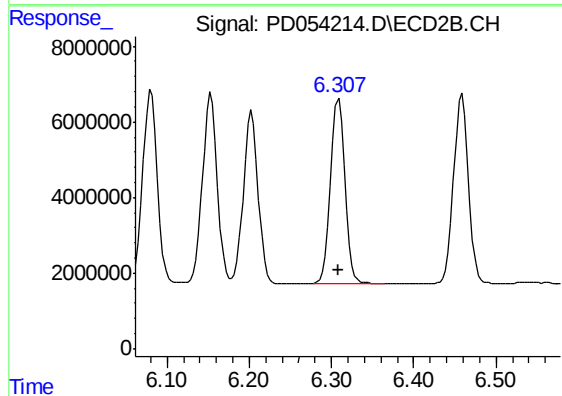

#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 59691925
Conc: 48.58 ng/ml




#13 Dieldrin

R.T.: 5.559 min
Delta R.T.: 0.000 min
Response: 45024813
Conc: 55.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#13 Dieldrin

R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 62441902
Conc: 49.69 ng/ml




#14 Endrin

R.T.: 5.813 min
Delta R.T.: 0.000 min
Response: 41305587
Conc: 55.16 ng/ml

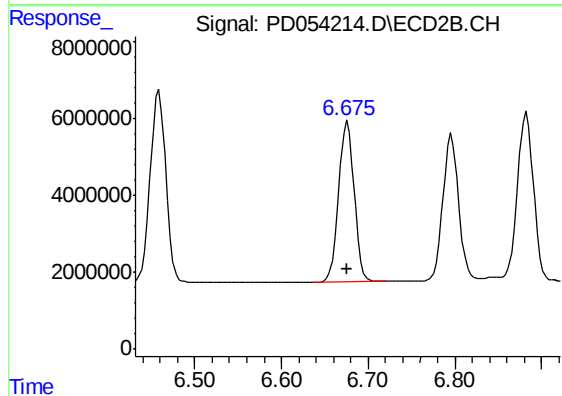

#14 Endrin

R.T.: 6.676 min
Delta R.T.: 0.000 min
Response: 52250676
Conc: 49.85 ng/ml




#15 Endosulfan II

R.T.: 6.086 min
Delta R.T.: -0.002 min
Response: 40343656
Conc: 53.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#15 Endosulfan II

R.T.: 6.883 min
Delta R.T.: 0.000 min
Response: 56851856
Conc: 49.17 ng/ml

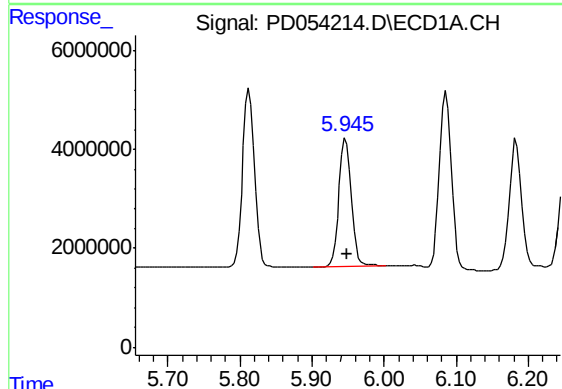


#16 4,4'-DDD

R.T.: 5.947 min
Delta R.T.: -0.001 min
Response: 30651685
Conc: 51.21 ng/ml

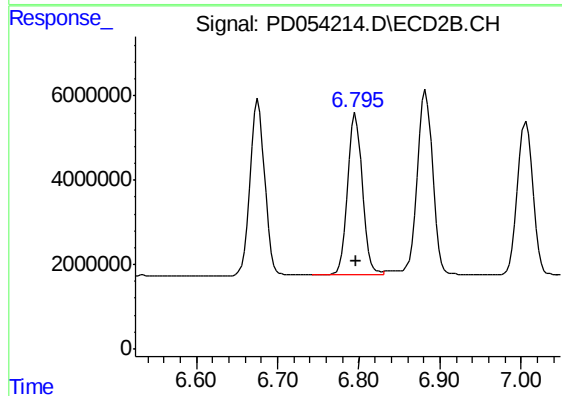

#16 4,4'-DDD

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 48005640
Conc: 47.52 ng/ml

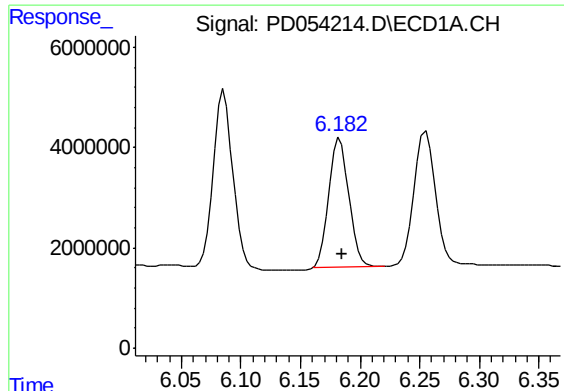


#17 4,4'-DDT

R.T.: 6.183 min
Delta R.T.: -0.001 min
Response: 30269550
Conc: 52.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM

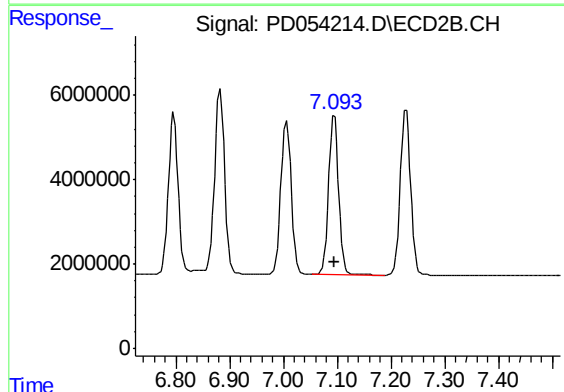


#17 4,4'-DDT

R.T.: 7.094 min
Delta R.T.: 0.000 min
Response: 48798737
Conc: 49.53 ng/ml

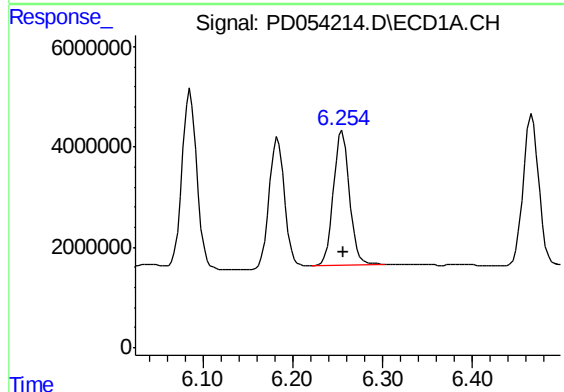


#18 Endrin aldehyde

R.T.: 6.255 min
Delta R.T.: -0.001 min
Response: 33166349
Conc: 52.22 ng/ml

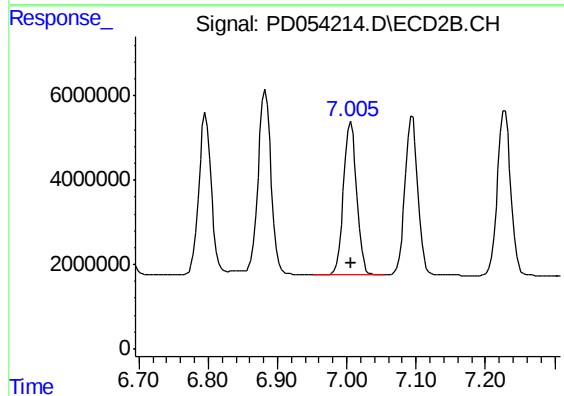

#18 Endrin aldehyde

R.T.: 7.006 min
Delta R.T.: 0.000 min
Response: 48099581
Conc: 48.36 ng/ml




#19 Endosulfan Sulfate

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 36408795
Conc: 51.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM

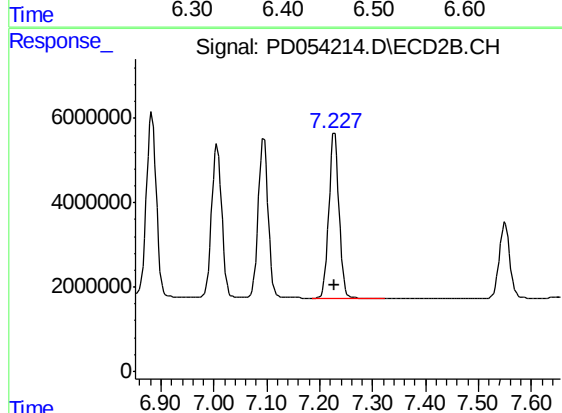


#19 Endosulfan Sulfate

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 52569049
Conc: 48.38 ng/ml

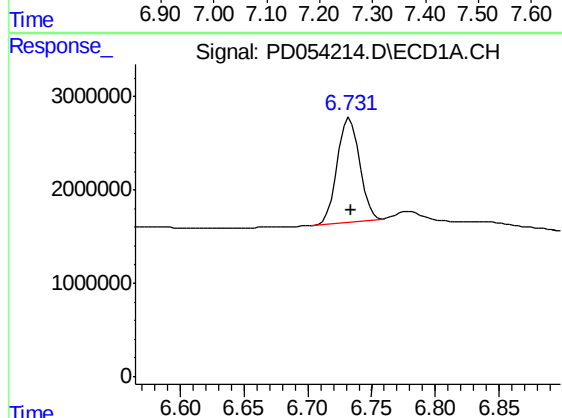


#20 Methoxychlor

R.T.: 6.731 min
Delta R.T.: -0.003 min
Response: 13776587
Conc: 48.21 ng/ml m

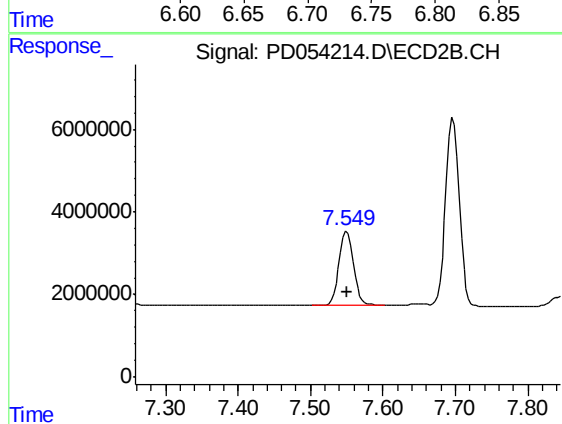

#20 Methoxychlor

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 24925639
Conc: 46.46 ng/ml




#21 Endrin ketone

R.T.: 6.951 min
Delta R.T.: -0.003 min
Response: 42769459
Conc: 53.37 ng/ml m

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM




#21 Endrin ketone

R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 59798426
Conc: 49.18 ng/ml




#22 Mirex

R.T.: 7.129 min
Delta R.T.: 0.000 min
Response: 33581165
Conc: 51.62 ng/ml

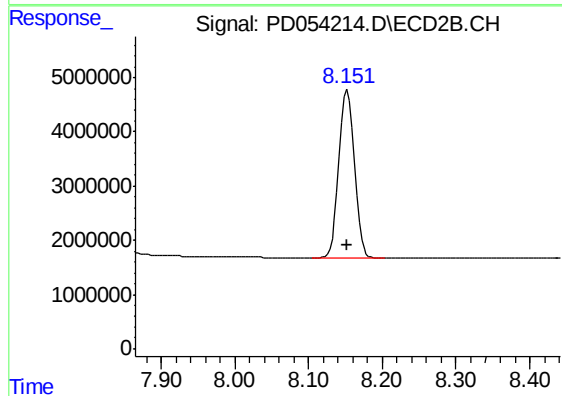

#22 Mirex

R.T.: 8.153 min
Delta R.T.: 0.000 min
Response: 44798769
Conc: 48.61 ng/ml

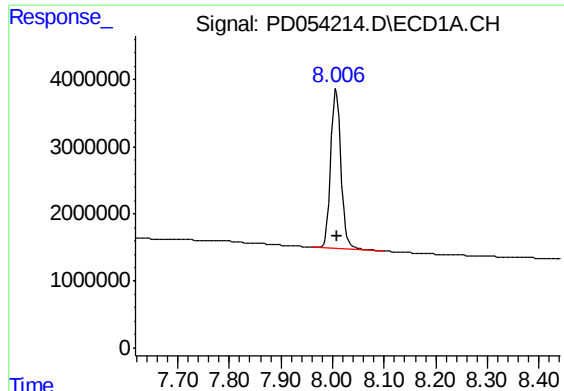


#28 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.002 min
Response: 33218691
Conc: 49.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:26 PM

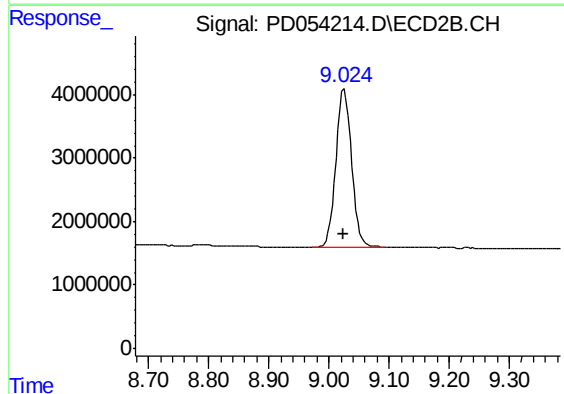

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.000 min
Response: 45356620
Conc: 48.93 ng/ml