

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080919\
 Data File : PD054233.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Aug 2019 17:46
 Operator : SM\AJ
 Sample : K4227-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 1S-J-(0-1)-COMP

Manual Integrations
 APPROVED

Ankita
 8/12/2019 1:20:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 05:53:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:33:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.982	14867344	19579048	25.832	22.476m
28)	SA Decachlor...	8.008	9.026	14825852	20966382	22.024	22.616

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080919\
Data File : PD054233.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Aug 2019 17:46
Operator : SM\AJ
Sample : K4227-04
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
1S-J-(0-1)-COMP


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 05:53:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:33:23 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

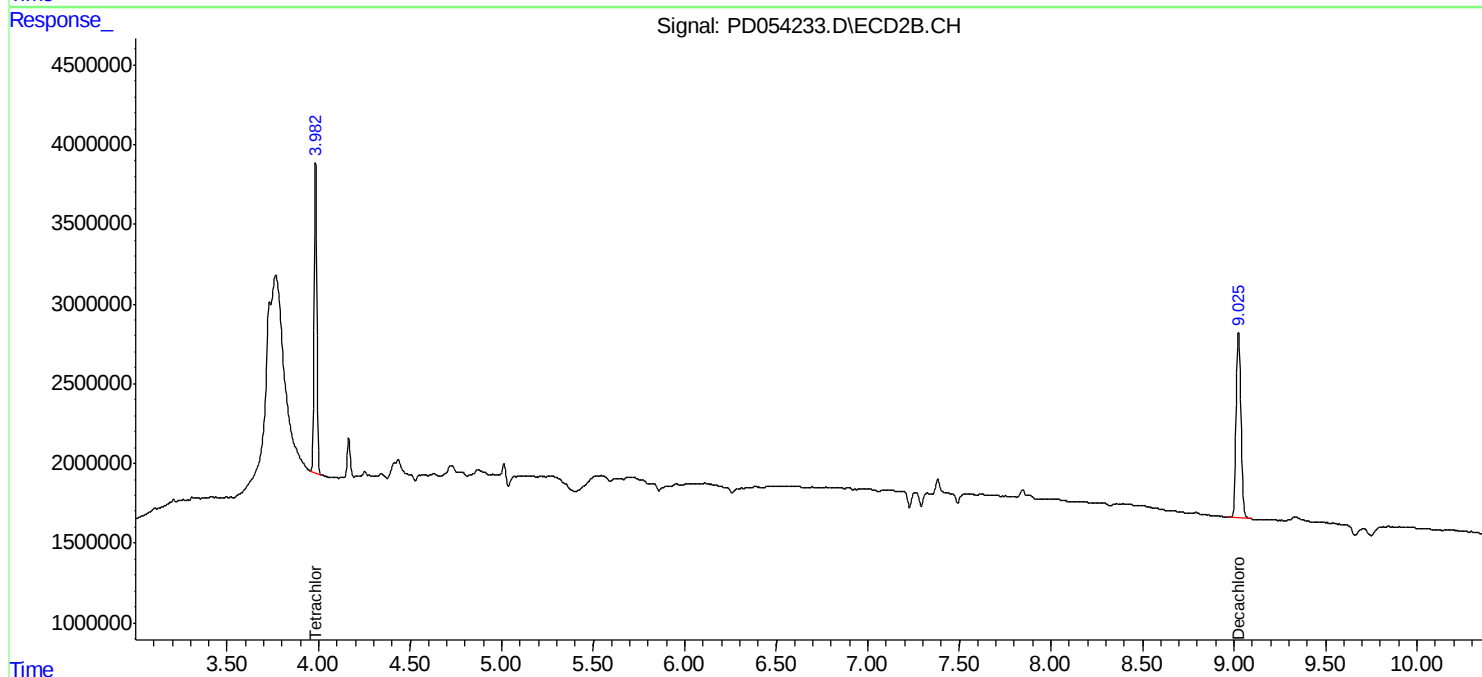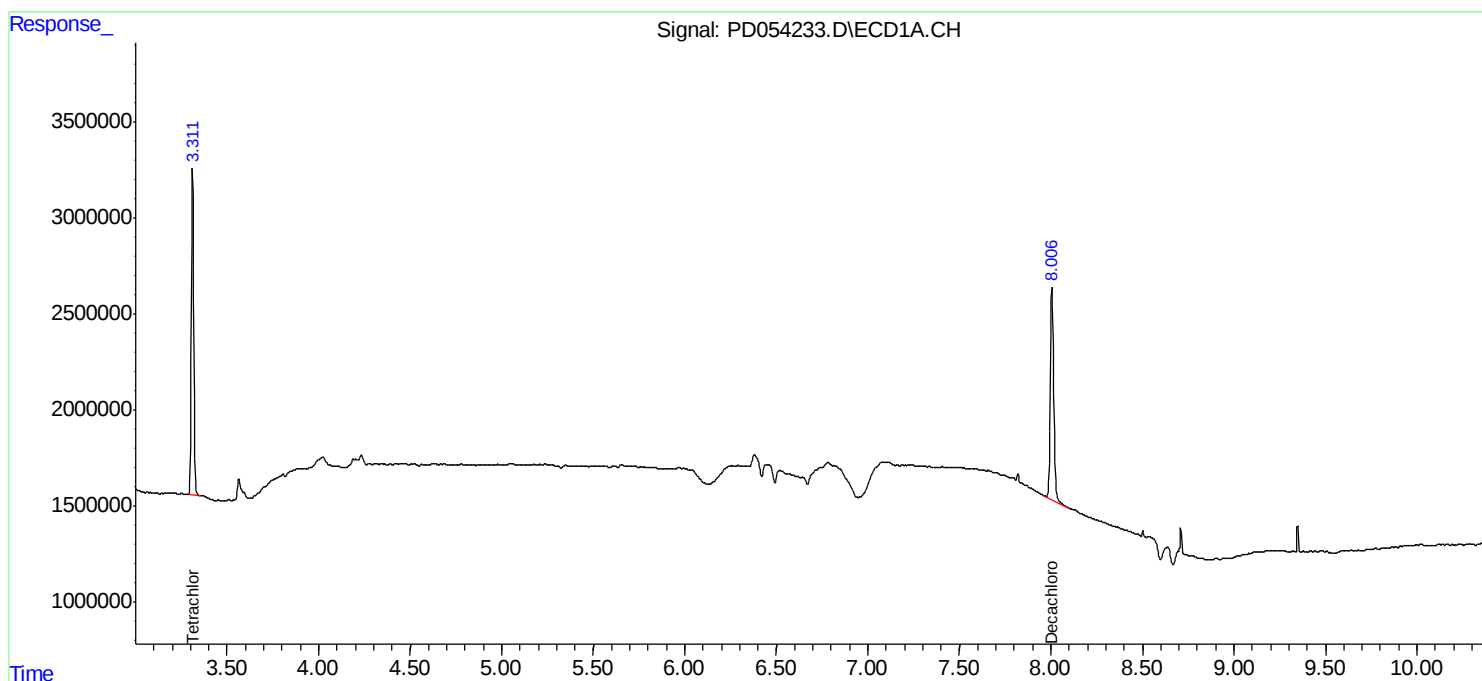

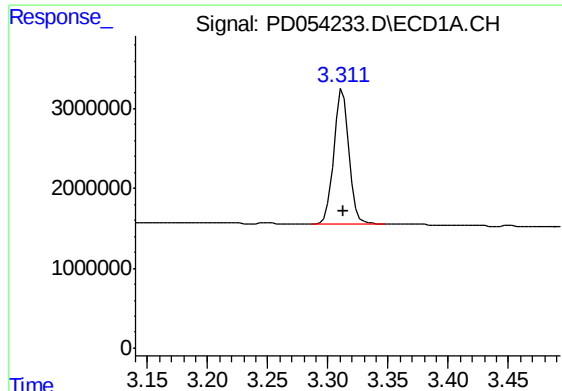


#1 Tetrachloro-m-xylene

R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 14867344
Conc: 25.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
1S-J-(0-1)-COMP


Manual Integrations
APPROVED

Ankita
8/12/2019 1:20:42 PM

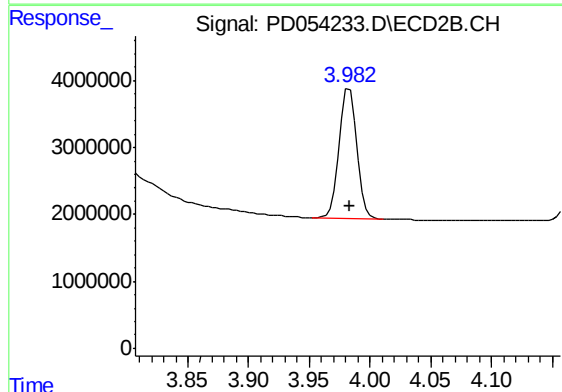


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: -0.001 min
Response: 19579048
Conc: 22.48 ng/ml m

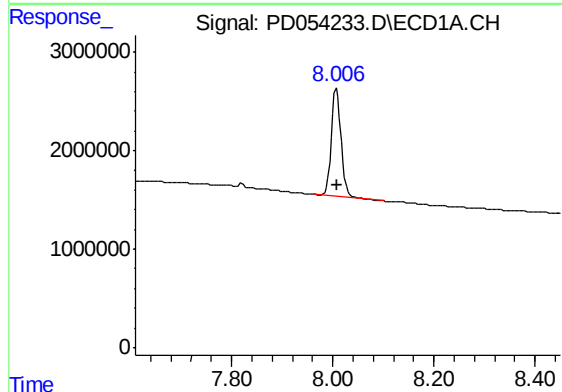

#28 Decachlorobiphenyl

R.T.: 8.008 min
Delta R.T.: -0.001 min
Response: 14825852
Conc: 22.02 ng/ml

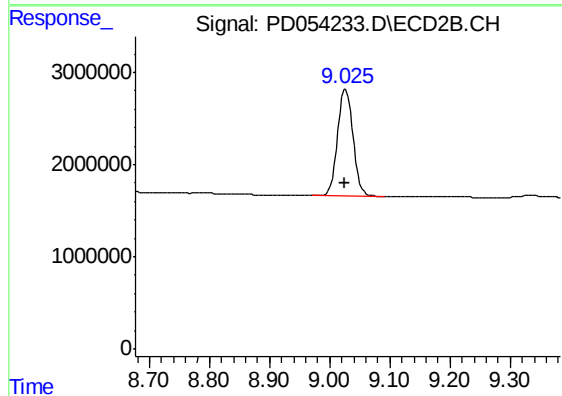

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.001 min
Response: 20966382
Conc: 22.62 ng/ml