

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080921\
 Data File : PD064839.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2021 15:58
 Operator : AR\AJ
 Sample : M3288-03MSD
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGB00MSD

Manual Integrations
 APPROVED

Ankita
 8/10/2021 12:55:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 05:20:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 28 07:07:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	5.405	4.618	20754511	183.0E6	17.399	20.031
27)	SA Decachlor...	11.303	10.360	36748324	205.7E6	27.916	34.595
Target Compounds							
2)	A alpha-BHC	5.988	5.319	90667866	700.3E6	55.656	56.816
3)	MA gamma-BHC...	6.385	5.740	85866156	612.5E6	54.749	53.715
4)	MA Heptachlor	7.035	6.147	80703000	558.5E6	48.020	49.256m
5)	MB Aldrin	7.405	6.472	73033377	494.0E6	46.366	46.958
6)	B beta-BHC	6.644	6.114	37596899	253.2E6	48.191	41.743m
7)	B delta-BHC	6.909	6.377	86682834	563.4E6	49.813	51.859
8)	B Heptachlo...	7.874	7.045	76029480	437.7E6	44.284	47.287
9)	A Endosulfan I	8.278	7.447	71184051	372.7E6	50.497	48.470
10)	B trans-Chl...	8.144	7.321	73989351	402.6E6	46.172	44.392
11)	B cis-Chlor...	8.226	7.390	73310770	387.7E6	47.051	43.580
12)	B 4,4'-DDE	8.421	7.602	135.2E6	659.3E6	93.818	87.376
13)	MA Dieldrin	8.569	7.732	157.5E6	708.0E6	105.619	88.147
14)	MA Endrin	8.807	8.022	136.8E6	598.3E6	106.829	104.156
15)	B Endosulfa...	9.043	8.331	133.9E6	545.6E6	103.119	94.511
16)	A 4,4'-DDD	8.961	8.185	127.7E6	532.5E6	104.037	92.459
17)	MA 4,4'-DDT	9.278	8.445	125.9E6	509.4E6	96.440	92.539
18)	B Endrin al...	9.179	8.518	106.7E6	419.1E6	94.200	84.927
19)	B Endosulfa...	9.417	8.748	136.7E6	497.1E6	99.214	92.214
20)	A Methoxychlor	9.771	9.037	354.0E6	1140.3E6	494.770	445.306
21)	B Endrin ke...	9.913	9.267	156.9E6	609.9E6	103.677	101.669

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080921\
Data File : PD064839.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2021 15:58
Operator : AR\AJ
Sample : M3288-03MSD
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 05:20:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072721CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 28 07:07:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

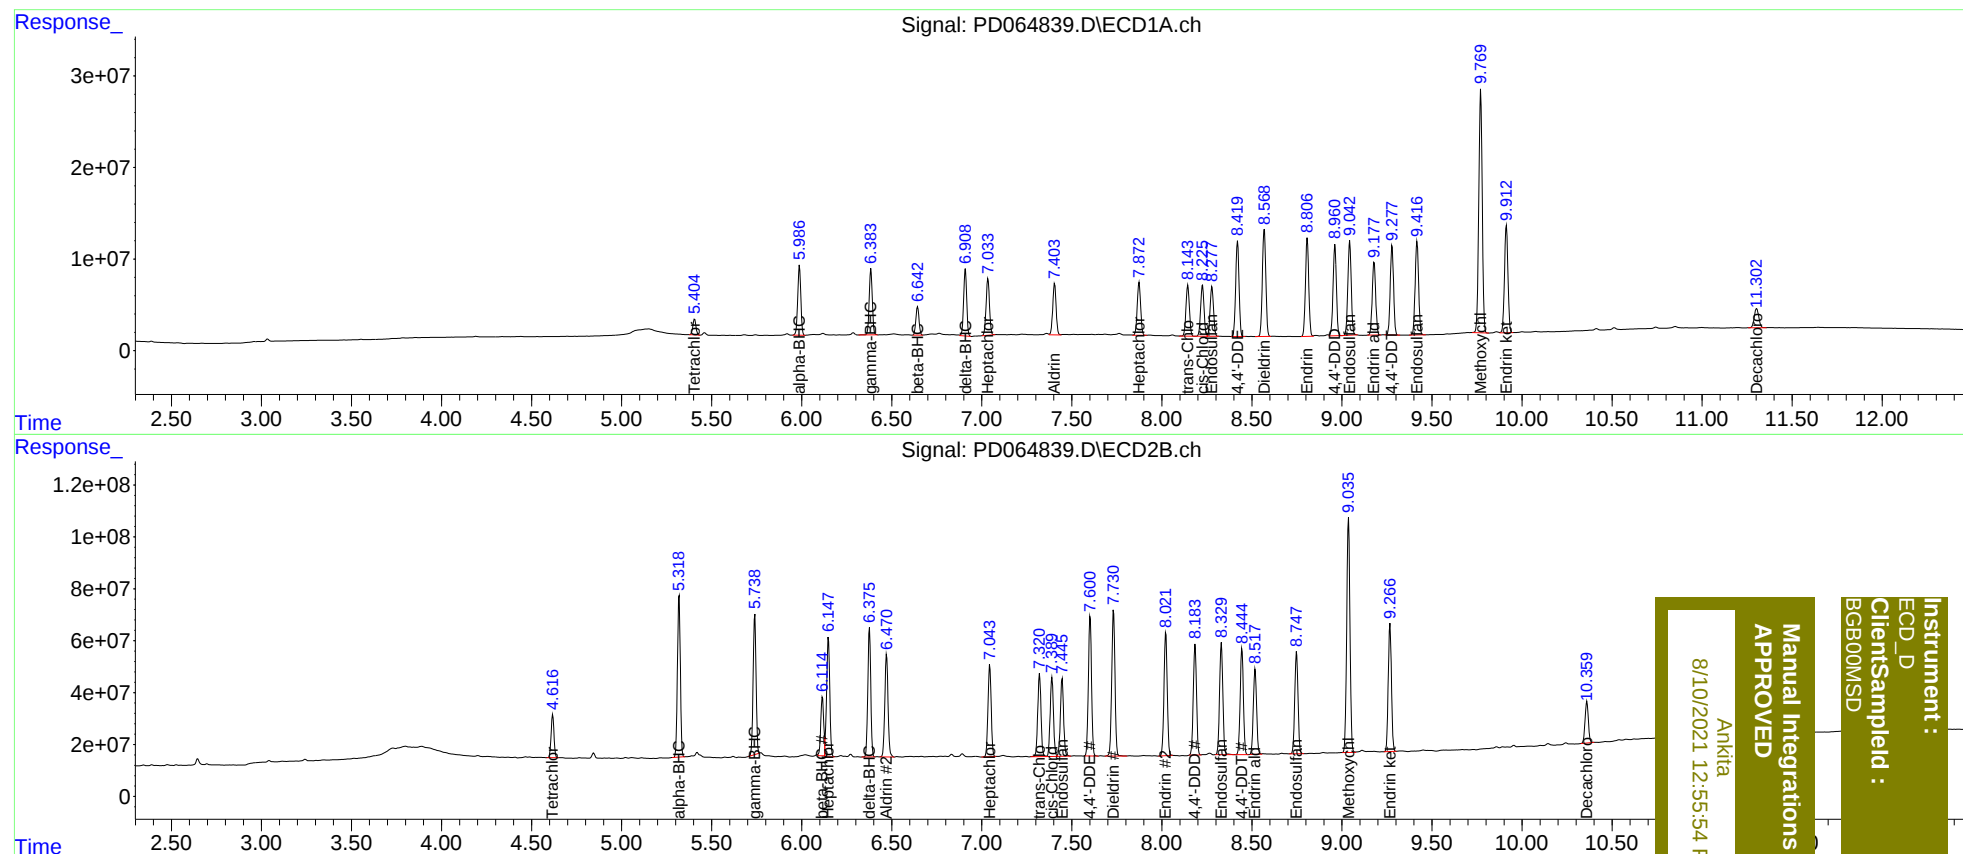

8/10/2021 12:55:54 PM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
BGB00M/SD