

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
 Data File : PD071467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 15:52
 Operator : AR\AJ
 Sample : N4047-01RE
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-DECANTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:17:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.814	3.574	33905054	240.9E6	11.955	8.556 #
28)	SA Decachlor...	8.011	9.102	41978285	80736743	15.135m	7.799 #
Target Compounds							
14)	MA Endrin	5.731	6.628	29799547	32232931	9.412m	2.577 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
Data File : PD071467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 15:52
Operator : AR\AJ
Sample : N4047-01RE
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:17:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

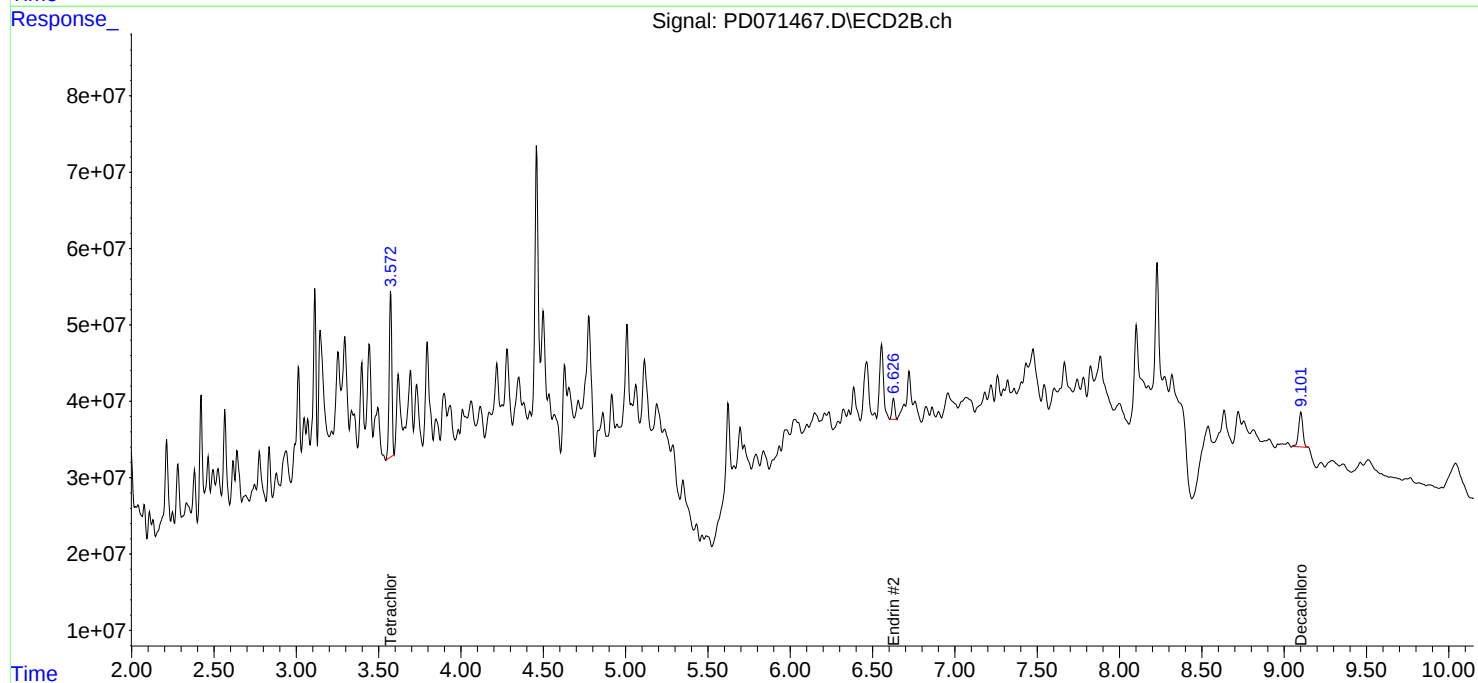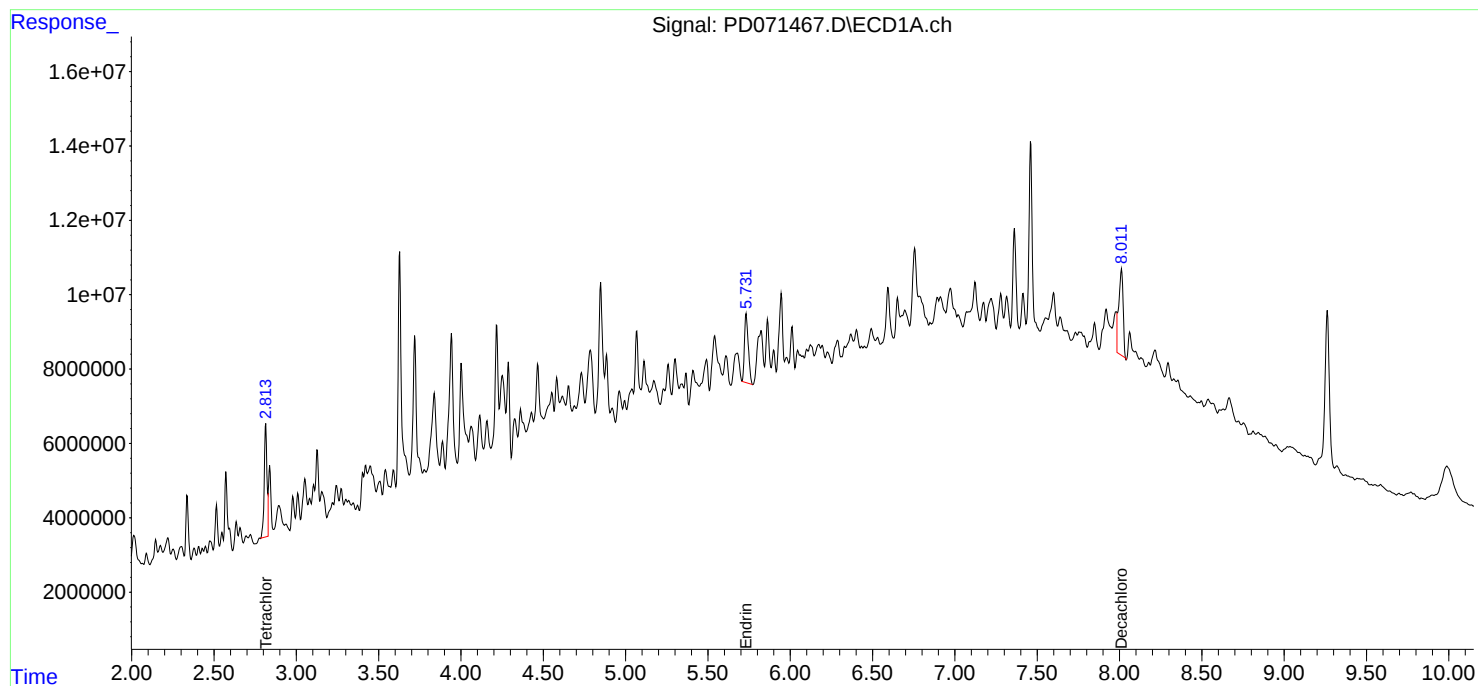

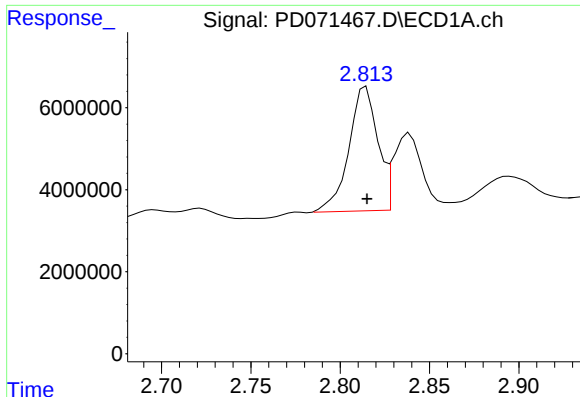


#1 Tetrachloro-m-xylene

R.T.: 2.814 min
Delta R.T.: 0.000 min
Response: 33905054
Conc: 11.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

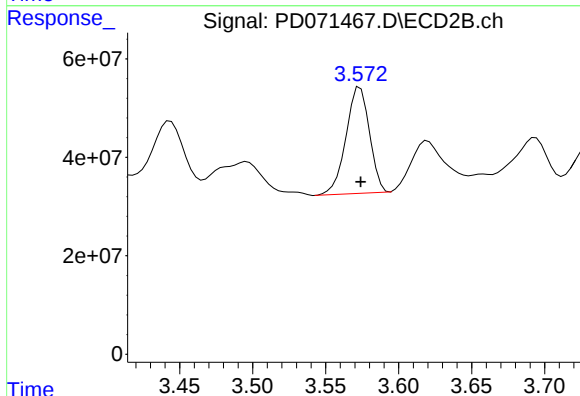


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.000 min
Response: 240851961
Conc: 8.56 ng/ml

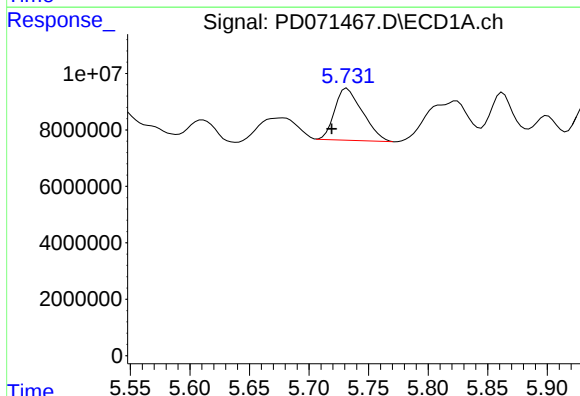


#14 Endrin

R.T.: 5.731 min
Delta R.T.: 0.012 min
Response: 29799547
Conc: 9.41 ng/ml m

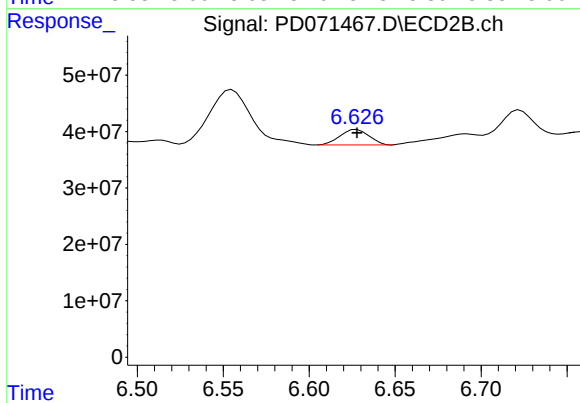

#14 Endrin

R.T.: 6.628 min
Delta R.T.: 0.000 min
Response: 32232931
Conc: 2.58 ng/ml

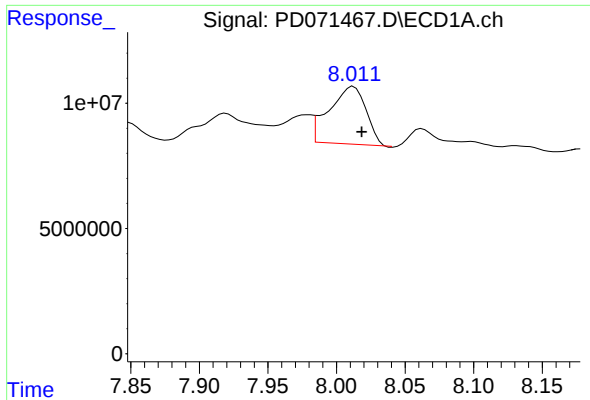


#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.007 min
Response: 41978285
Conc: 15.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-DECANTRE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

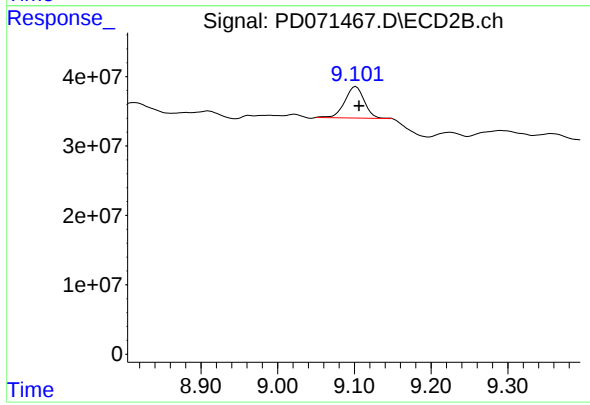

#28 Decachlorobiphenyl

R.T.: 9.102 min
Delta R.T.: -0.004 min
Response: 80736743
Conc: 7.80 ng/ml