

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
 Data File : PD071468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 16:05
 Operator : AR\AJ
 Sample : N4049-01RE
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BI-WEEKLY-INFLUENTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:17:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.815	3.573	26583367	254.5E6	9.374	9.042
28) SA Decachlor...	8.014	9.110	11851115	43977230	4.273	4.248m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
Data File : PD071468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 16:05
Operator : AR\AJ
Sample : N4049-01RE
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:17:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

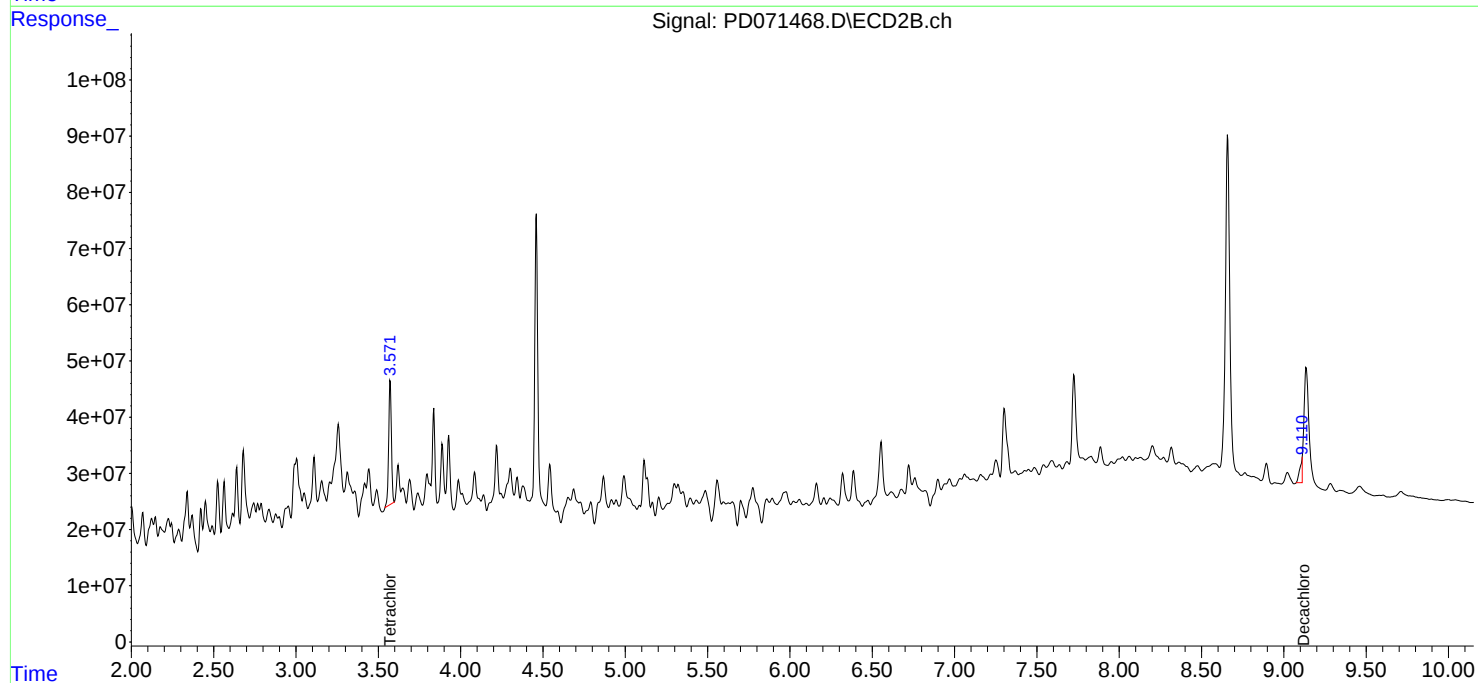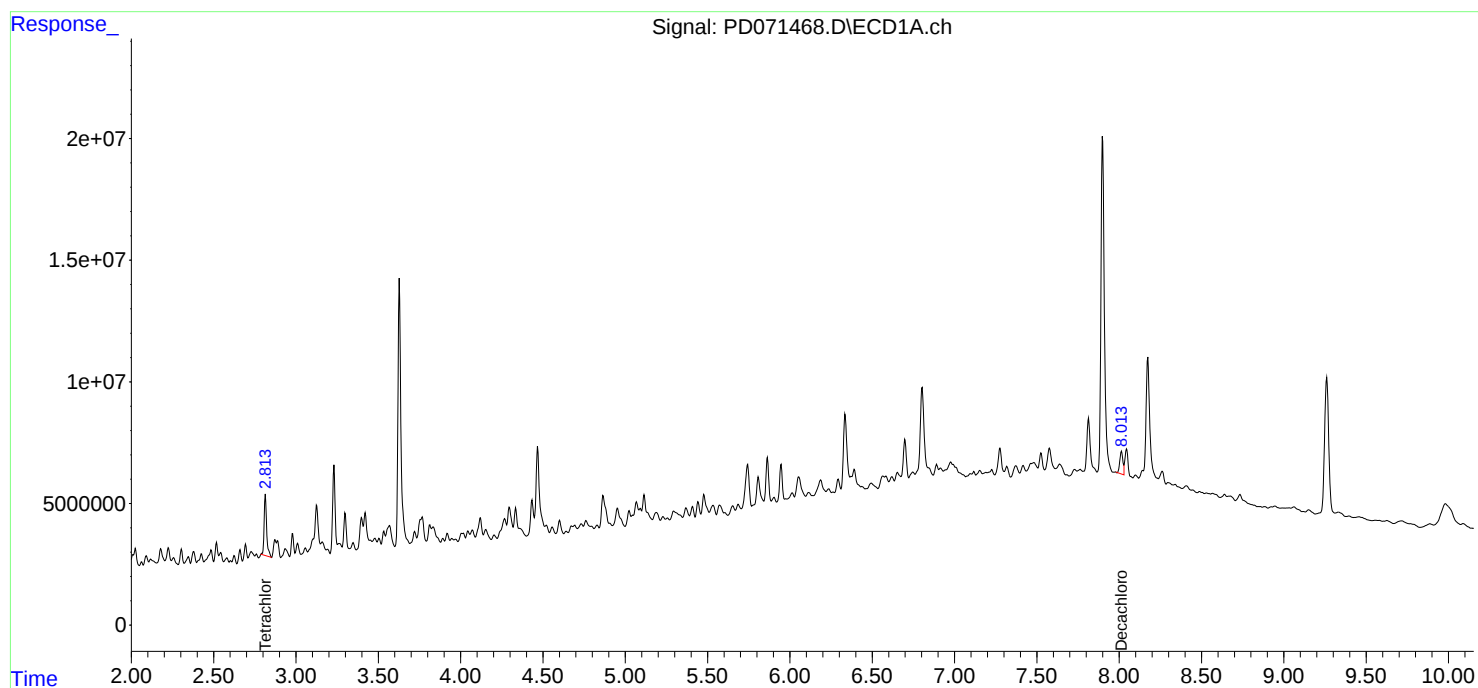

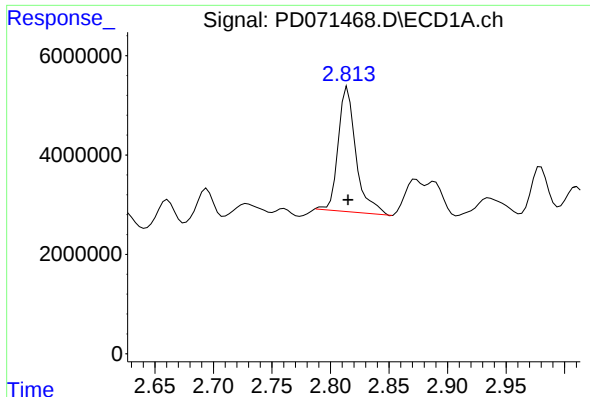


#1 Tetrachloro-m-xylene

R.T.: 2.815 min
Delta R.T.: 0.000 min
Response: 26583367
Conc: 9.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

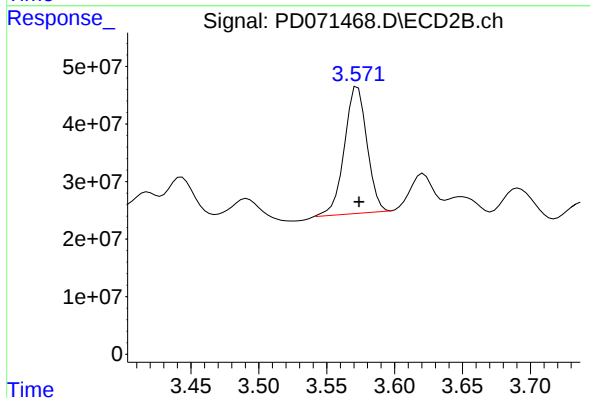


#1 Tetrachloro-m-xylene

R.T.: 3.573 min
Delta R.T.: -0.001 min
Response: 254537494
Conc: 9.04 ng/ml

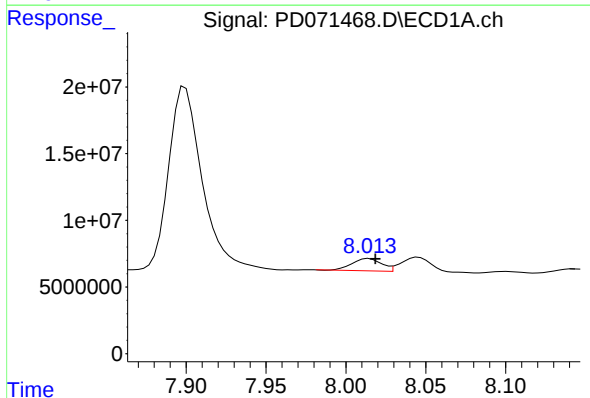

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.004 min
Response: 11851115
Conc: 4.27 ng/ml

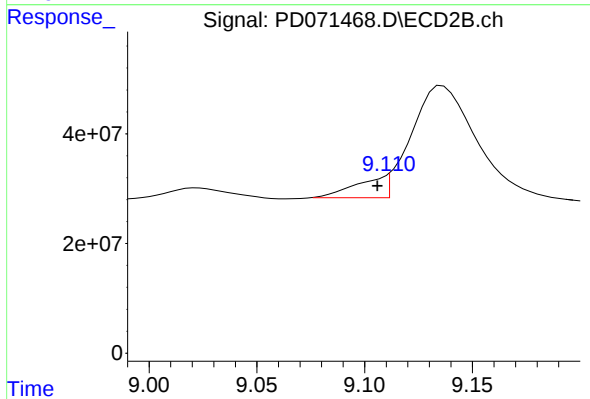

#28 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: 0.004 min
Response: 43977230
Conc: 4.25 ng/ml m