

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
 Data File : PD071469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Aug 2022 16:19
 Operator : AR\AJ
 Sample : N4051-01RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MONTHLY-OUTFALL-002RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/10/2022
 Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 00:17:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 03:39:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.814	3.572	45079569	309.7E6	15.896	11.001 #
28) SA Decachlor...	8.012	9.101	26313288	59182356	9.487	5.717 #
Target Compounds						
14) MA Endrin	5.729	6.630	29024276	72074581	9.167m	5.762 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080922\
Data File : PD071469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Aug 2022 16:19
Operator : AR\AJ
Sample : N4051-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 00:17:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 03:39:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

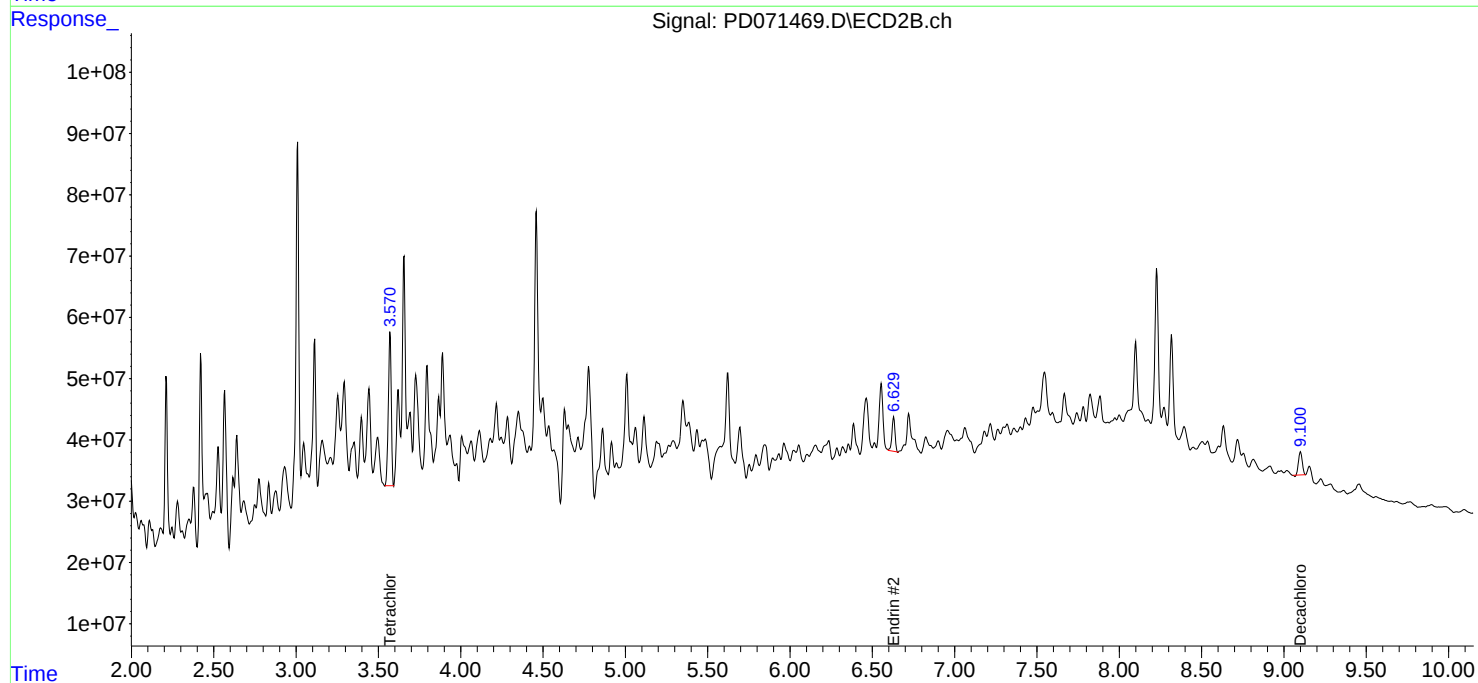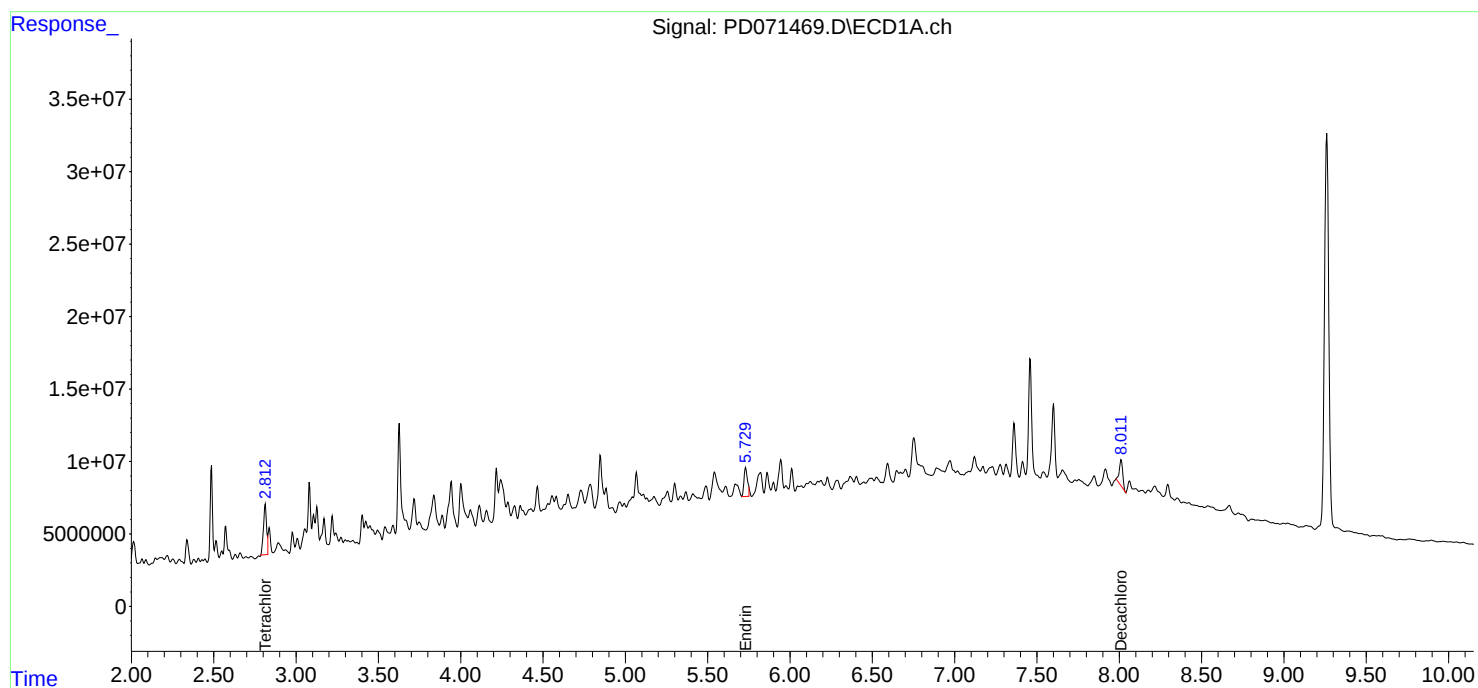

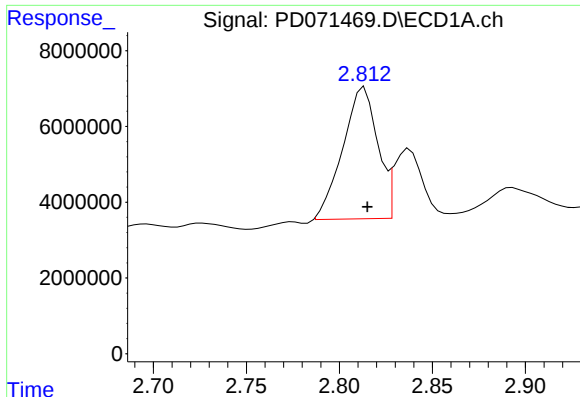


#1 Tetrachloro-m-xylene

R.T.: 2.814 min
Delta R.T.: -0.001 min
Response: 45079569
Conc: 15.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

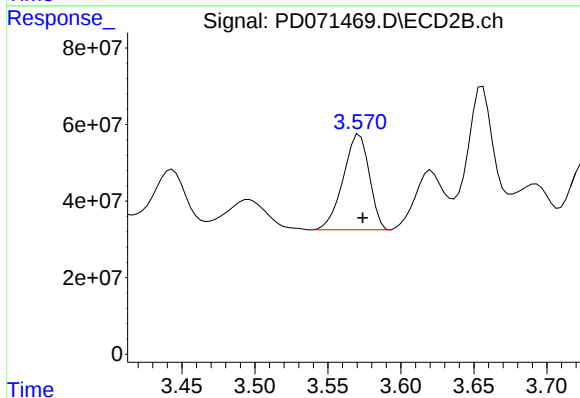


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: -0.002 min
Response: 309682708
Conc: 11.00 ng/ml

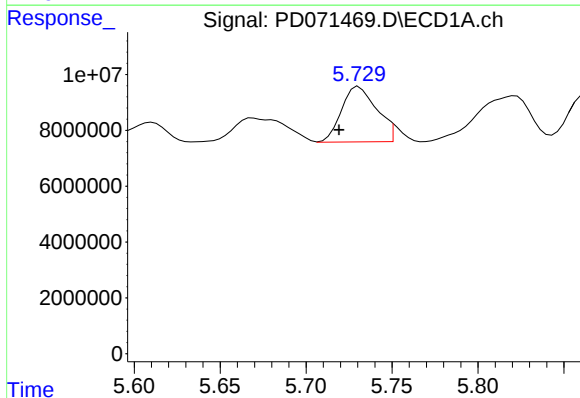


#14 Endrin

R.T.: 5.729 min
Delta R.T.: 0.010 min
Response: 29024276
Conc: 9.17 ng/ml m

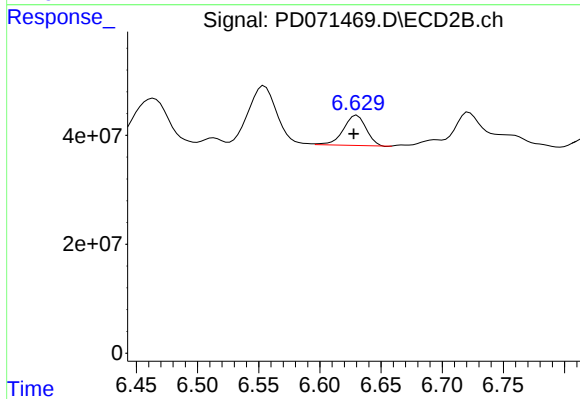

#14 Endrin

R.T.: 6.630 min
Delta R.T.: 0.002 min
Response: 72074581
Conc: 5.76 ng/ml

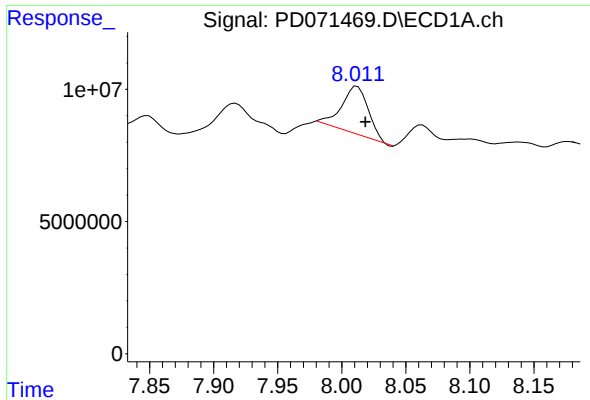


#28 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.006 min
Response: 26313288
Conc: 9.49 ng/ml

Instrument :
ECD_D
ClientSampleId :
MONTHLY-OUTFALL-002RE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/10/2022
Supervised By :Ankita Jodhani 08/10/2022

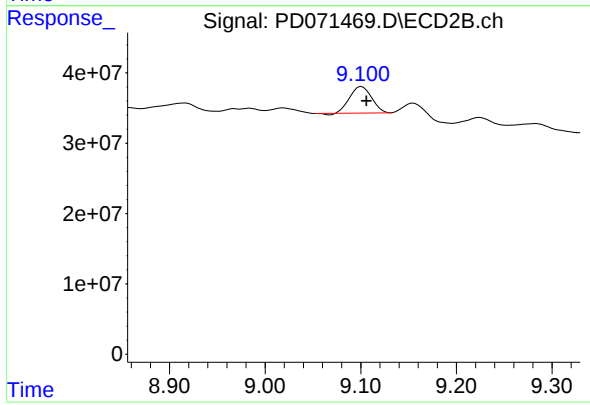

#28 Decachlorobiphenyl

R.T.: 9.101 min
Delta R.T.: -0.005 min
Response: 59182356
Conc: 5.72 ng/ml