

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081018\
 Data File : PD048793.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Aug 2018 9:15
 Operator : AJ\SJ
 Sample : PB111902BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 23:14:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072818CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 28 05:19:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.371	3.967	24161355	326.2E6	17.536	16.958
27) SA Decachlor...	8.068	8.993	57169194	612.6E6	35.293	34.126
Target Compounds						
4) MA Heptachlor	0.000	5.096f	0	5829610	N.D.	0.233


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081018\
Data File : PD048793.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Aug 2018 9:15
Operator : AJ\SJ
Sample : PB111902BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 23:14:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD072818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jul 28 05:19:54 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

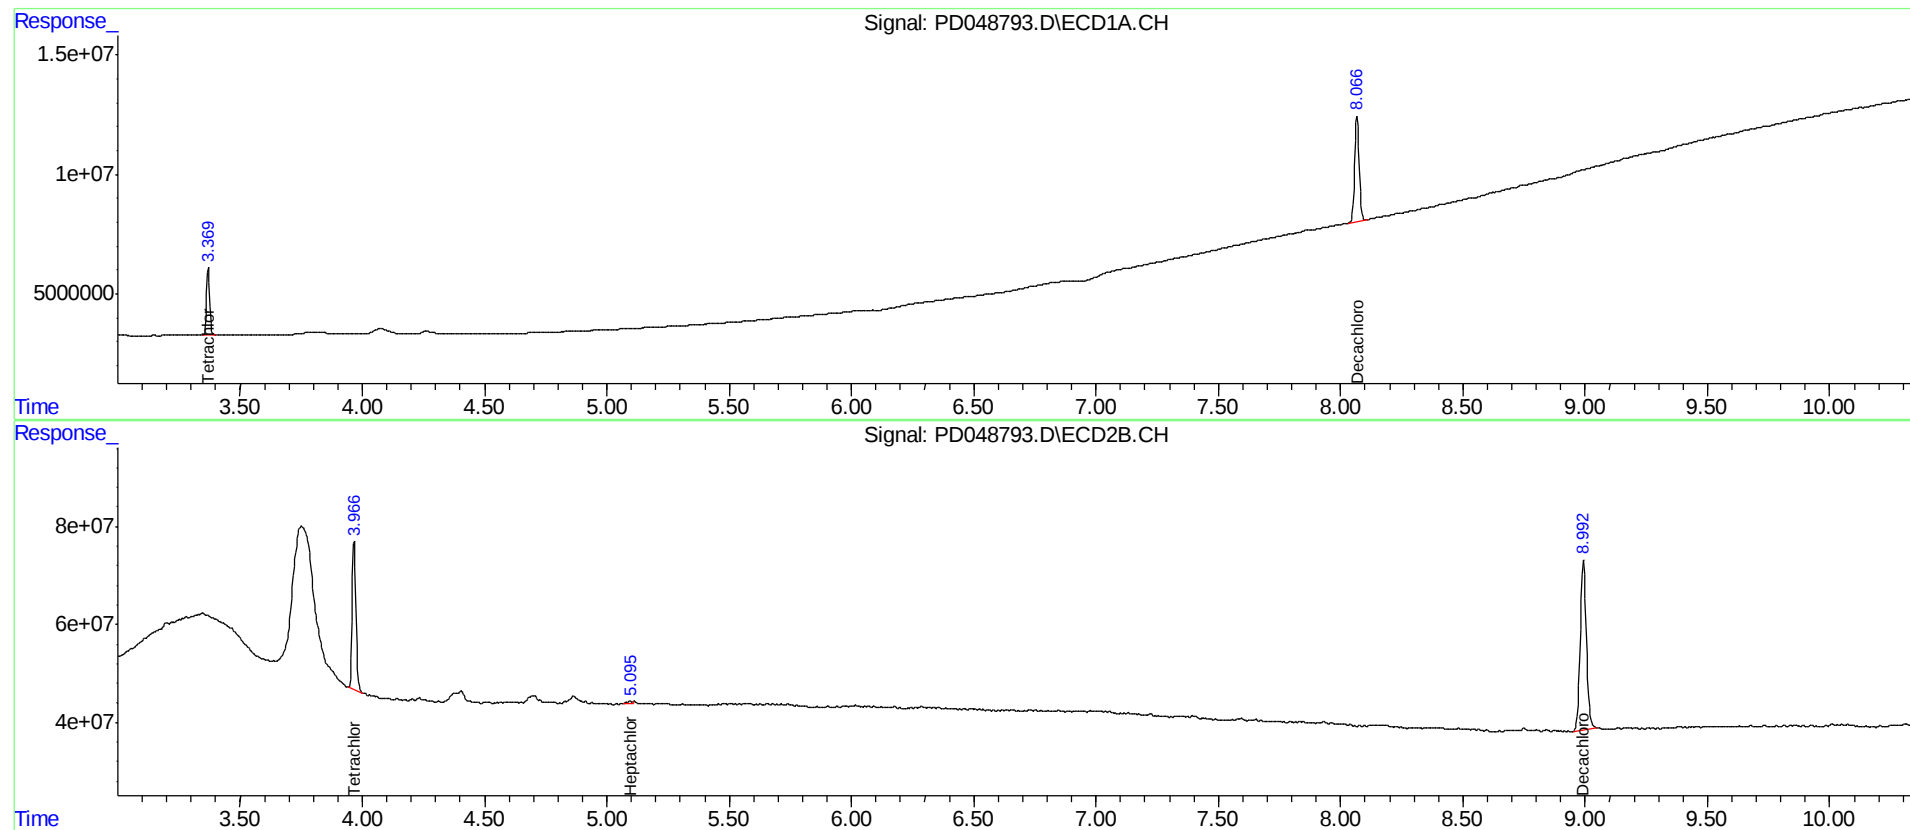


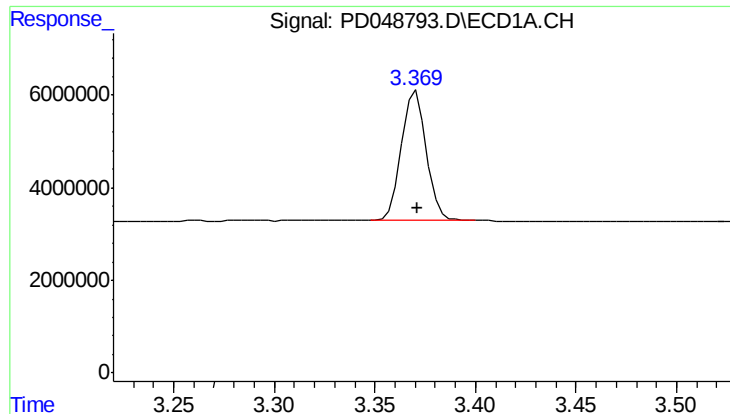

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 24161355
Conc: 17.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK02

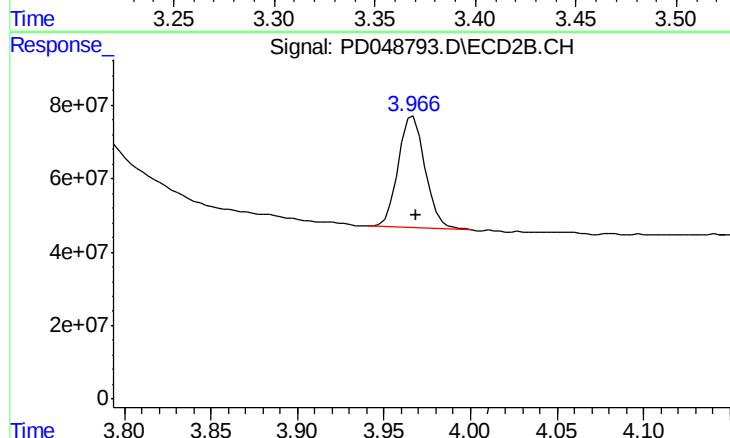


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.001 min
Response: 326207379
Conc: 16.96 ng/ml

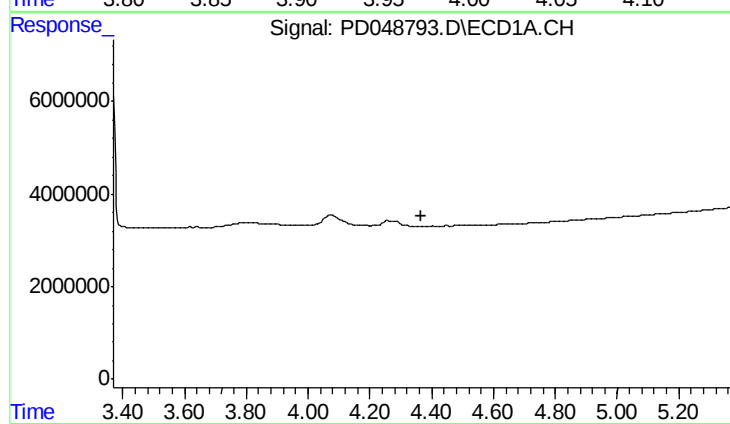


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.368 min
Response: 0
Conc: N.D.

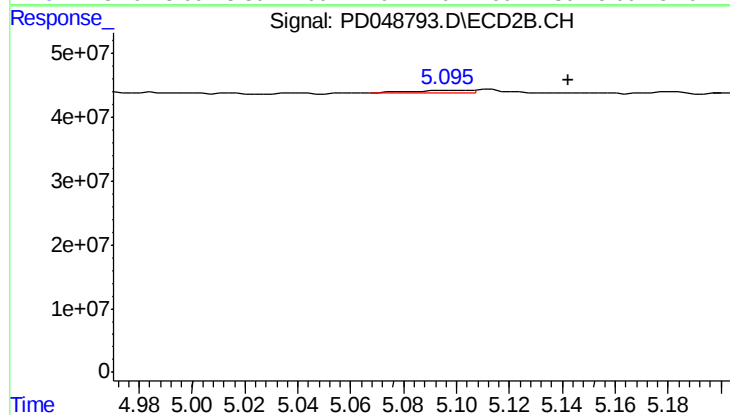

#4 Heptachlor


R.T.: 5.096 min
Delta R.T.: -0.046 min
Response: 5829610
Conc: 0.23 ng/ml

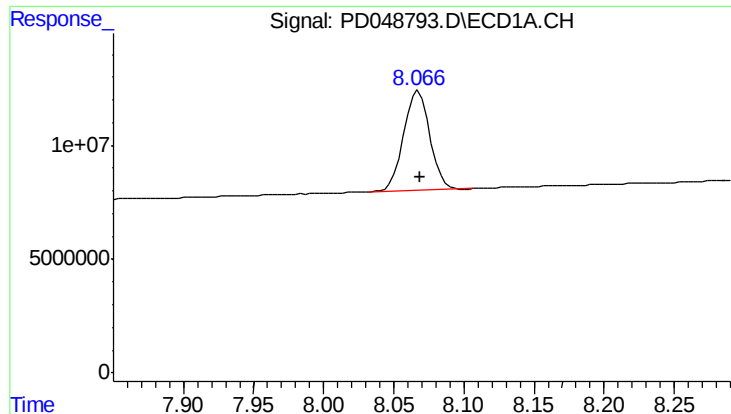

#27 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 57169194
Conc: 35.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK02

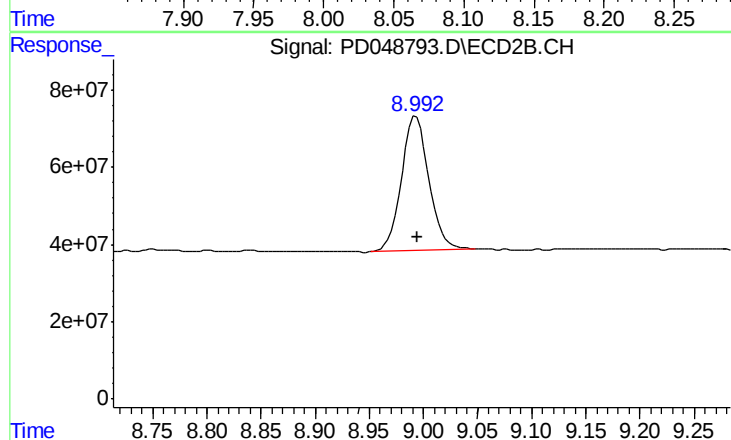

#27 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: -0.001 min
Response: 612585859
Conc: 34.13 ng/ml