

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
 Data File : PD071475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2022 17:38
 Operator : AR\AJ
 Sample : TOXAPH101
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 21:23:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 10 21:17:27 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.808	3.565	14706461	169.5E6	5.394	5.772
27)	SA Decachlor...	8.003	9.095	25408643	103.4E6	10.530	11.901
Target Compounds							
22)	Toxaphene-1	5.394	6.272	9374358	63399341	521.635	578.993
23)	Toxaphene-2	5.756	6.675	9221087	46302488	484.636	586.216
24)	Toxaphene-3	6.040	7.097	10858953	162.7E6	504.027	542.834
25)	Toxaphene-4	6.806	7.190	40945437	131.1E6	470.532	542.802
26)	Toxaphene-5	7.123	7.618	18259306	78038406	455.151	552.156

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 17:38
Operator : AR\AJ
Sample : TOXAPH101
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 21:23:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 21:17:27 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

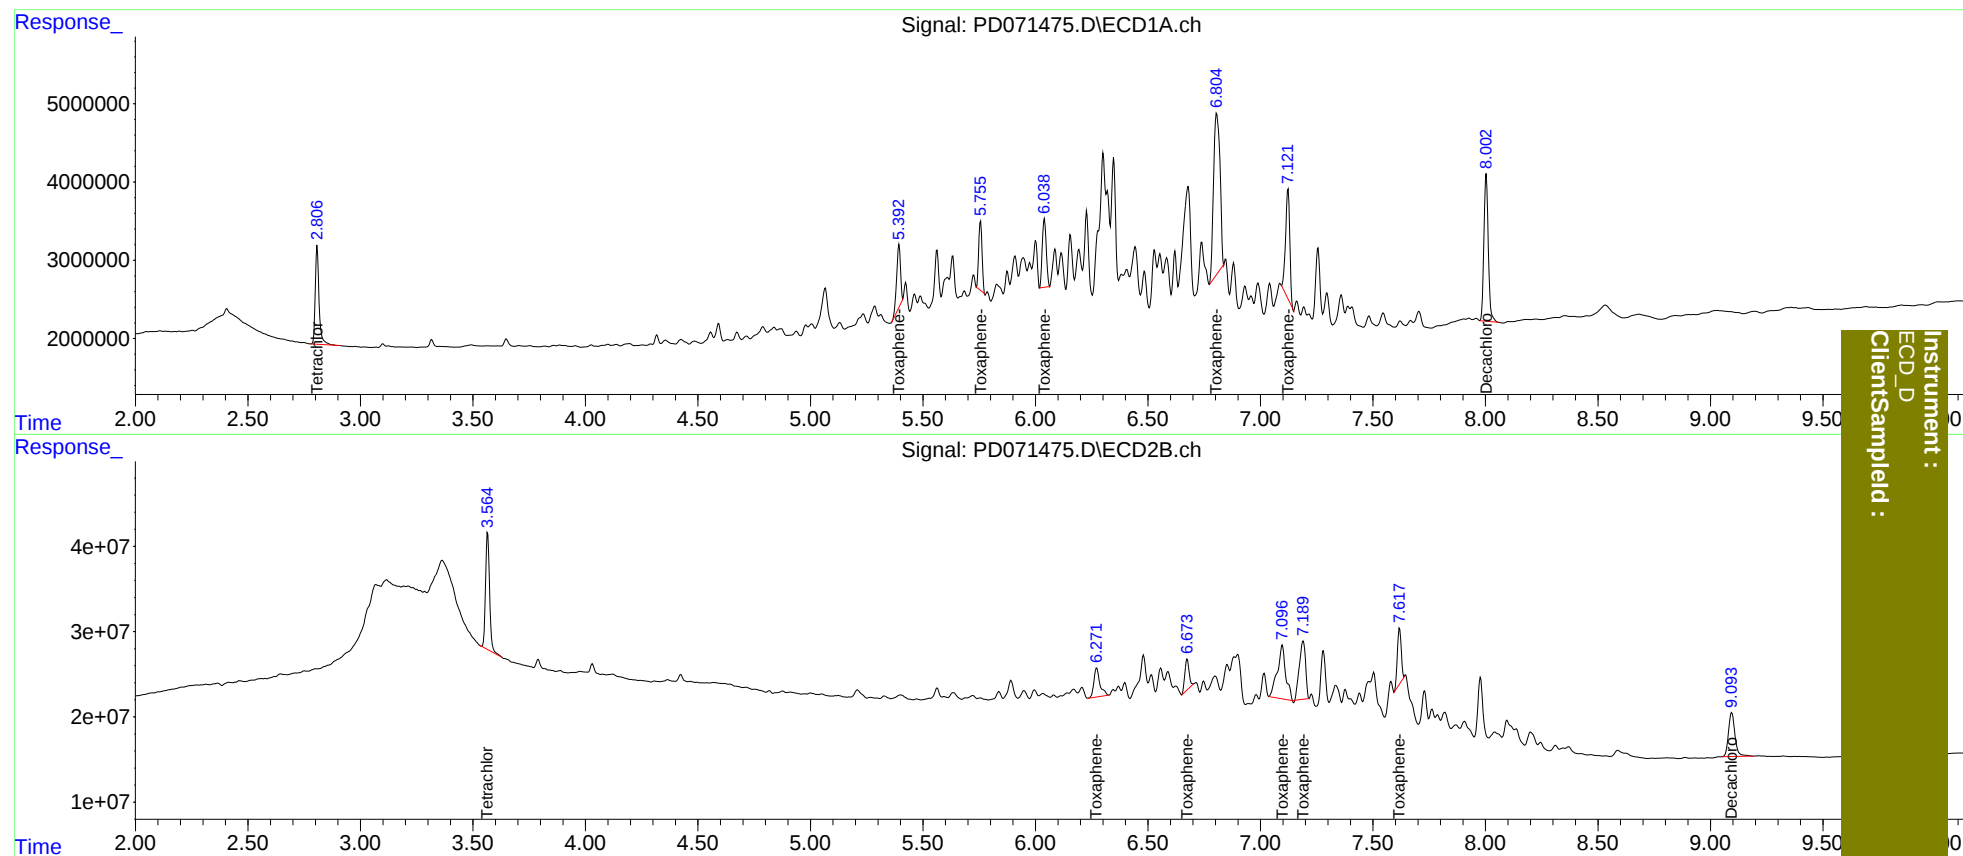

Instrument :
ECD_D
ClientSampled :
0