

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
 Data File : PD071473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2022 17:11
 Operator : AR\AJ
 Sample : RESC034
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC036

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 22:51:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 10 22:43:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.808	3.566	52080207	574.6E6	18.392	18.546
27)	SA Decachlor...	8.004	9.094	91556646	351.0E6	35.909	37.037
Target Compounds							
2)	A alpha-BHC	3.317	4.032	37456100	405.6E6	8.900	10.023
3)	MA gamma-BHC...	3.651	4.368	35488391	339.0E6	9.112	10.197
4)	MA Heptachlor	3.997	4.945	37027942	255.8E6	9.196	10.487
5)	MB Aldrin	4.282	5.288	36994383	217.6E6	9.098	10.275
6)	B beta-BHC	3.950	4.574	15939871	136.5E6	9.373	9.919
7)	B delta-BHC	4.183	4.821	34083001	261.1E6	8.739	9.863
8)	B Heptachlo...	4.789	5.719	33711847	178.3E6	9.170	10.135
9)	A Endosulfan I	5.162	6.107	31572829	157.5E6	9.446	10.256
10)	B trans-Chl...	5.042	5.974	34801320	172.1E6	8.993	9.840
11)	B cis-Chlor...	5.106	6.052	34224799	166.4E6	8.994	9.837
12)	B 4,4'-DDE	5.297	6.225	59640929	289.8E6	17.623	19.361
13)	MA Dieldrin	5.429	6.385	68732940	314.0E6	18.265	19.791
14)	MA Endrin	5.707	6.618	59233301	251.7E6	18.413	19.542
15)	B Endosulfa...	6.002	6.844	54488852	240.2E6	18.269	19.386
16)	A 4,4'-DDD	5.856	6.749	46568928	219.7E6	17.822	19.016
17)	MA 4,4'-DDT	6.109	7.061	47045782	215.9E6	16.896	18.698
18)	B Endrin al...	6.183	6.975	47193092	201.6E6	18.754	19.477
19)	B Endosulfa...	6.407	7.207	53165101	224.6E6	18.201	19.340
20)	A Methoxychlor	6.689	7.537	129.6E6	496.9E6	93.676	99.710
21)	B Endrin ke...	6.917	7.699	68192517	248.5E6	19.771	19.824

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 17:11
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 22:51:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 22:43:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

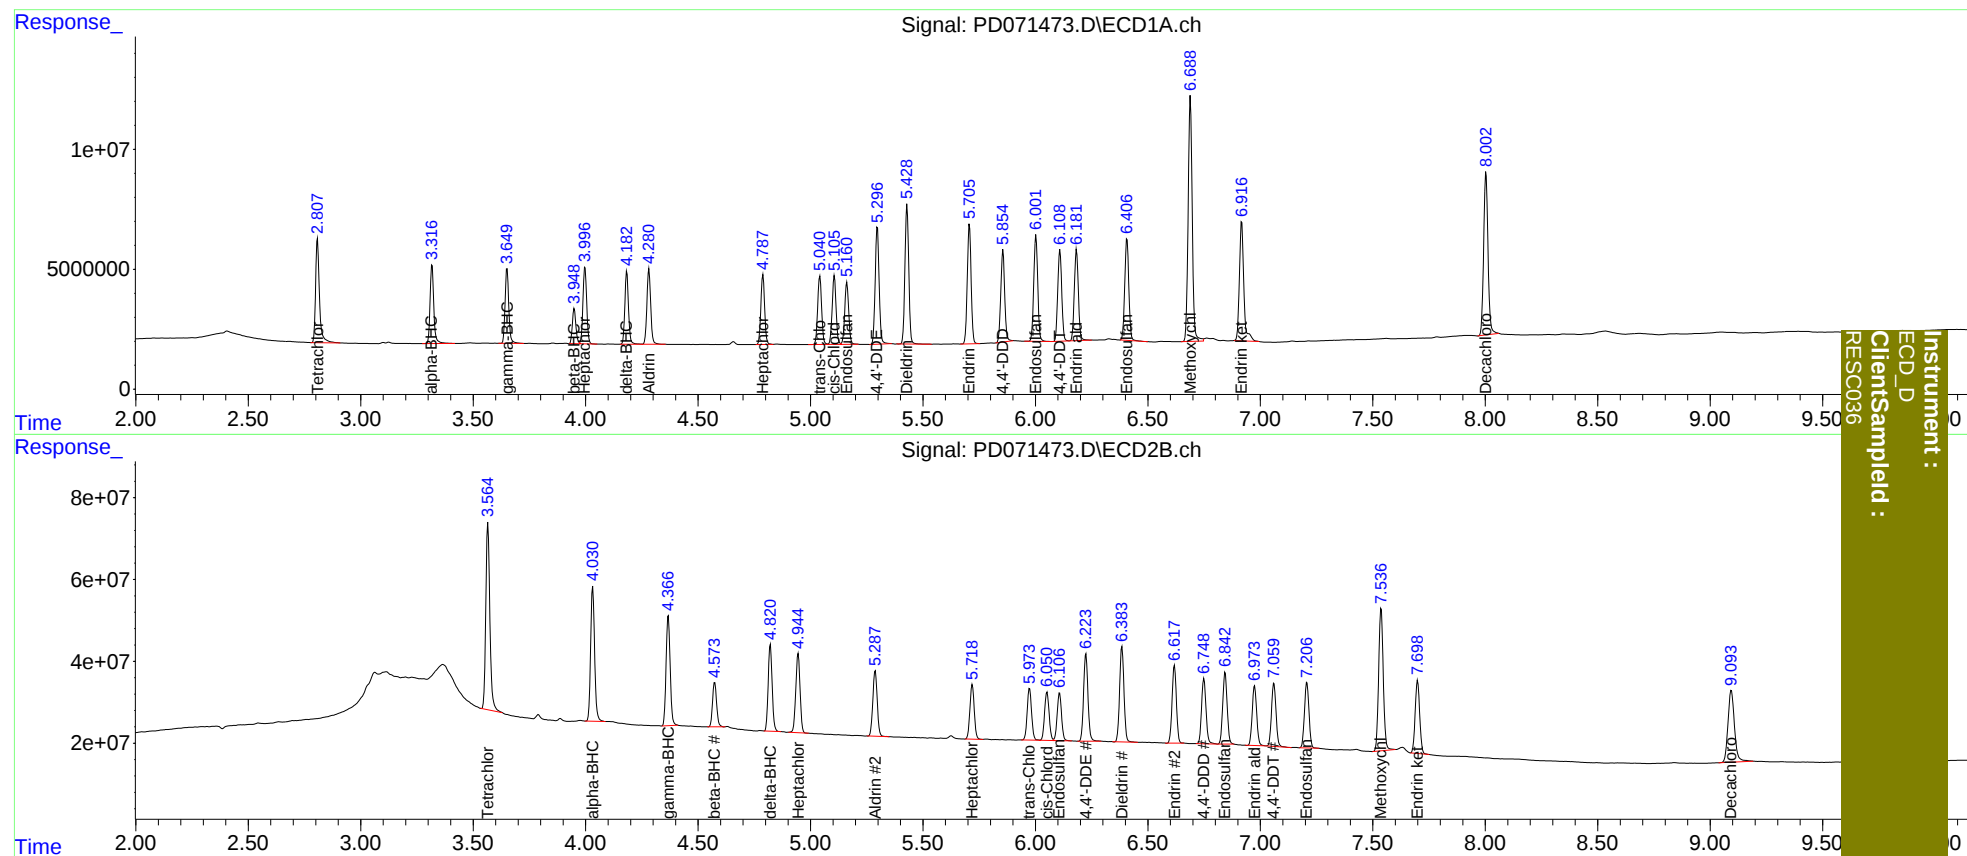

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071473.D
Acq On : 10 Aug 2022 17:11
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Title : GC Extractables
Last Update : Wed Aug 10 22:43:30 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
2.808	3.317	100.00%
3.317	3.651	100.00%
3.651	3.950	100.00%
3.950	3.997	97.73%
3.997	4.183	100.00%
4.183	4.282	100.00%
4.282	4.789	100.00%
4.789	5.042	100.00%
5.042	5.106	100.00%
5.106	5.162	99.56%
5.162	5.297	100.00%
5.297	5.429	100.00%
5.429	5.707	100.00%
5.707	5.856	100.00%
5.856	6.002	100.00%
6.002	6.109	100.00%
6.109	6.183	100.00%
6.183	6.407	100.00%
6.407	6.689	100.00%
6.689	6.917	100.00%
6.917	8.004	100.00%

Signal #2


3.566	4.032	100.00%
4.032	4.368	100.00%
4.368	4.574	100.00%
4.574	4.821	100.00%
4.821	4.945	100.00%
4.945	5.288	100.00%
5.288	5.719	100.00%
5.719	5.974	100.00%
5.974	6.052	99.97%
6.052	6.107	96.51%
6.107	6.225	100.00%
6.225	6.385	100.00%
6.385	6.618	100.00%
6.618	6.749	100.00%
6.749	6.844	100.00%
6.844	6.975	100.00%
6.975	7.061	100.00%
7.061	7.207	100.00%
7.207	7.537	100.00%
7.537	7.699	100.00%
7.699	9.094	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 17:11
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 22:51:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 22:43:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

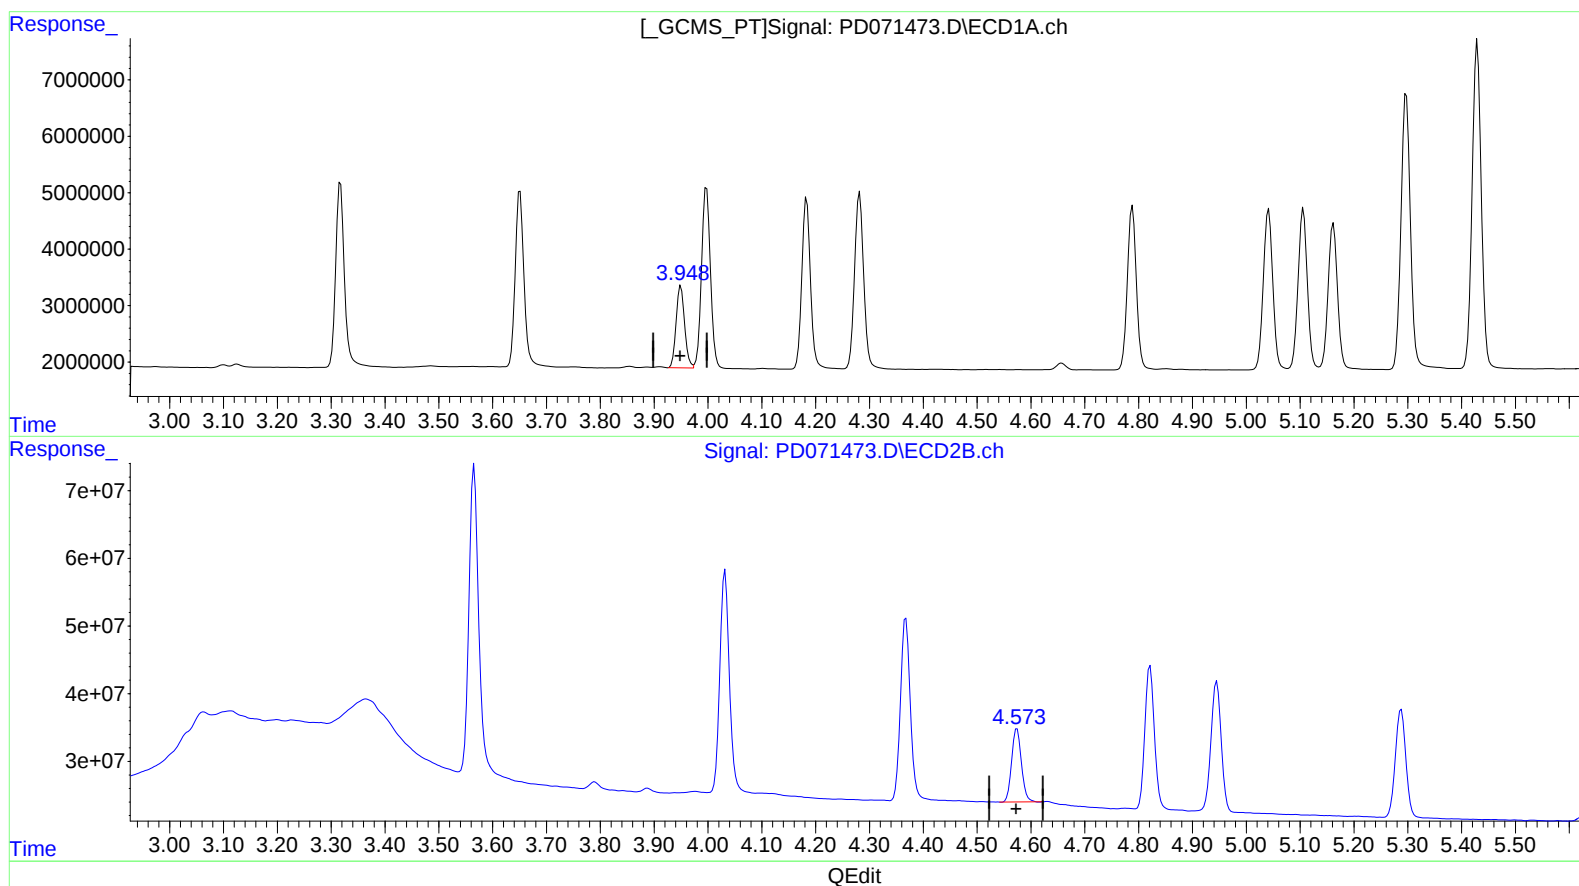

(6) beta-BHC (B)
3.950min 9.373 ng/ml
response 15939871


(6) beta-BHC #2 (B)
4.574min 9.919 ng/ml
response 136475265

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 17:11
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 22:51:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 22:43:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

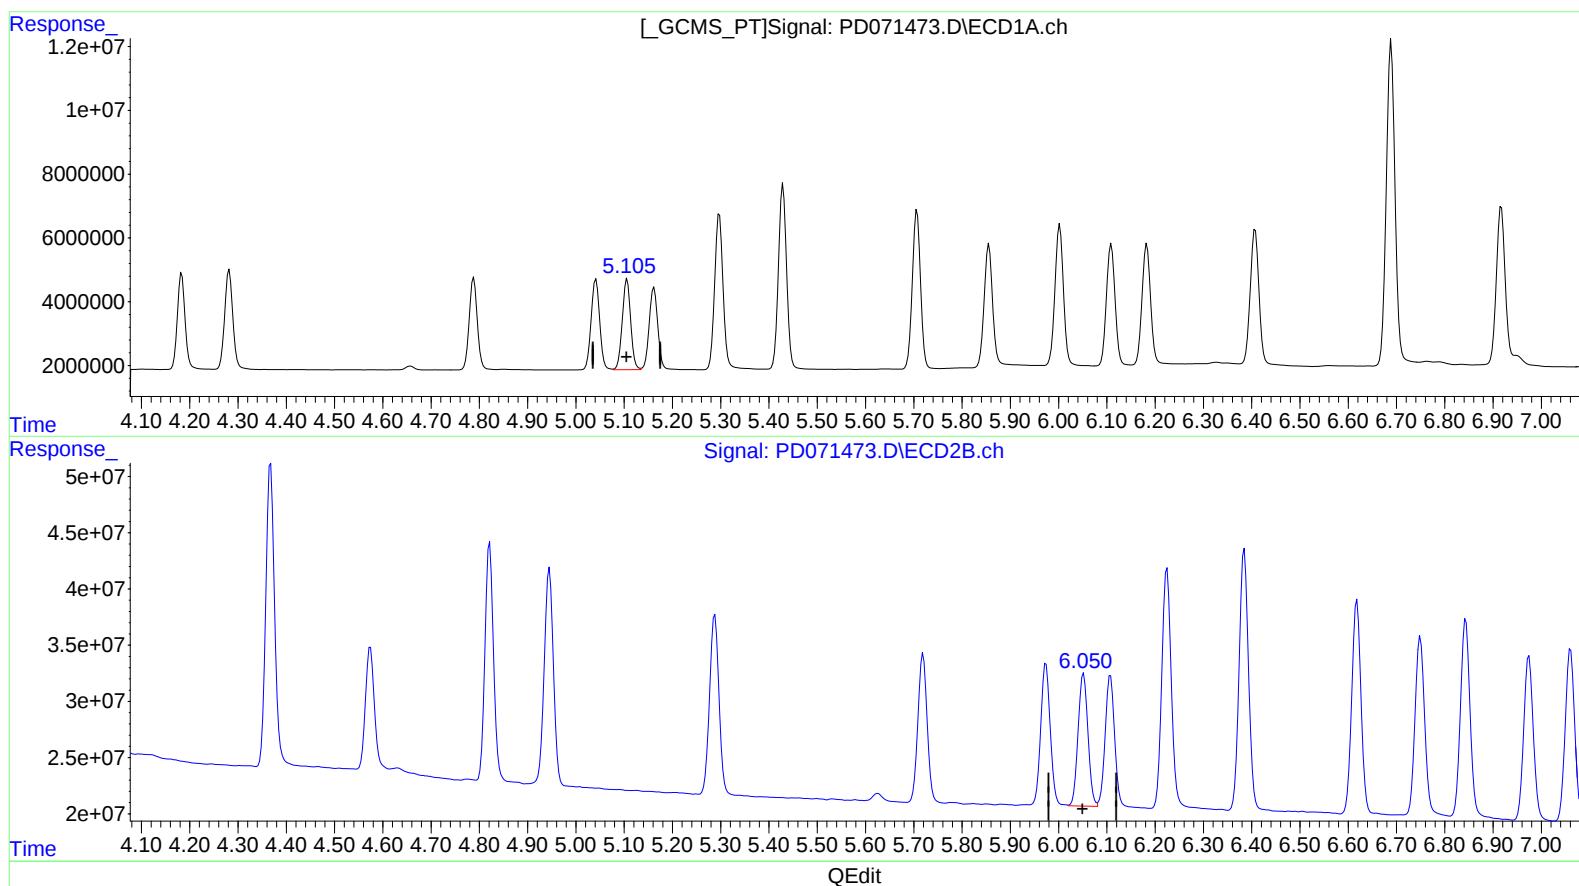

(11) cis-Chlordane (B)

5.106min 8.994 ng/ml

response 34224799

(11) cis-Chlordane #2 (B)

6.052min 9.837 ng/ml


response 166356784

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081022\
Data File : PD071473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 17:11
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 22:51:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081022CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 10 22:43:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

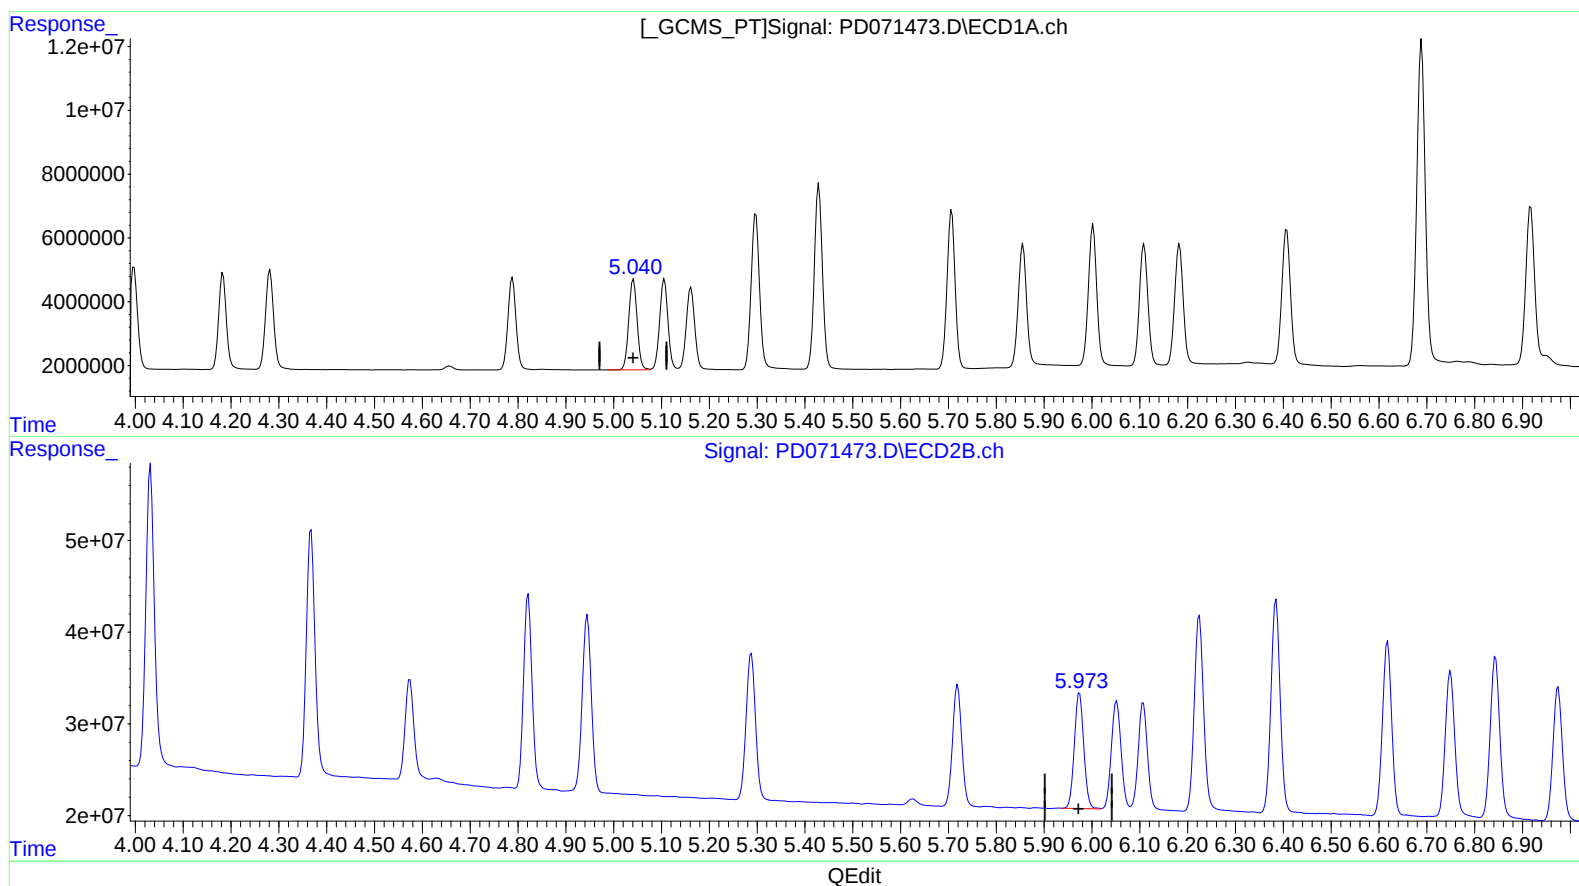

(10) trans-Chlordane (B)

5.042min 8.993 ng/ml

response 34801320

(10) trans-Chlordane #2 (B)

5.974min 9.840 ng/ml

response 172126894