

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081023\
 Data File : PD077067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 12:48
 Operator : AR\AJ
 Sample : 03572-09
 Misc : TOX MDL 50PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/11/2023
 Supervised By :Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:43:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 15:26:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.551	2.762	43045040	24617514	18.685	18.441
7) SA Decachlor...	9.098f	7.907	60287285	27808503	22.112	20.389
Target Compounds						
2) Toxaphene-1	6.260	4.993	1507553	469125	60.837	51.499
3) Toxaphene-2	7.172	5.677	2847966	452087	48.387	49.703
4) Toxaphene-3	7.271	6.592	1917691	982310	53.318	38.664 #
5) Toxaphene-4	7.596	6.721	2216433	1842216	51.420m	44.984
6) Toxaphene-5	7.961	7.035	1830771	625603	42.487	42.627

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081023\
Data File : PD077067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 12:48
Operator : AR\AJ
Sample : 03572-09
Misc : TOX MDL 50PPB
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:43:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 15:26:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

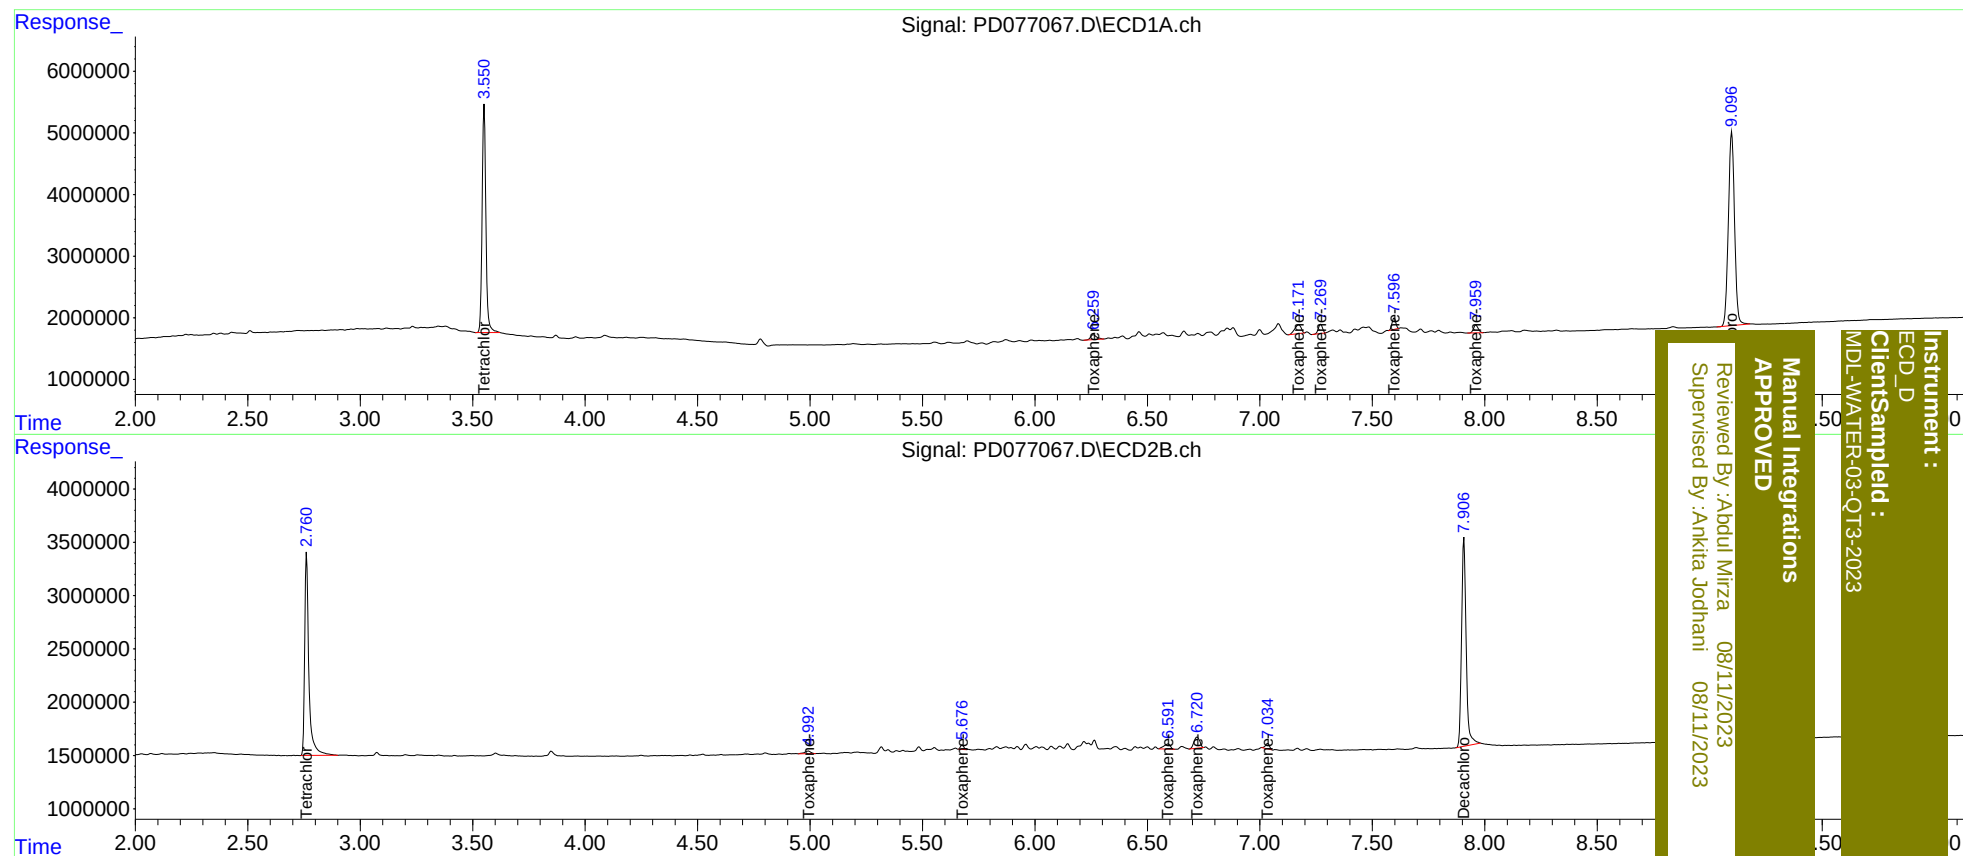

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/11/2023
Supervised By: Ankita Jodhani 08/11/2023

Instrument :
ECD_D
Client Sample :
MDL-WATER-03-QT3-2023