

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081023\
 Data File : PD077097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2023 21:00
 Operator : AR\AJ
 Sample : 03956-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B-PP23A

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2023
 Supervised By : Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 06:33:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	26684261	16160273	11.276	11.864
28)	SA Decachlor...	9.087	7.904	37783300	18349557	13.789	12.822
Target Compounds							
11)	B alpha-Chl...	6.035	5.027	3432406	838554	1.047	0.502m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081023\
Data File : PD077097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2023 21:00
Operator : AR\AJ
Sample : 03956-02
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
B-PP23A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2023
Supervised By : Ankita Jodhani 08/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 06:33:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

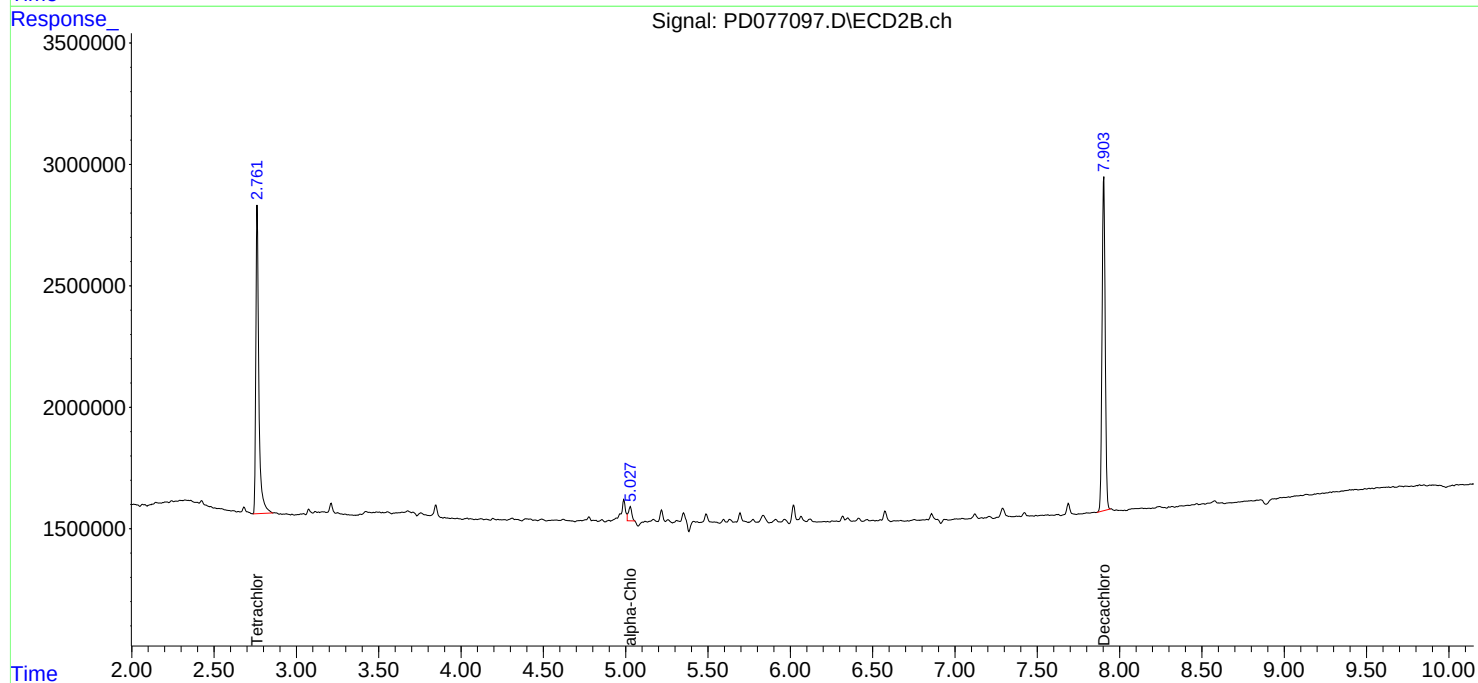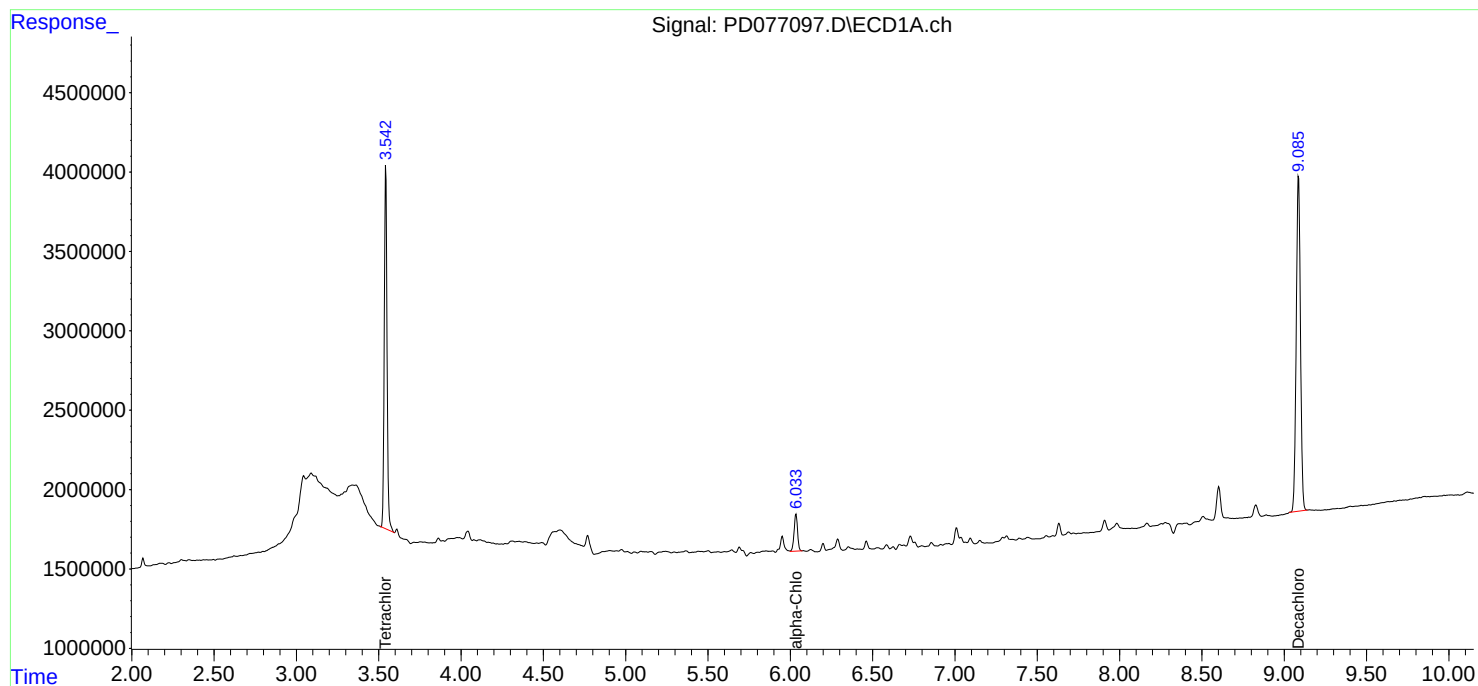

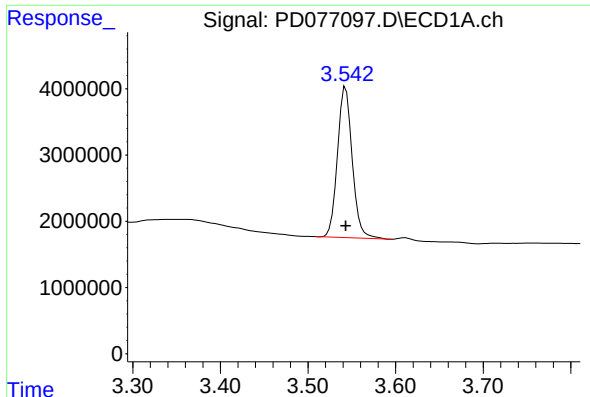


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 26684261
Conc: 11.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
B-PP23A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

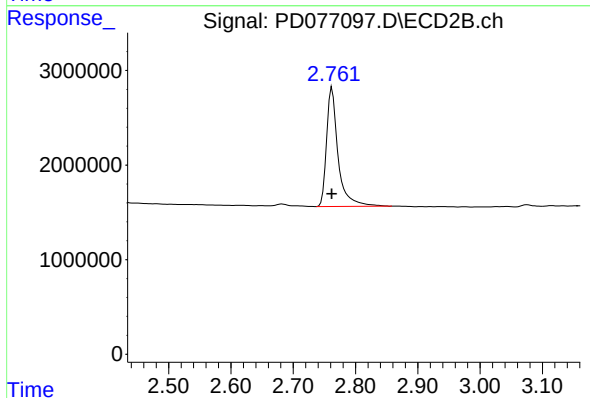


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 16160273
Conc: 11.86 ng/ml

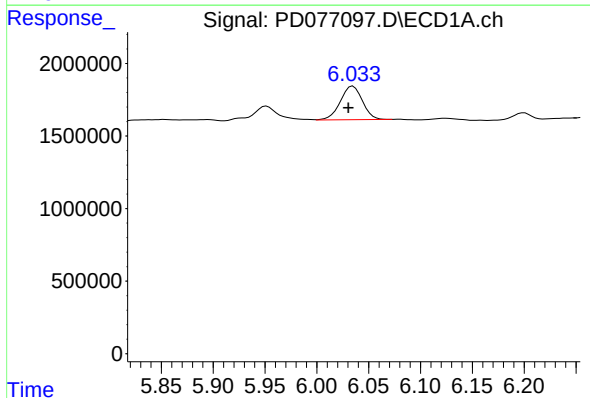


#11 alpha-Chlordane

R.T.: 6.035 min
Delta R.T.: 0.005 min
Response: 3432406
Conc: 1.05 ng/ml

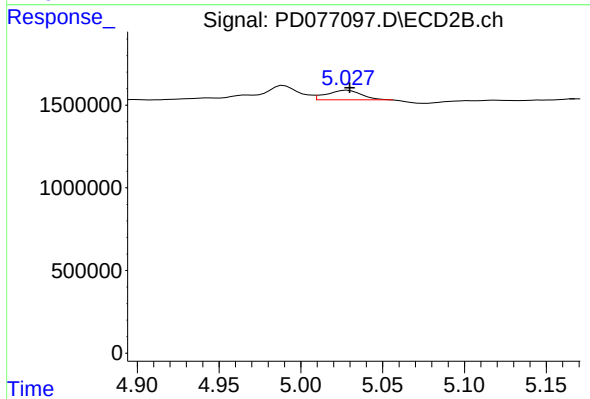

#11 alpha-Chlordane

R.T.: 5.027 min
Delta R.T.: -0.003 min
Response: 838554
Conc: 0.50 ng/ml m

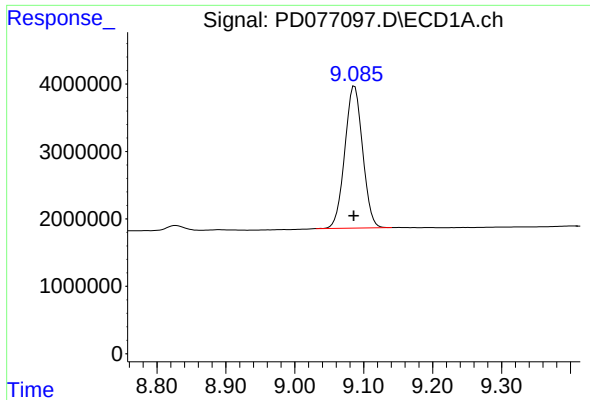


#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: 0.001 min
Response: 37783300
Conc: 13.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
B-PP23A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2023
Supervised By :Ankita Jodhani 08/11/2023

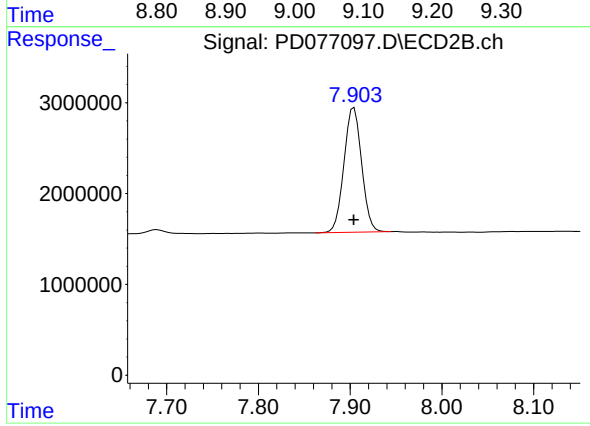

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 18349557
Conc: 12.82 ng/ml