

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081122\
 Data File : PD071523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 11:09
 Operator : AR\AJ
 Sample : N4015-01
 Misc : PEST MDL 1 PPB
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2022-05

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/12/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 05:54:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.807	3.565	49963728	566.9E6	17.515	17.296
27)	SA Decachlor...	8.002	9.093	99047802	353.1E6	35.278	36.837
Target Compounds							
2)	A alpha-BHC	3.316	4.031	3481602	43580344	0.846	1.032
3)	MA gamma-BHC...	3.650	4.367	3203940	38316003	0.814	1.090 #
4)	MA Heptachlor	3.995	4.944	3553696	29072228	0.874m	1.130 #
5)	MB Aldrin	4.280	5.287	3431847	23736893	0.828	1.061 #
6)	B beta-BHC	3.947	4.573	1557146	16806442	0.880m	1.164 #
7)	B delta-BHC	4.182	4.821	3068924	23381986	0.773	0.834
8)	B Heptachlo...	4.788	5.719	3314470	22468980	0.869	1.129 #
9)	A Endosulfan I	5.160	6.106	3097981	17522286	0.910m	1.087
10)	B trans-Chl...	5.041	5.973	3424369	17884820	0.861	0.978
11)	B cis-Chlor...	5.104	6.051	3413962	17924383	0.877m	1.003
12)	B 4,4'-DDE	5.296	6.223	2858770	17360638	0.804	1.103 #
13)	MA Dieldrin	5.429	6.384	3251141	18741480	0.857	1.131 #
14)	MA Endrin	5.705	6.616	2968412	13949228	0.905	1.099
15)	B Endosulfa...	6.000	6.841	3128594	14063088	1.003	1.076m
16)	A 4,4'-DDD	5.853	6.748	2382401	12959449	0.876m	1.064
17)	MA 4,4'-DDT	6.109	7.060	1754198	12206356	0.621	1.032 #
18)	B Endrin al...	6.183	6.974	2606102	11377171	0.972	1.035
19)	B Endosulfa...	6.406	7.206	2885125	12763903	0.938	1.041
20)	A Methoxychlor	6.689	7.536	1240950	6152119	0.860	1.170 #
21)	B Endrin ke...	6.916	7.698	1981598	13998702	0.580	1.067 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081122\
Data File : PD071523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 11:09
Operator : AR\AJ
Sample : N4015-01
Misc : PEST MDL 1 PPB
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 05:54:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

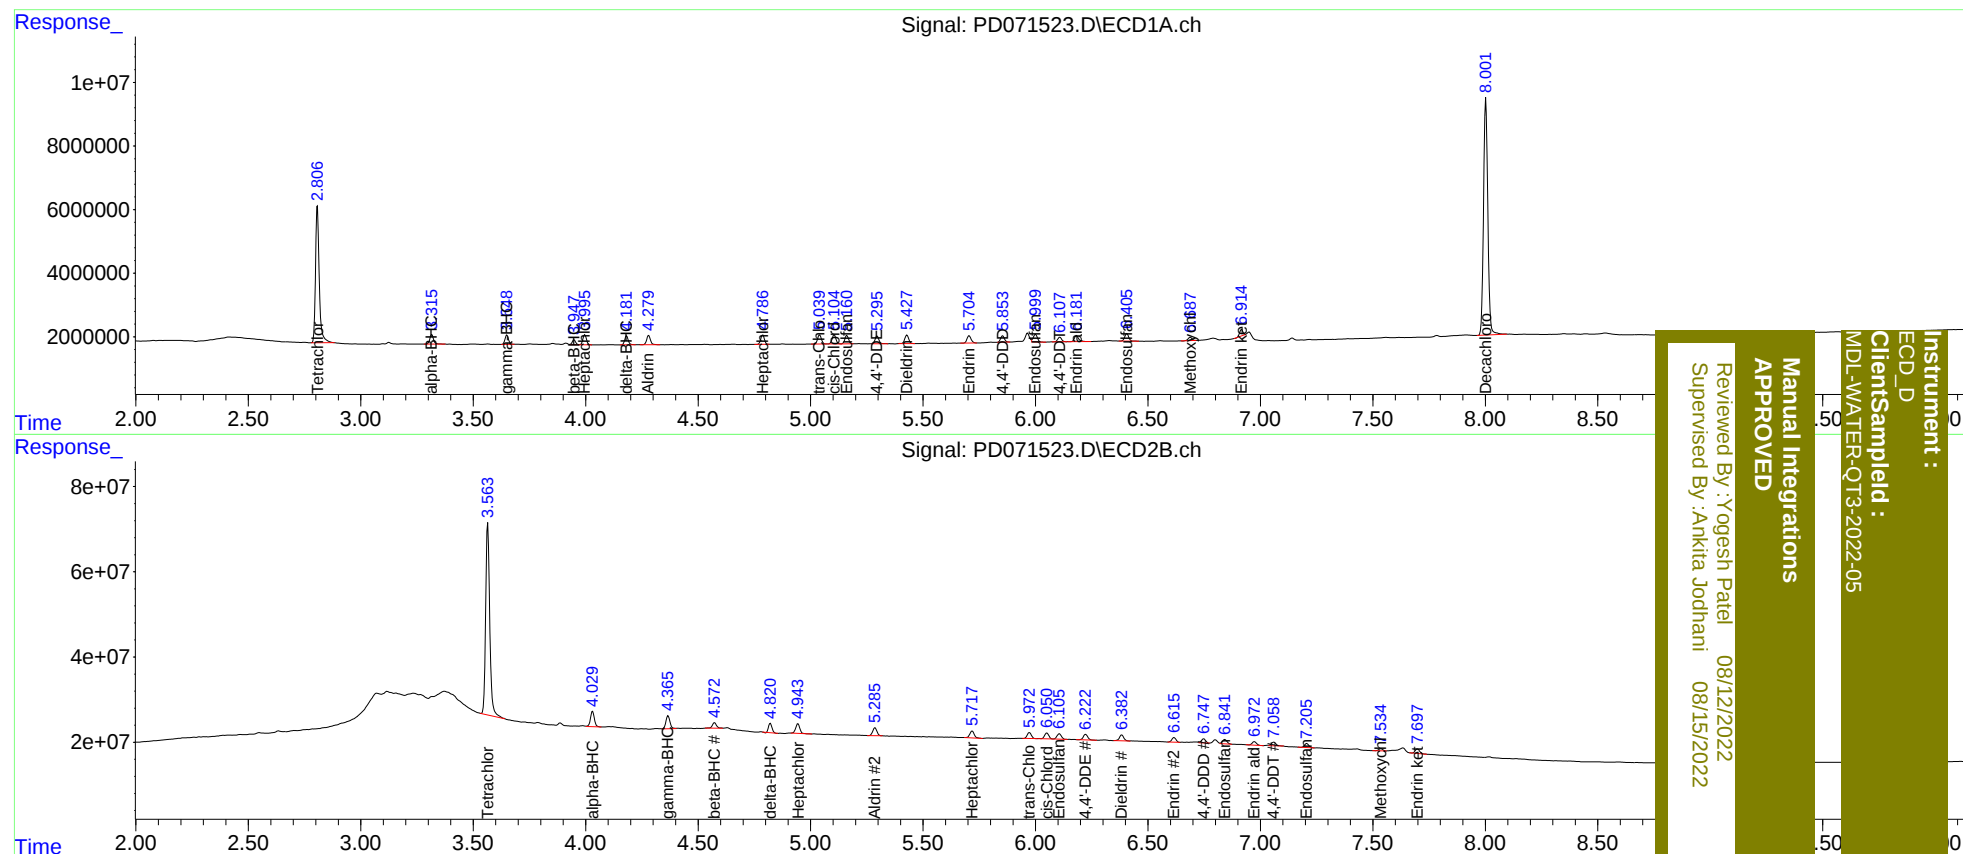

Reviewed By : Yogesh Patel 08/12/2022
Supervised By : Ankita Jodhani 08/15/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT3-2022-05