

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
 Data File : PD077107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 13:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:09:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.762	50073297	28903116	21.159	21.219
28)	SA Decachlor...	9.089	7.905	63275048	28817584	23.092	20.137
Target Compounds							
4)	MA Heptachlor	4.914	0.000	343236	0	0.095	N.D. #
7)	B delta-BHC	4.768	0.000	1447013	0	0.415	N.D. #
8)	B Heptachlo...	5.692	0.000	2009612	0	0.607	N.D. #
9)	A Endosulfan I	6.113f	0.000	276063	0	0.091	N.D. #
15)	B Endosulfa...	6.784f	0.000	1659108	0	0.521	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
Data File : PD077107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 13:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:09:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

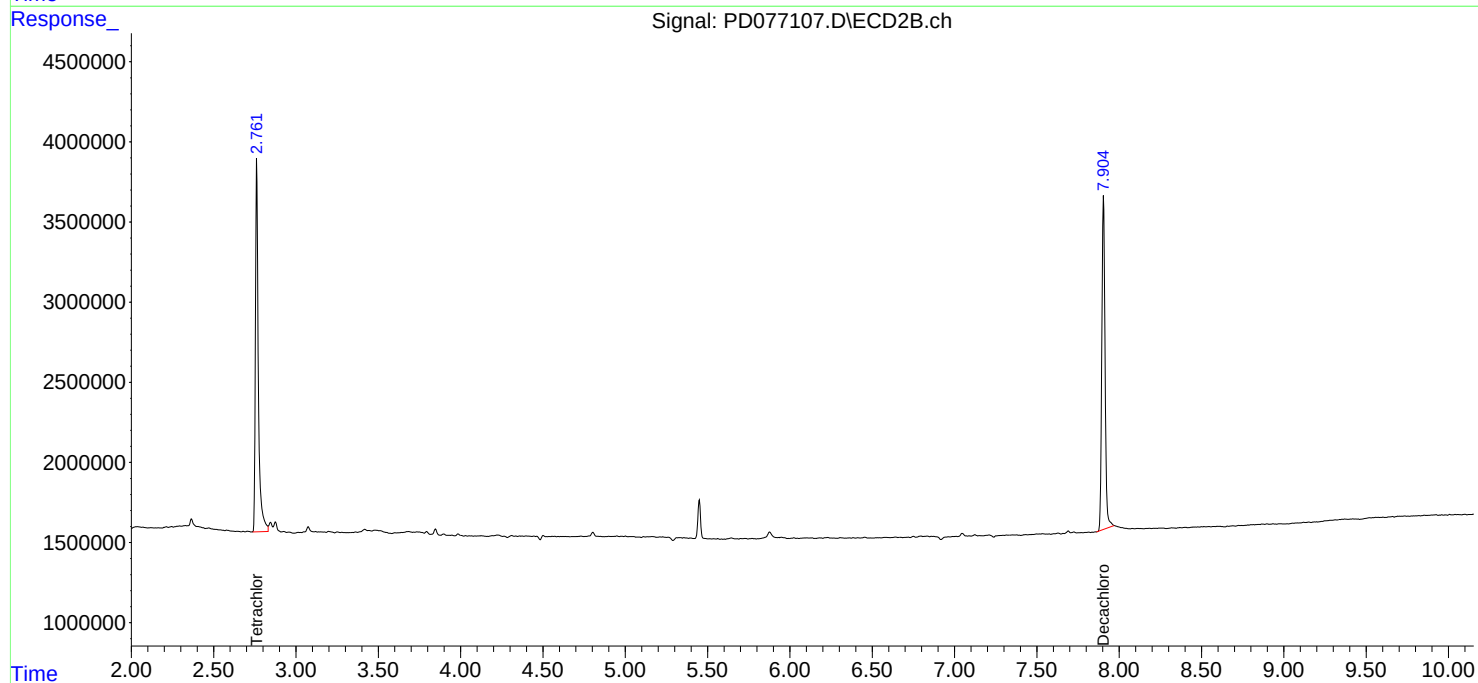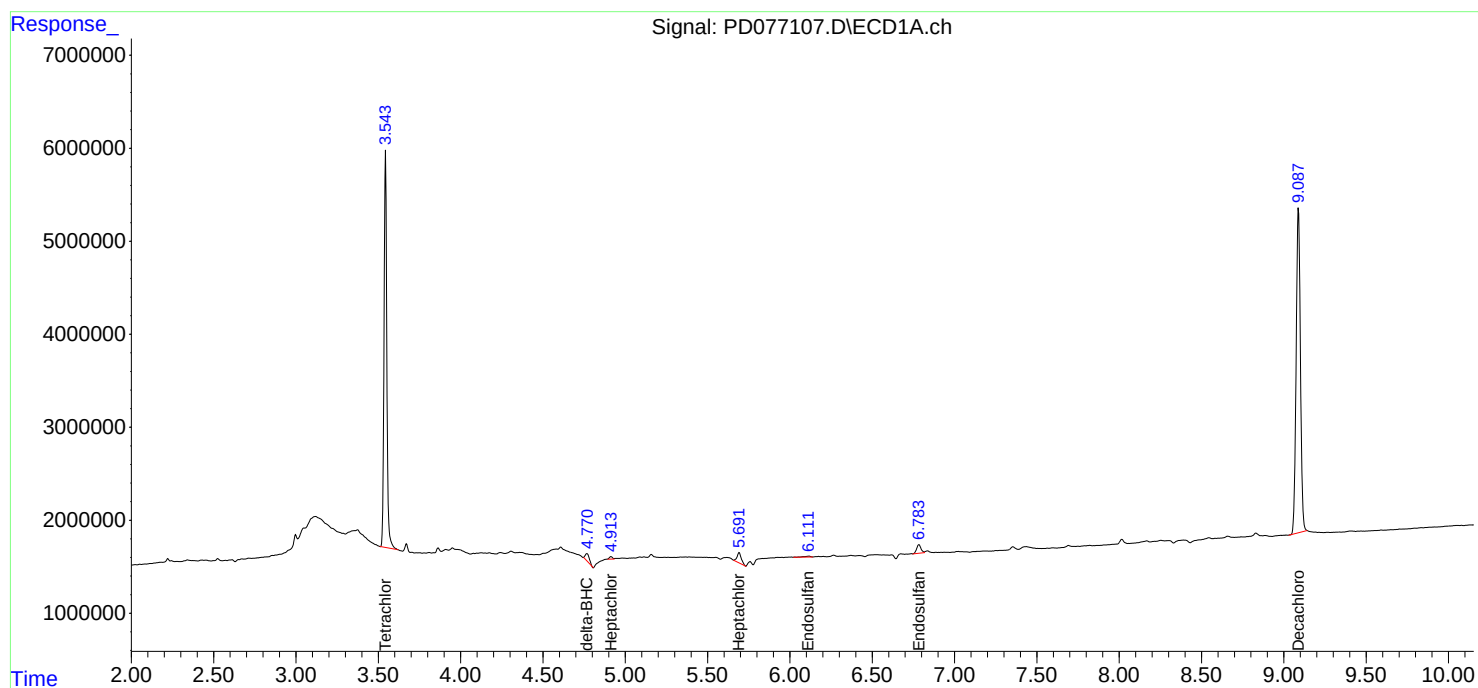


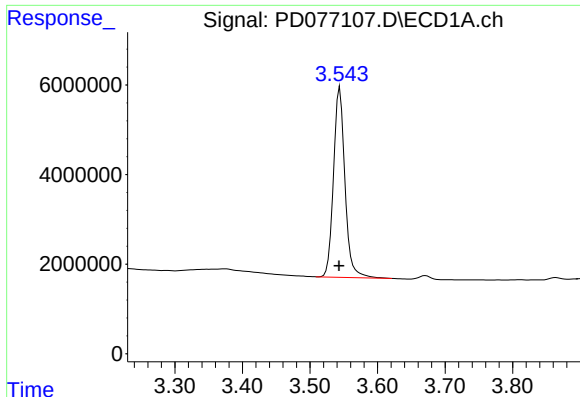

#1 Tetrachloro-m-xylene


R.T.: 3.544 min
Delta R.T.: 0.001 min
Response: 50073297
Conc: 21.16 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

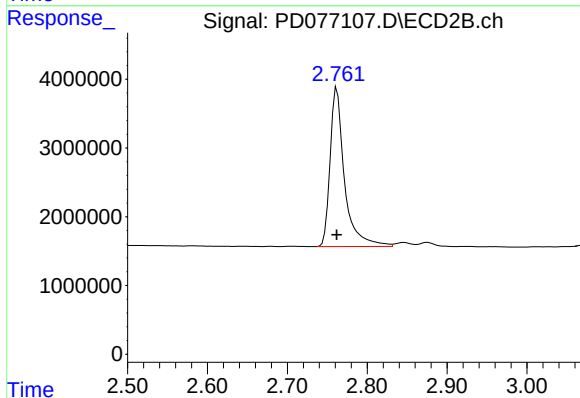


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 28903116
Conc: 21.22 ng/ml

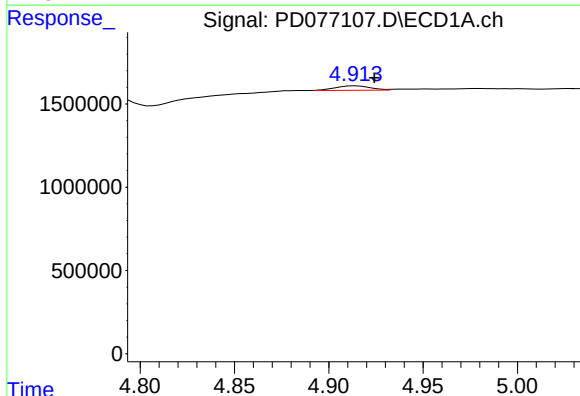


#4 Heptachlor

R.T.: 4.914 min
Delta R.T.: -0.010 min
Response: 343236
Conc: 0.10 ng/ml

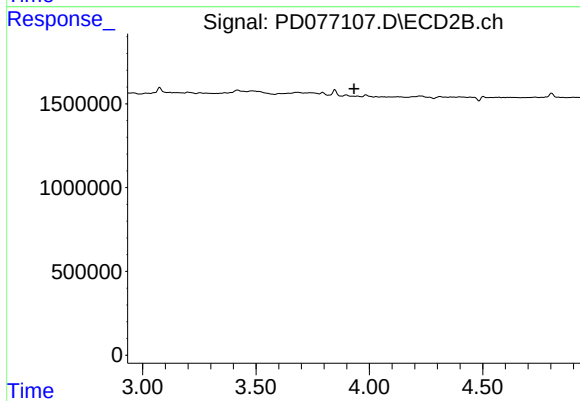

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.933 min
Response: 0
Conc: N.D.

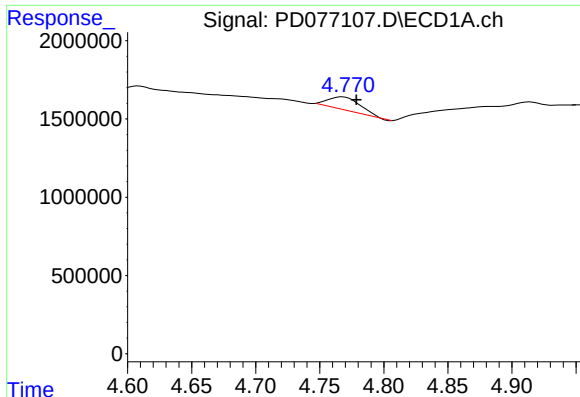

#7 delta-BHC


R.T.: 4.768 min
Delta R.T.: -0.010 min
Response: 1447013
Conc: 0.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

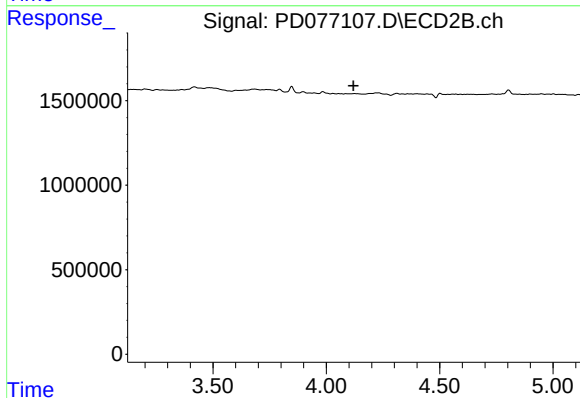


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

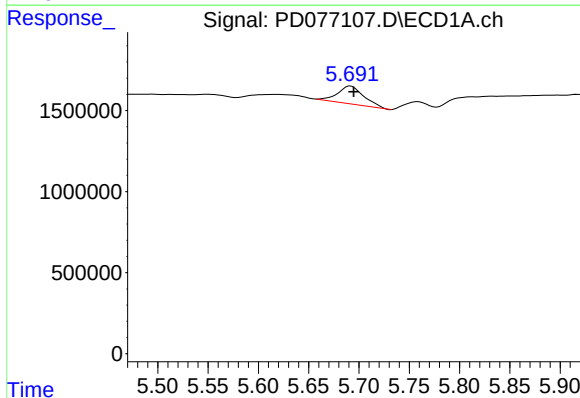


#8 Heptachlor epoxide

R.T.: 5.692 min
Delta R.T.: -0.003 min
Response: 2009612
Conc: 0.61 ng/ml

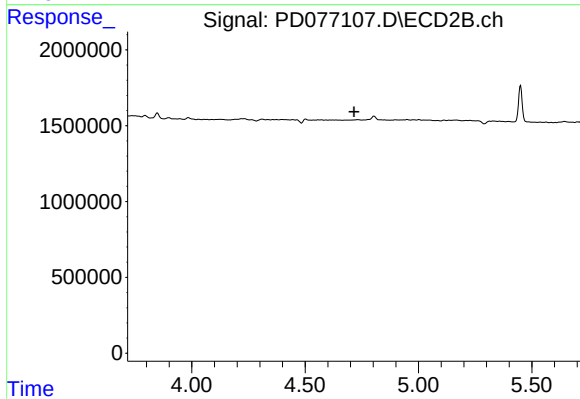

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

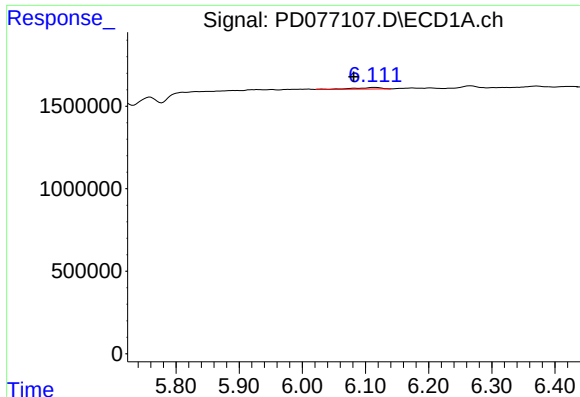

#9 Endosulfan I


R.T.: 6.113 min
Delta R.T.: 0.032 min
Response: 276063
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

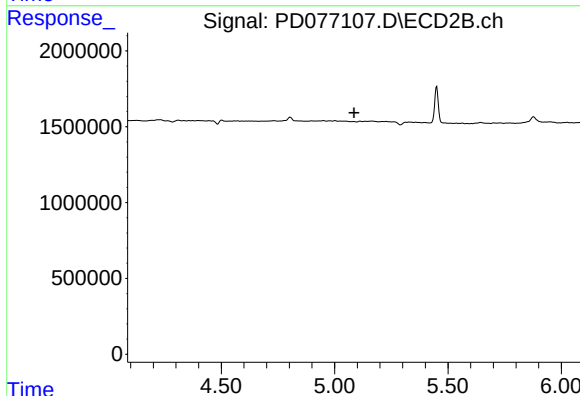


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

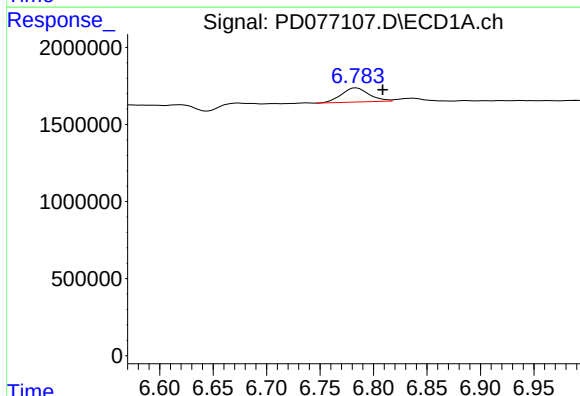


#15 Endosulfan II

R.T.: 6.784 min
Delta R.T.: -0.025 min
Response: 1659108
Conc: 0.52 ng/ml

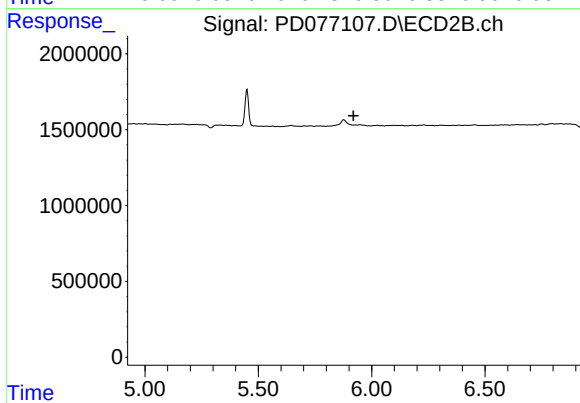

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

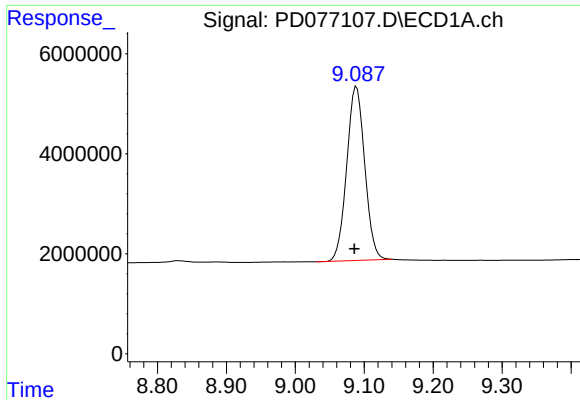

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.003 min
Response: 63275048
Conc: 23.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

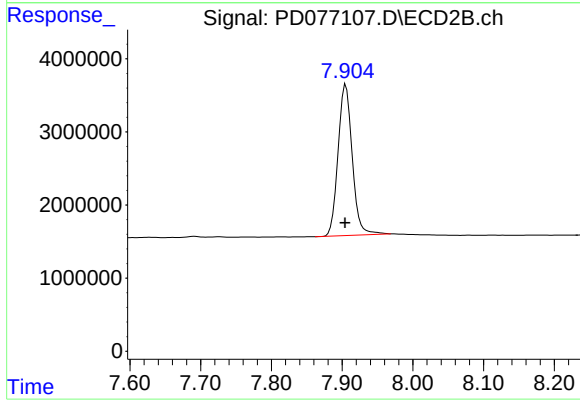

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.001 min
Response: 28817584
Conc: 20.14 ng/ml