

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
 Data File : PD077119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 17:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:16:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 14:17:41 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	2.762	45118188	28670985	19.065	21.049
28)	SA Decachlor...	9.086	7.904	55384832	26251846	20.212	18.344
Target Compounds							
4)	MA Heptachlor	4.911	0.000	273668	0	0.076	N.D. #
6)	B beta-BHC	4.559f	0.000	630480	0	0.419	N.D. #
7)	B delta-BHC	4.768	0.000	1227661	0	0.352	N.D. #
8)	B Heptachlo...	5.690	0.000	1880807	0	0.568	N.D. #
9)	A Endosulfan I	6.111f	0.000	323437	0	0.106	N.D. #
13)	MA Dieldrin	6.372	0.000	389791	0	0.119	N.D. #
15)	B Endosulfa...	6.782f	0.000	770027	0	0.242	N.D. #
21)	B Endrin ke...	7.692f	0.000	419441	0	0.139	N.D. #
24)	Chlordane-2	0.000	4.346	0	394089	N.D.	7.008 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
Data File : PD077119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 17:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:16:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 14:17:41 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

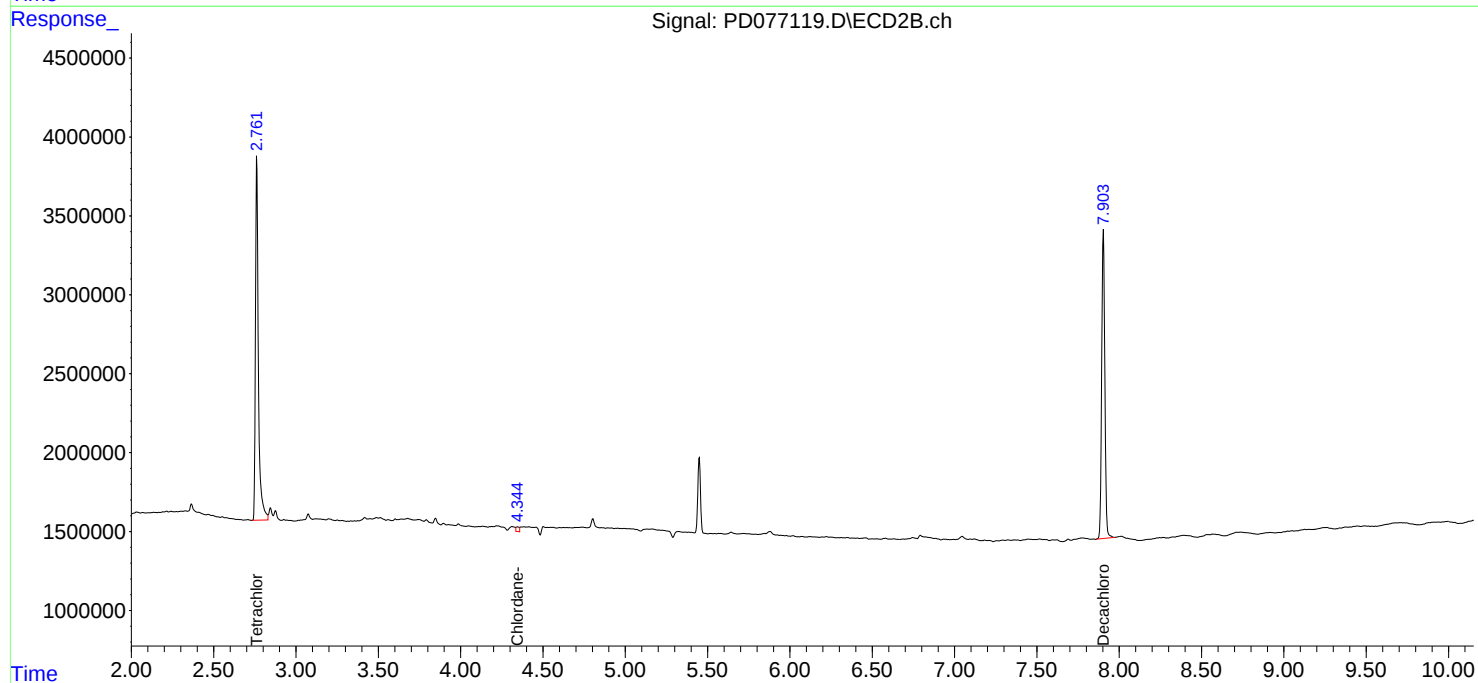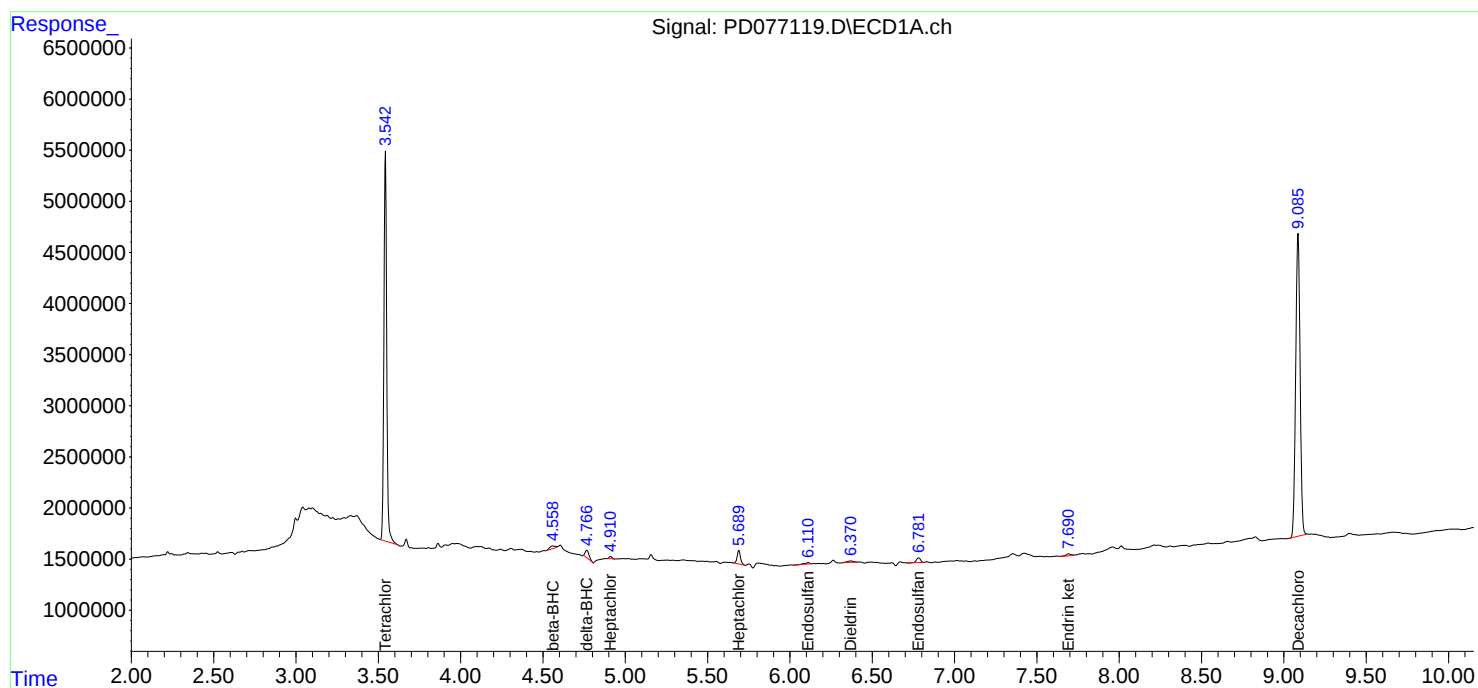


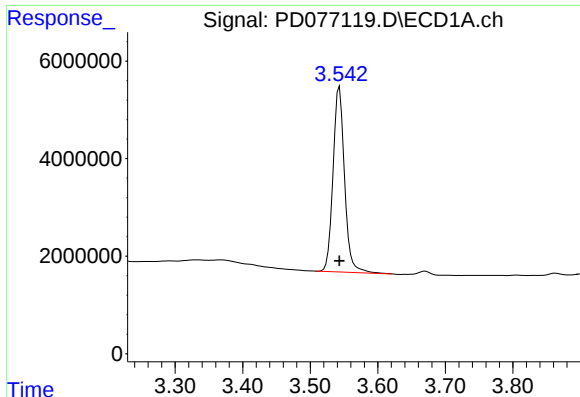

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 45118188
Conc: 19.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

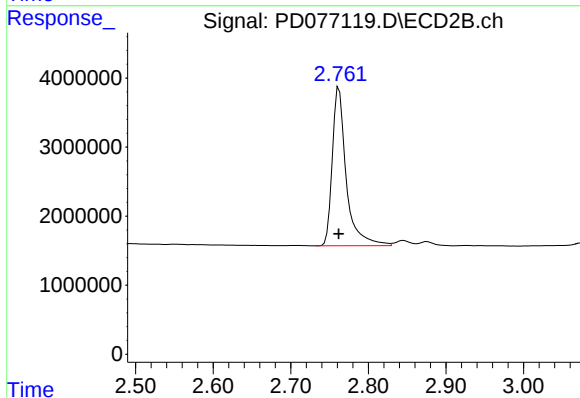


#1 Tetrachloro-m-xylene

R.T.: 2.762 min
Delta R.T.: 0.000 min
Response: 28670985
Conc: 21.05 ng/ml

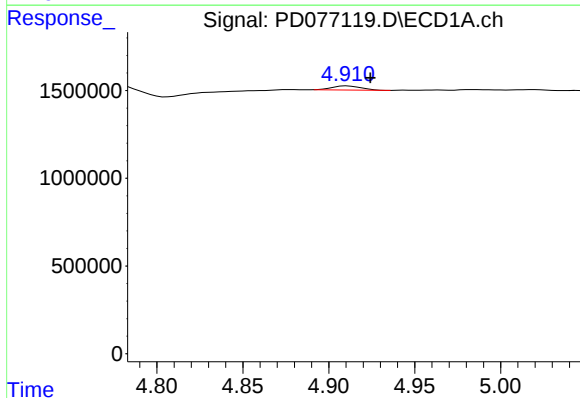


#4 Heptachlor

R.T.: 4.911 min
Delta R.T.: -0.013 min
Response: 273668
Conc: 0.08 ng/ml

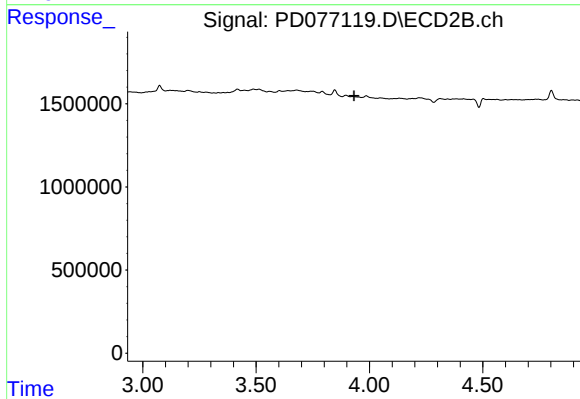

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.933 min
Response: 0
Conc: N.D.

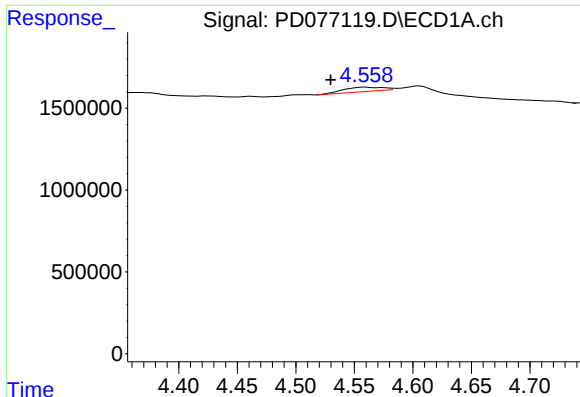

#6 beta-BHC


R.T.: 4.559 min
Delta R.T.: 0.029 min
Response: 630480
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

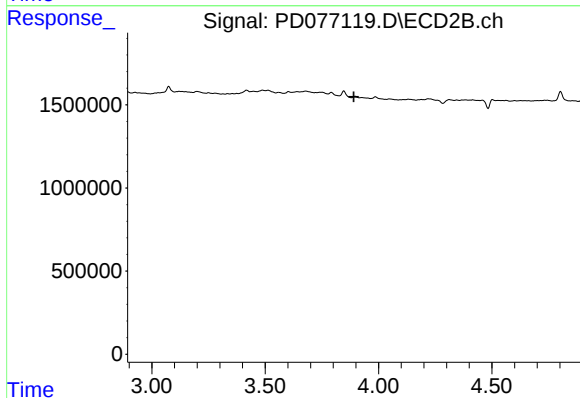


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.890 min
Response: 0
Conc: N.D.

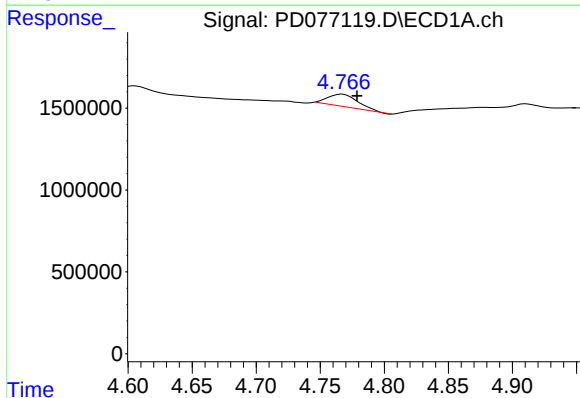


#7 delta-BHC

R.T.: 4.768 min
Delta R.T.: -0.011 min
Response: 1227661
Conc: 0.35 ng/ml

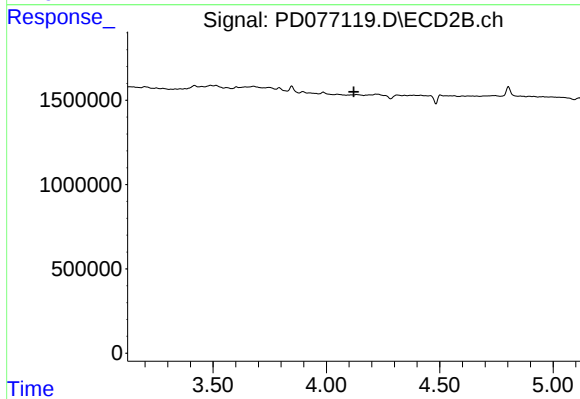

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.120 min
Response: 0
Conc: N.D.

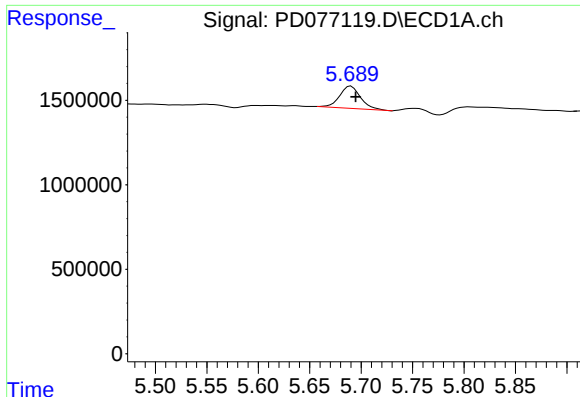

#8 Heptachlor epoxide


R.T.: 5.690 min
Delta R.T.: -0.005 min
Response: 1880807
Conc: 0.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

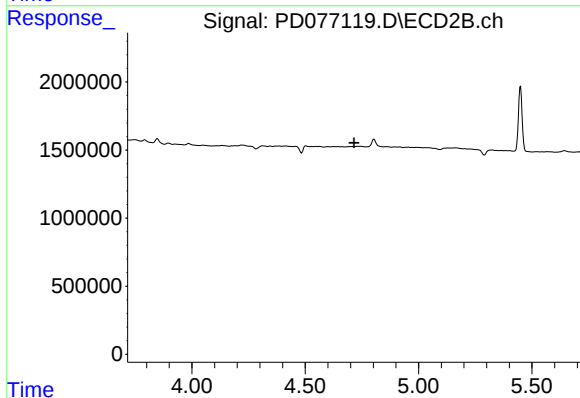


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.716 min
Response: 0
Conc: N.D.

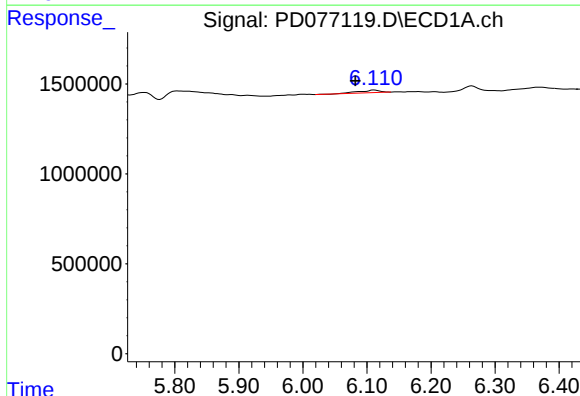


#9 Endosulfan I

R.T.: 6.111 min
Delta R.T.: 0.030 min
Response: 323437
Conc: 0.11 ng/ml

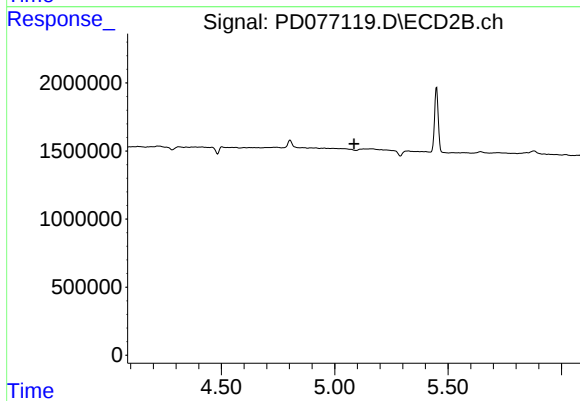

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.086 min
Response: 0
Conc: N.D.

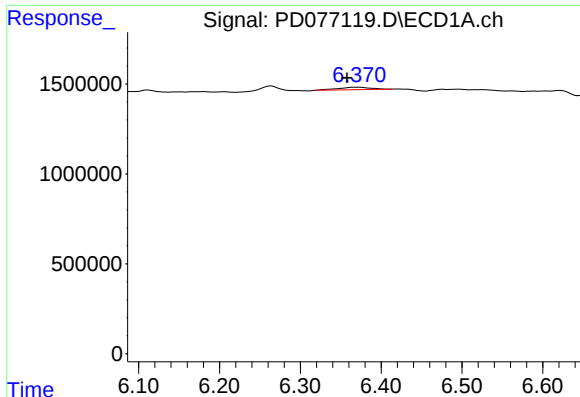

#13 Dieldrin


R.T.: 6.372 min
Delta R.T.: 0.014 min
Response: 389791
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

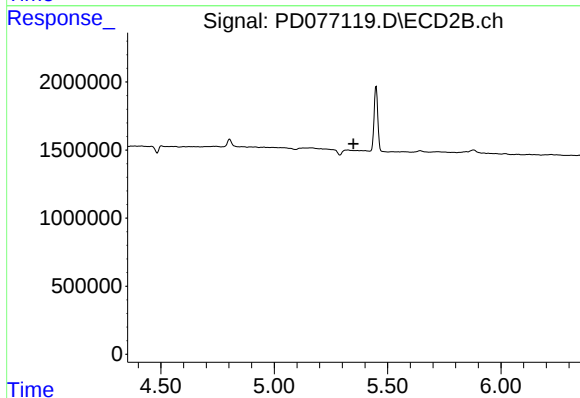


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

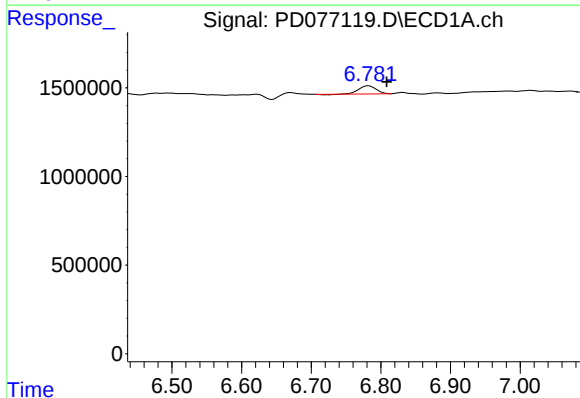


#15 Endosulfan II

R.T.: 6.782 min
Delta R.T.: -0.026 min
Response: 770027
Conc: 0.24 ng/ml

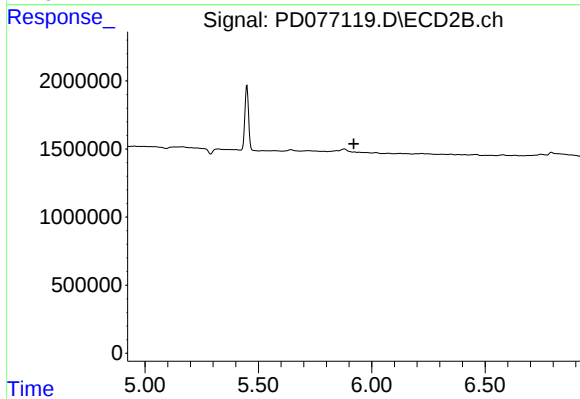

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.920 min
Response: 0
Conc: N.D.

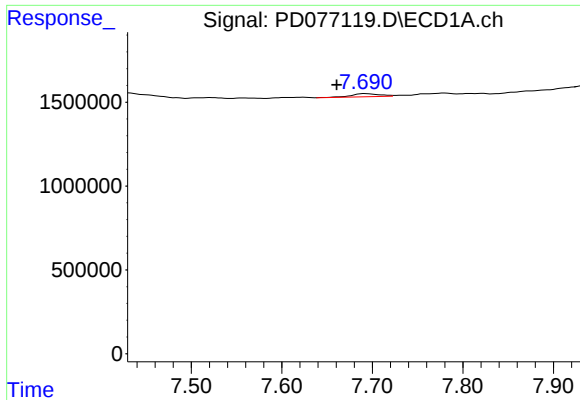

#21 Endrin ketone


R.T.: 7.692 min
Delta R.T.: 0.032 min
Response: 419441
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

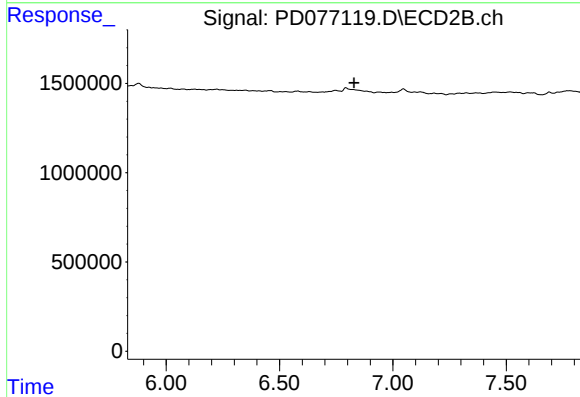


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

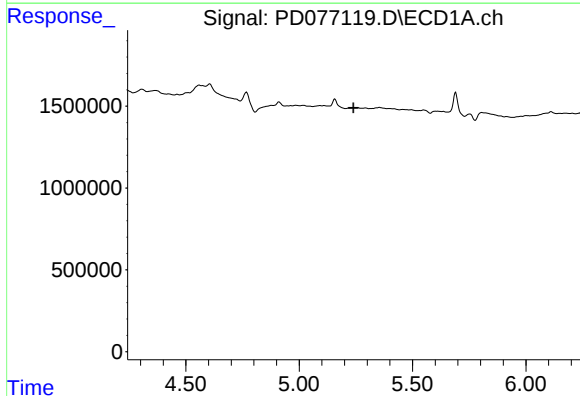


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.240 min
Response: 0
Conc: N.D.

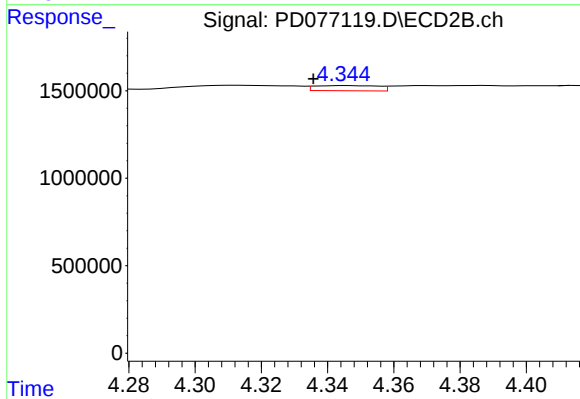

#24 Chlordane-2


R.T.: 4.346 min
Delta R.T.: 0.010 min
Response: 394089
Conc: 7.01 ng/ml

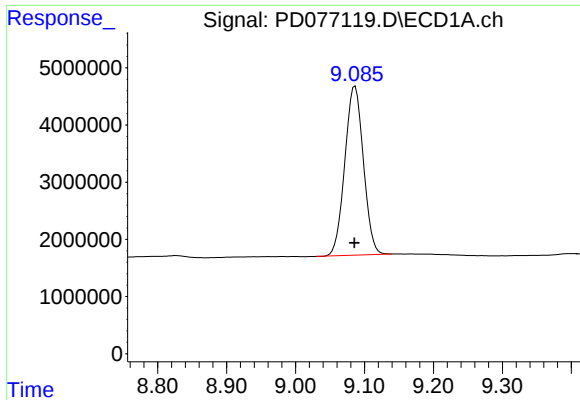

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 55384832
Conc: 20.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

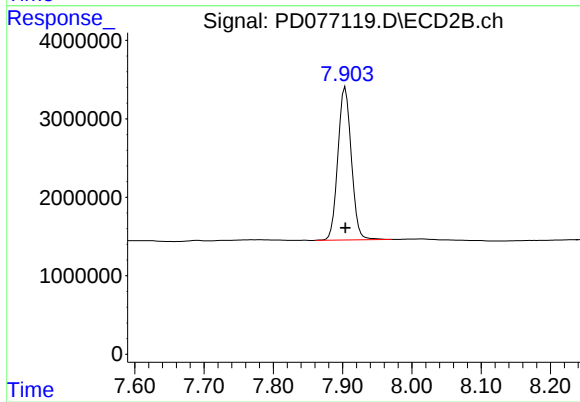

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: 0.000 min
Response: 26251846
Conc: 18.34 ng/ml