

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
 Data File : PD077106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2023 12:34
 Operator : AR\AJ
 Sample : 03572-09
 Misc : TOX MDL 50PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-03-QT3-2023

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/14/2023
 Supervised By :Ankita Jodhani 08/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:34:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX080323.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 03 15:26:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.762	41236381	24349095	17.900	18.240
7) SA Decachlor...	9.095	7.907	56723976	24849427	20.805	18.219
Target Compounds						
2) Toxaphene-1	6.258	4.993	1427764	425340	57.617	46.693
3) Toxaphene-2	7.171	5.676	2680348	441970	45.539	48.591
4) Toxaphene-3	7.269	6.591	1855898	797962	51.600	31.408 #
5) Toxaphene-4	7.594	6.719	2092660	1605954	48.549m	39.215
6) Toxaphene-5	7.959	7.036	1762571	621959	40.904	42.379

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081123\
Data File : PD077106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2023 12:34
Operator : AR\AJ
Sample : 03572-09
Misc : TOX MDL 50PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:34:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX080323.M
Quant Title : GC Extractables
QLast Update : Thu Aug 03 15:26:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

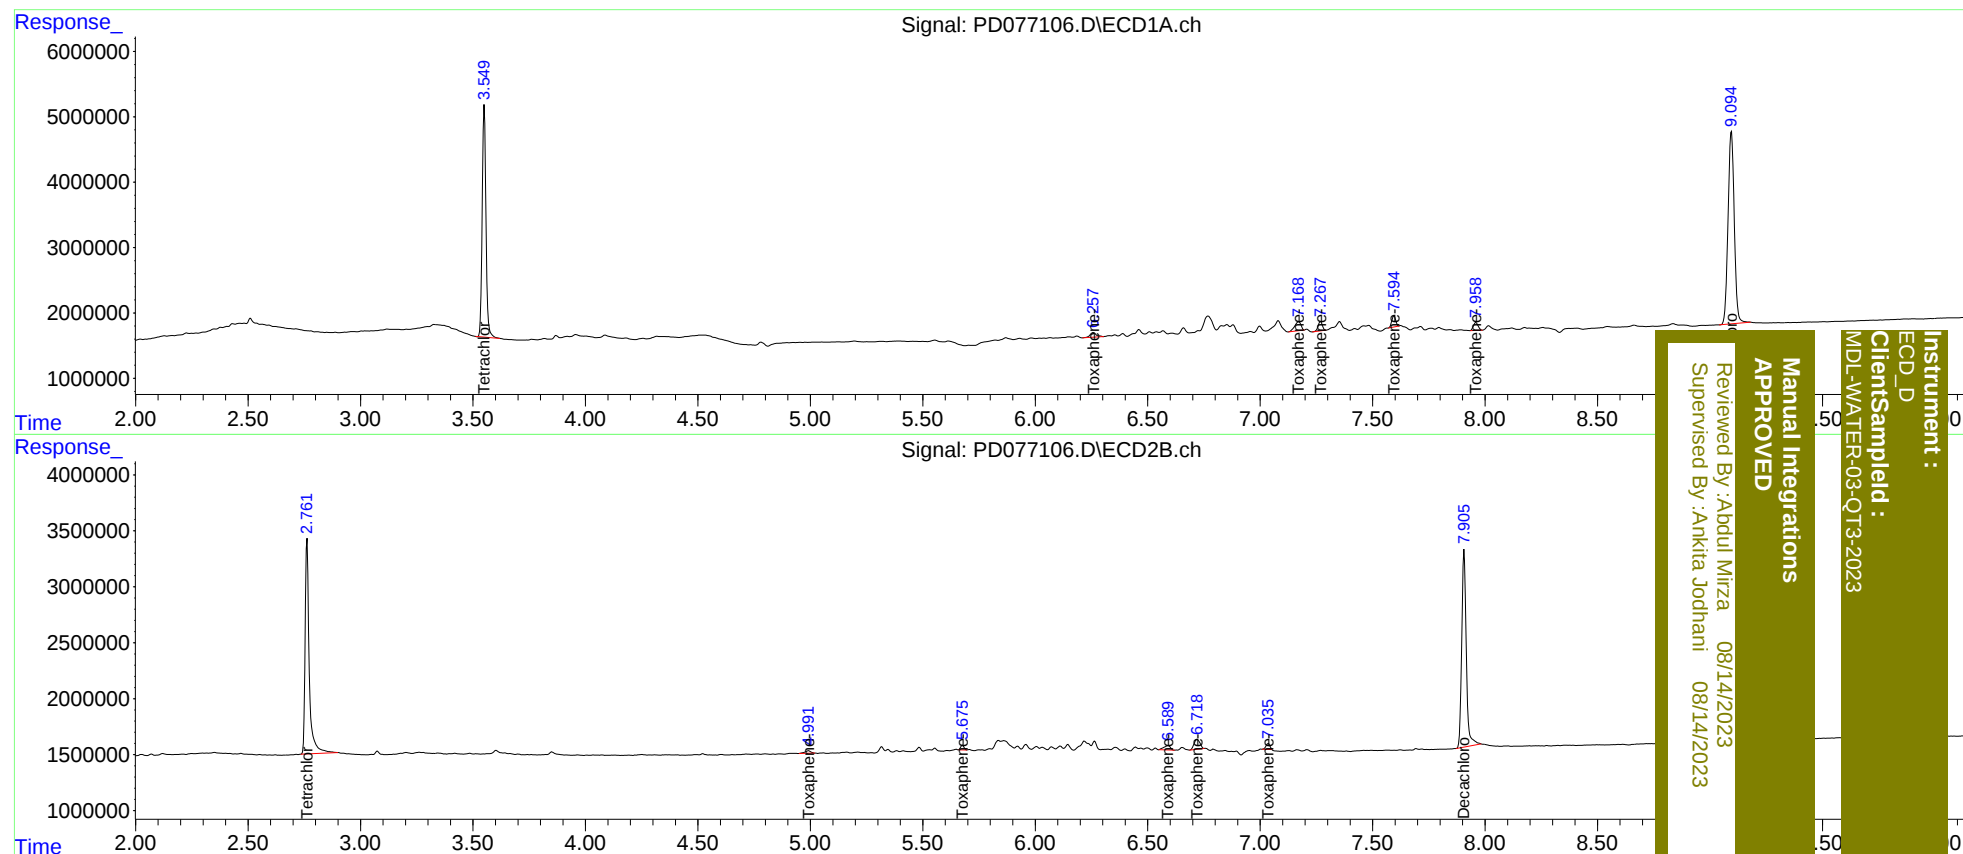

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/14/2023
Supervised By: Ankita Jodhani 08/14/2023

Instrument :
ECD_D
Client Sample :
MDL-WATER-03-QT3-2023