

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081218\
 Data File : PD048844.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2018 11:56
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 08:12:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.377	3.967	31197662	286.5E6	28.141	21.343
28)	SA Decachlor...	8.078	8.996	29956568	327.9E6	21.393	21.714
Target Compounds							
2)	A alpha-BHC	3.810	0.000	5963	0	0.003	N.D. #
10)	B gamma-Chl...	0.000	6.003f	0	4213926	N.D.	0.227 #
14)	MA Endrin	0.000	6.669	0	39275494	N.D.	2.421 #
16)	A 4,4'-DDD	0.000	6.719f	0	13454120	N.D.	1.061 #
17)	MA 4,4'-DDT	6.235	0.000	5504878	0	3.884	N.D. #
19)	B Endosulfa...	6.590f	0.000	561513	0	0.424	N.D. #
20)	A Methoxychlor	6.797	7.545	265448	28197772	0.341	4.674 #
25)	Chlordane-3	0.000	6.003	0	4213926	N.D.	1.729 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081218\
Data File : PD048844.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2018 11:56
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 08:12:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

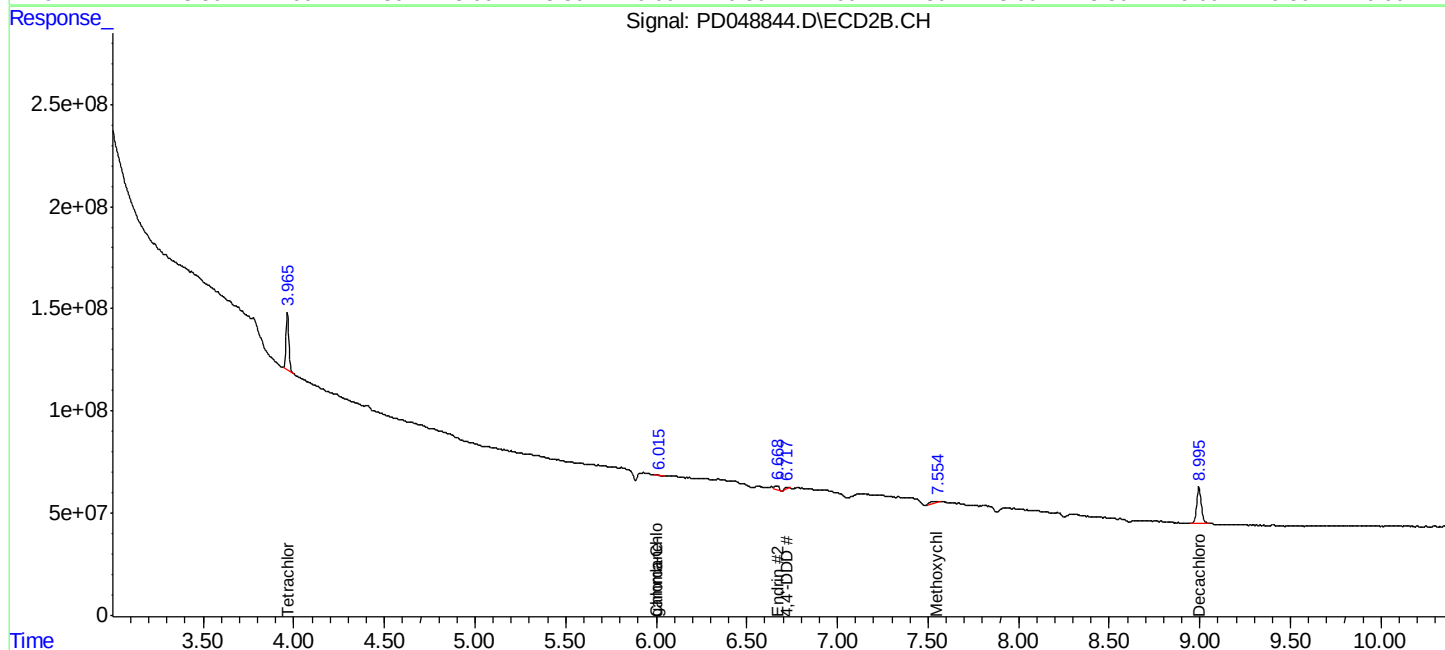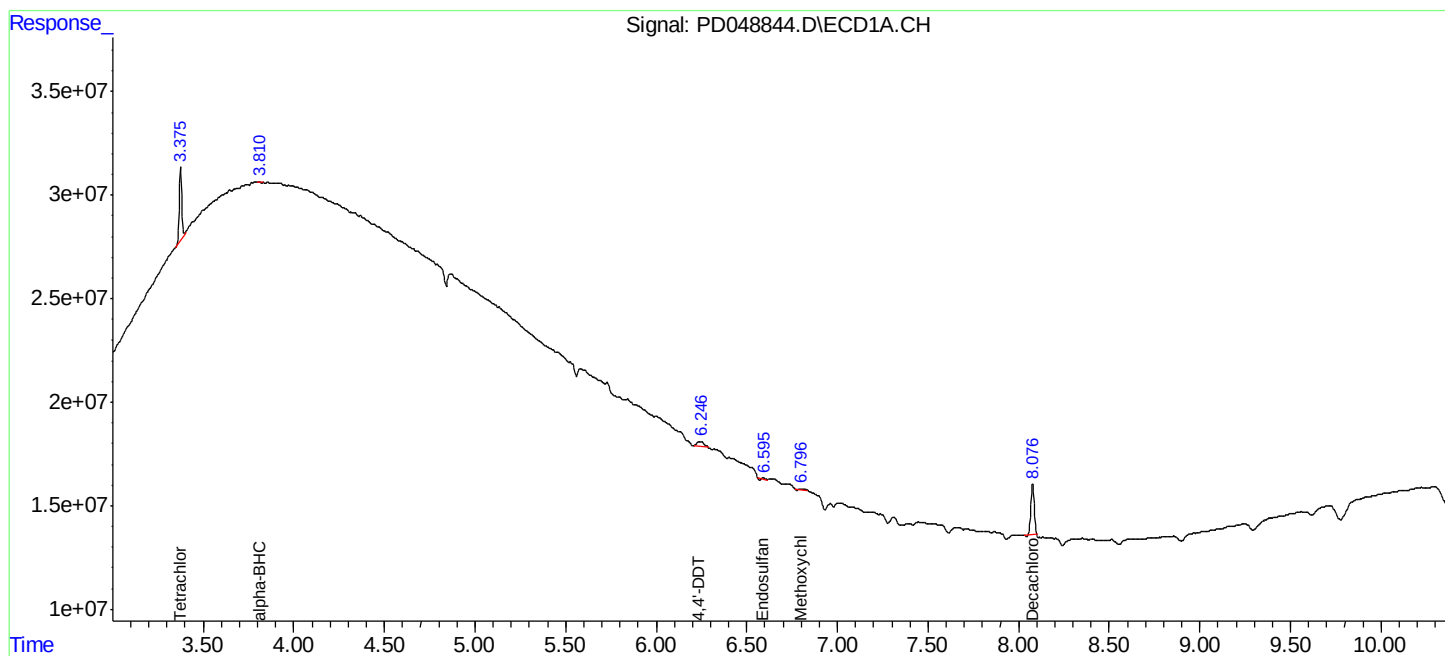


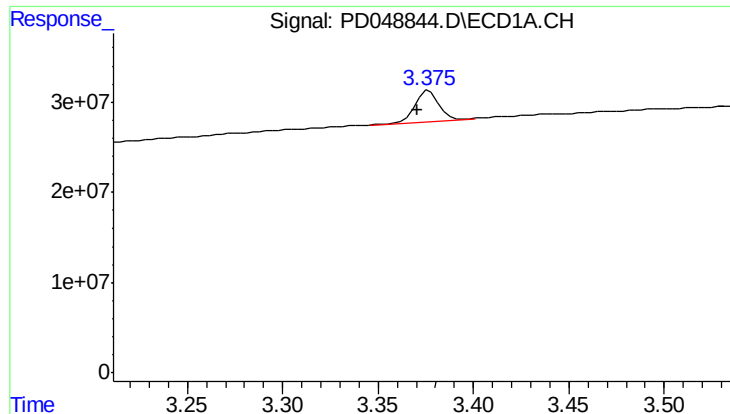

#1 Tetrachloro-m-xylene


R.T.: 3.377 min
Delta R.T.: 0.006 min
Response: 31197662
Conc: 28.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

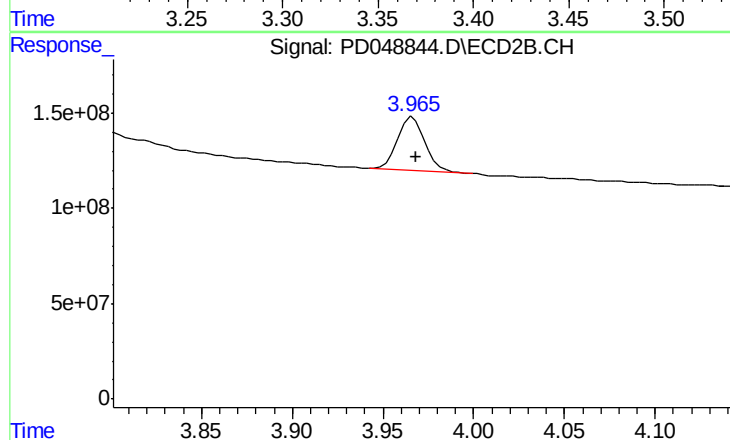


#1 Tetrachloro-m-xylene

R.T.: 3.967 min
Delta R.T.: -0.001 min
Response: 286508055
Conc: 21.34 ng/ml

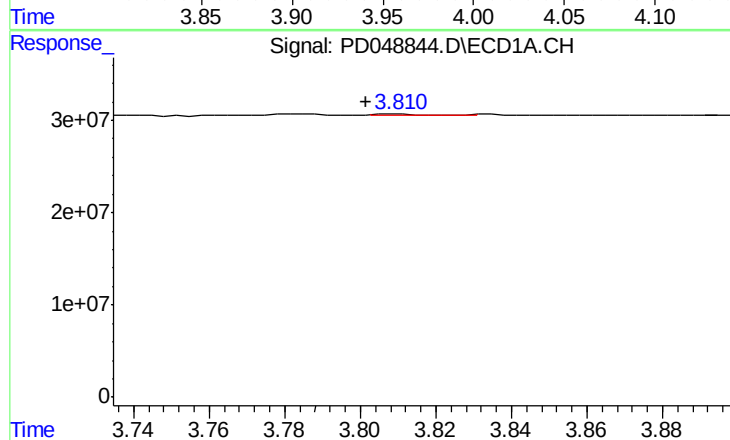


#2 alpha-BHC

R.T.: 3.810 min
Delta R.T.: 0.009 min
Response: 5963
Conc: 0.00 ng/ml

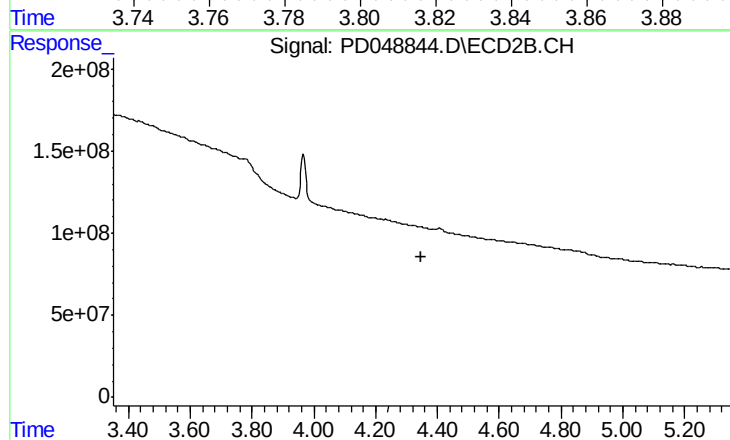

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

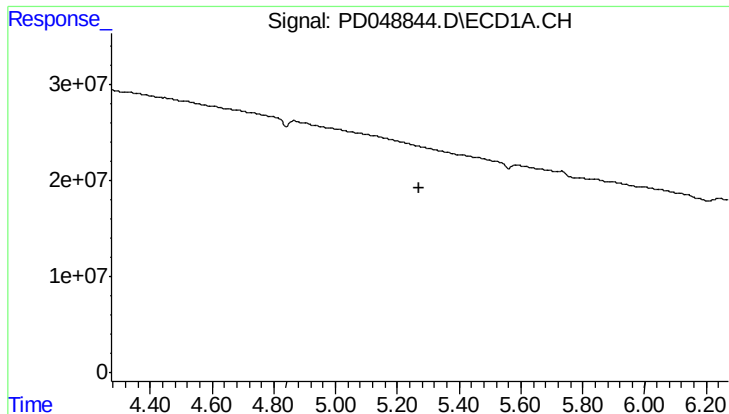

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.272 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

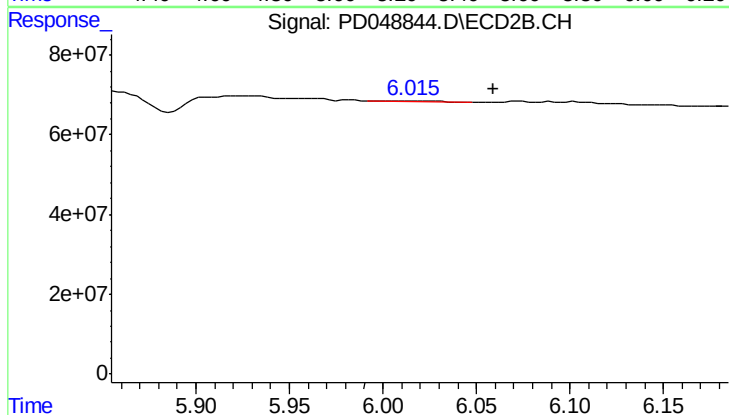


#10 gamma-Chlordane

R.T.: 6.003 min
Delta R.T.: -0.056 min
Response: 4213926
Conc: 0.23 ng/ml

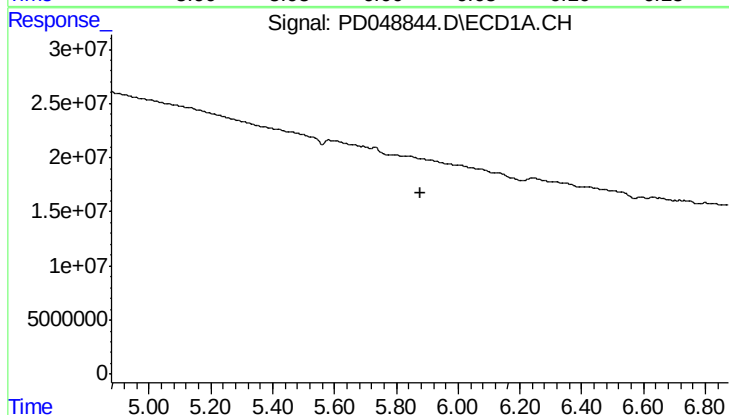


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.878 min
Response: 0
Conc: N.D.

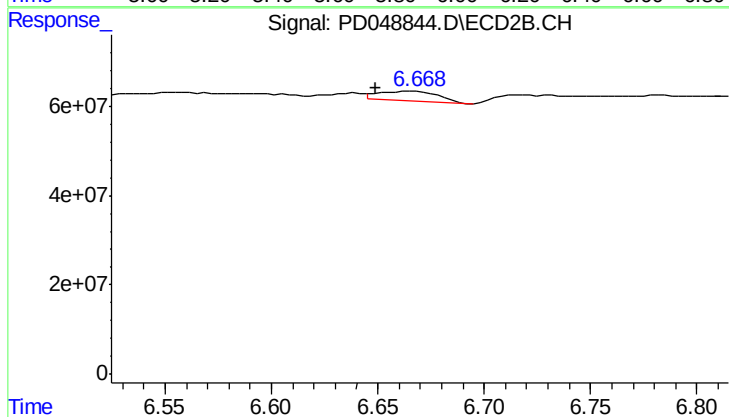

#14 Endrin


R.T.: 6.669 min
Delta R.T.: 0.020 min
Response: 39275494
Conc: 2.42 ng/ml

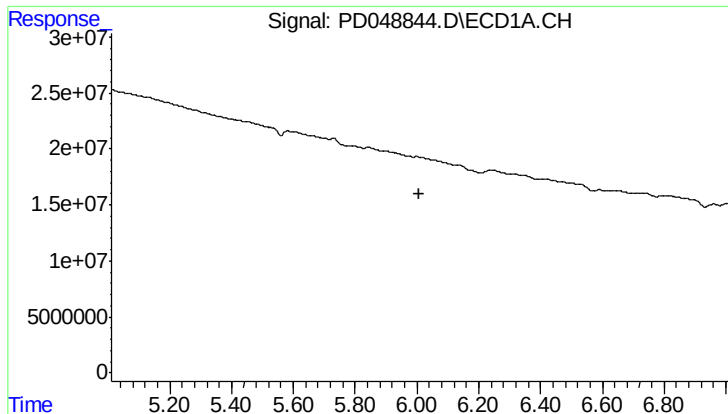

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

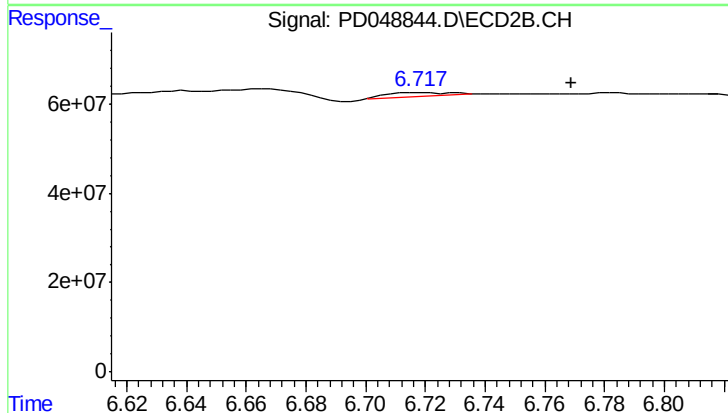


#16 4,4'-DDD

R.T.: 6.719 min
Delta R.T.: -0.050 min
Response: 13454120
Conc: 1.06 ng/ml

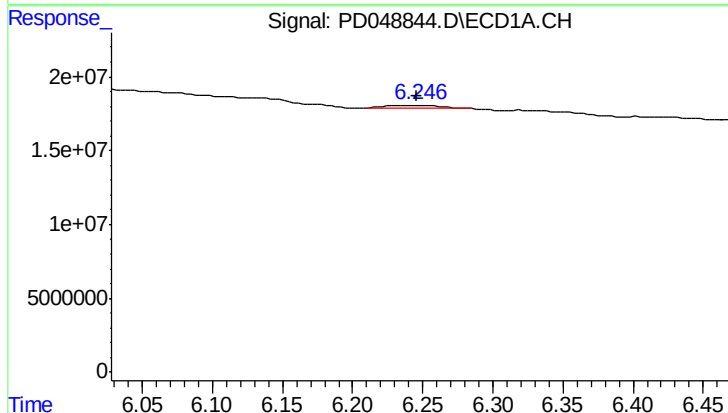


#17 4,4'-DDT

R.T.: 6.235 min
Delta R.T.: -0.011 min
Response: 5504878
Conc: 3.88 ng/ml

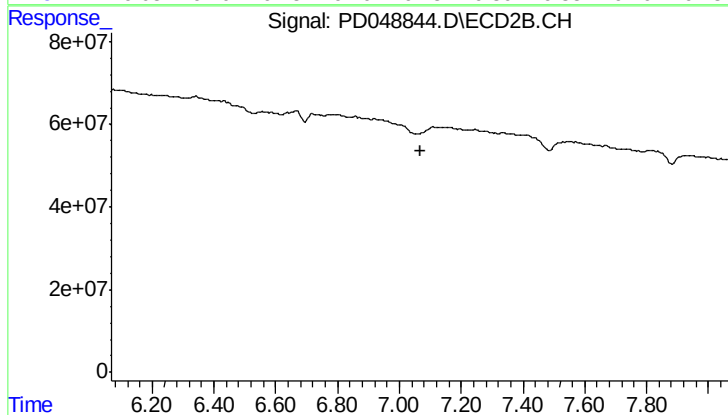

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.067 min
Response: 0
Conc: N.D.

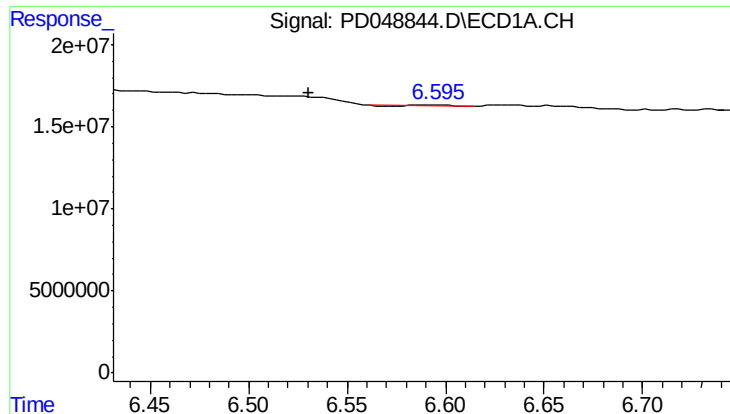

#19 Endosulfan Sulfate


R.T.: 6.590 min
Delta R.T.: 0.059 min
Response: 561513
Conc: 0.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

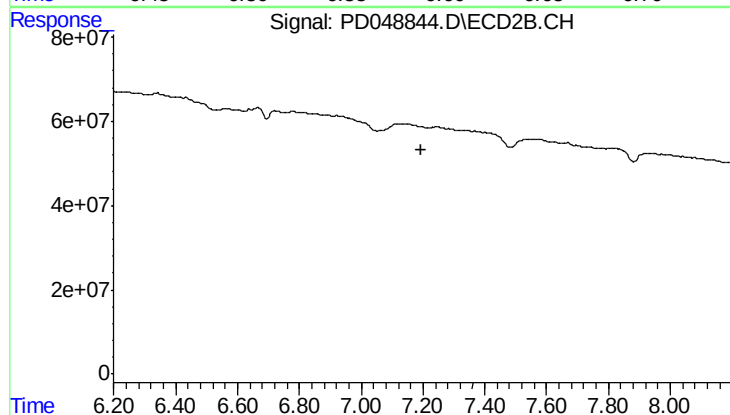


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.196 min
Response: 0
Conc: N.D.

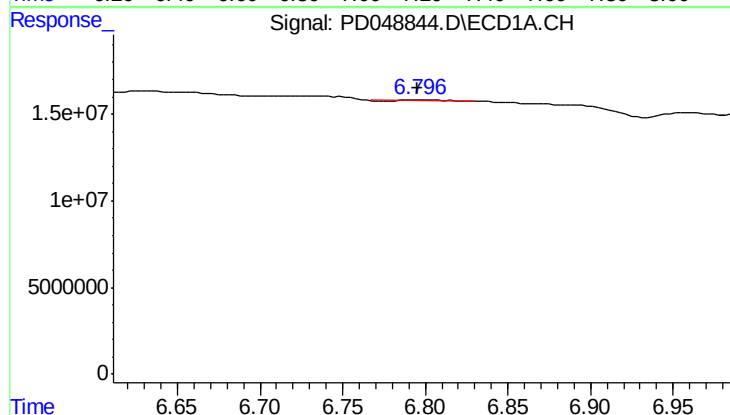


#20 Methoxychlor

R.T.: 6.797 min
Delta R.T.: 0.002 min
Response: 265448
Conc: 0.34 ng/ml

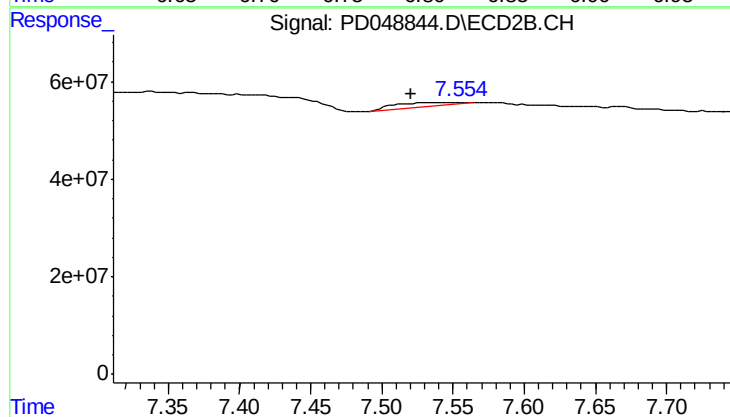

#20 Methoxychlor


R.T.: 7.545 min
Delta R.T.: 0.024 min
Response: 28197772
Conc: 4.67 ng/ml

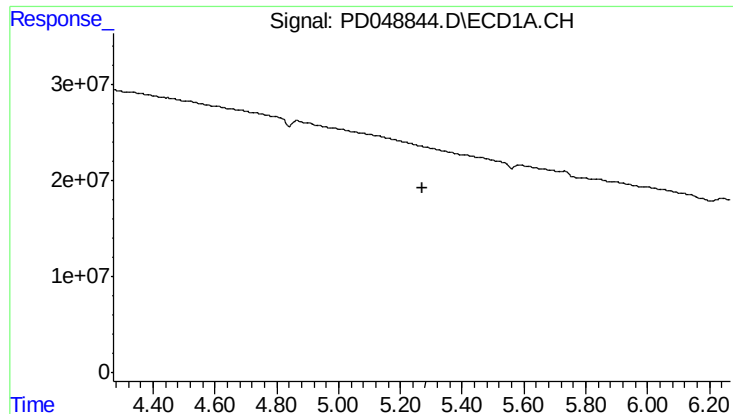

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

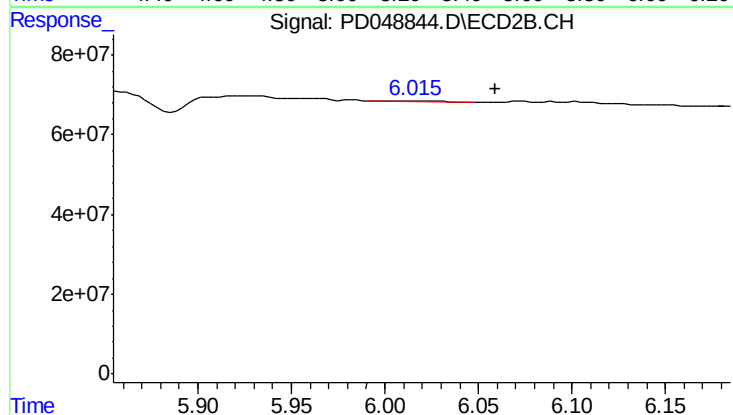


#25 Chlordane-3

R.T.: 6.003 min
Delta R.T.: -0.056 min
Response: 4213926
Conc: 1.73 ng/ml

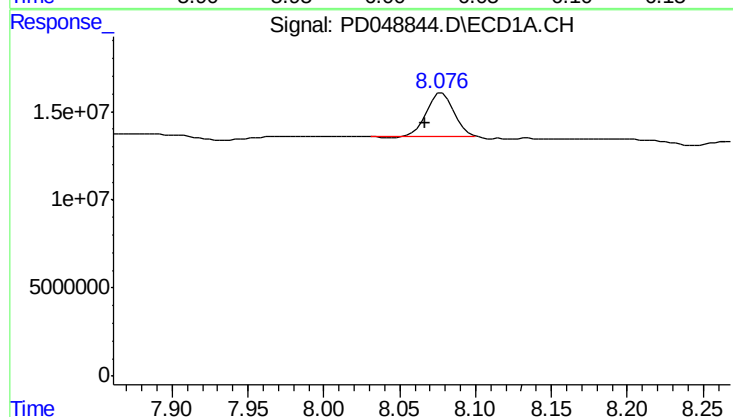

#28 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: 0.011 min
Response: 29956568
Conc: 21.39 ng/ml

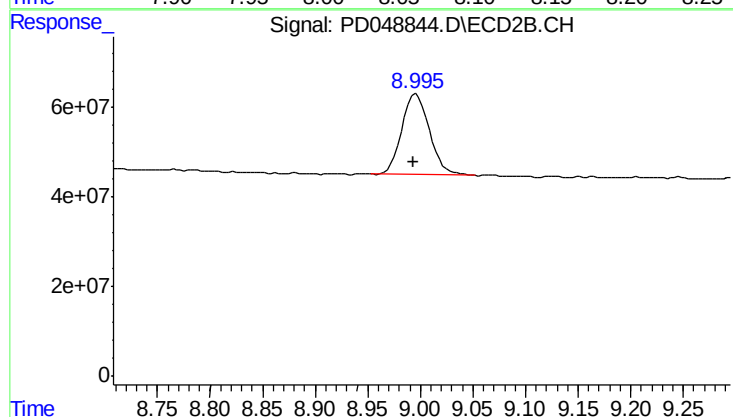

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.002 min
Response: 327939368
Conc: 21.71 ng/ml