

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD D\Data\PD081218\
 Data File : PD048848.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Aug 2018 12:51
 Operator : AJ\SJ
 Sample : J4409-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 2018-NYSEG-CLARK-AREA-9B

Manual Integrations
 APPROVED

Sohil
 8/13/2018 12:40:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 08:38:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.371	3.965	13694816	109.3E6	12.353m	8.143m#
28) SA Decachlor...	8.067	8.994	13937605	177.8E6	9.953	11.774

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081218\
Data File : PD048848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Aug 2018 12:51
Operator : AJ\SJ
Sample : J4409-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
2018-NYSEG-CLARK-AREA-9B


Manual Integrations
APPROVED

Sohil
8/13/2018 12:40:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 08:38:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

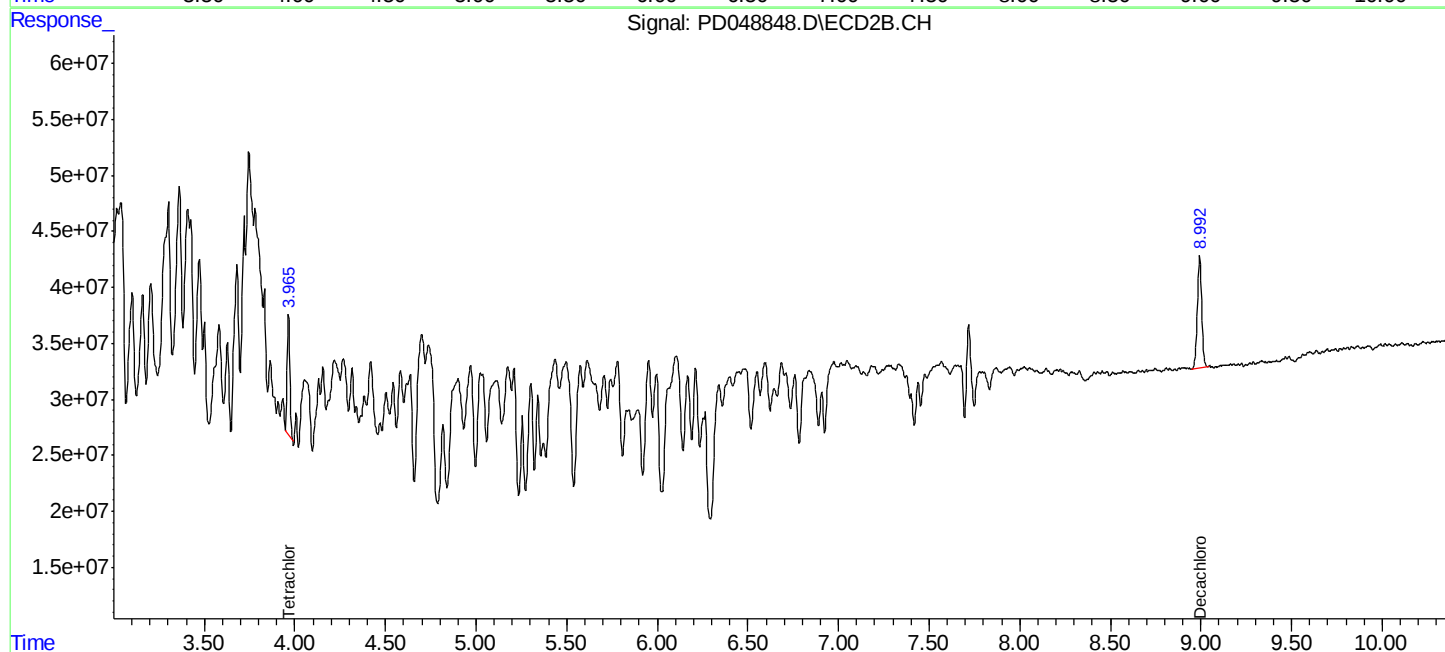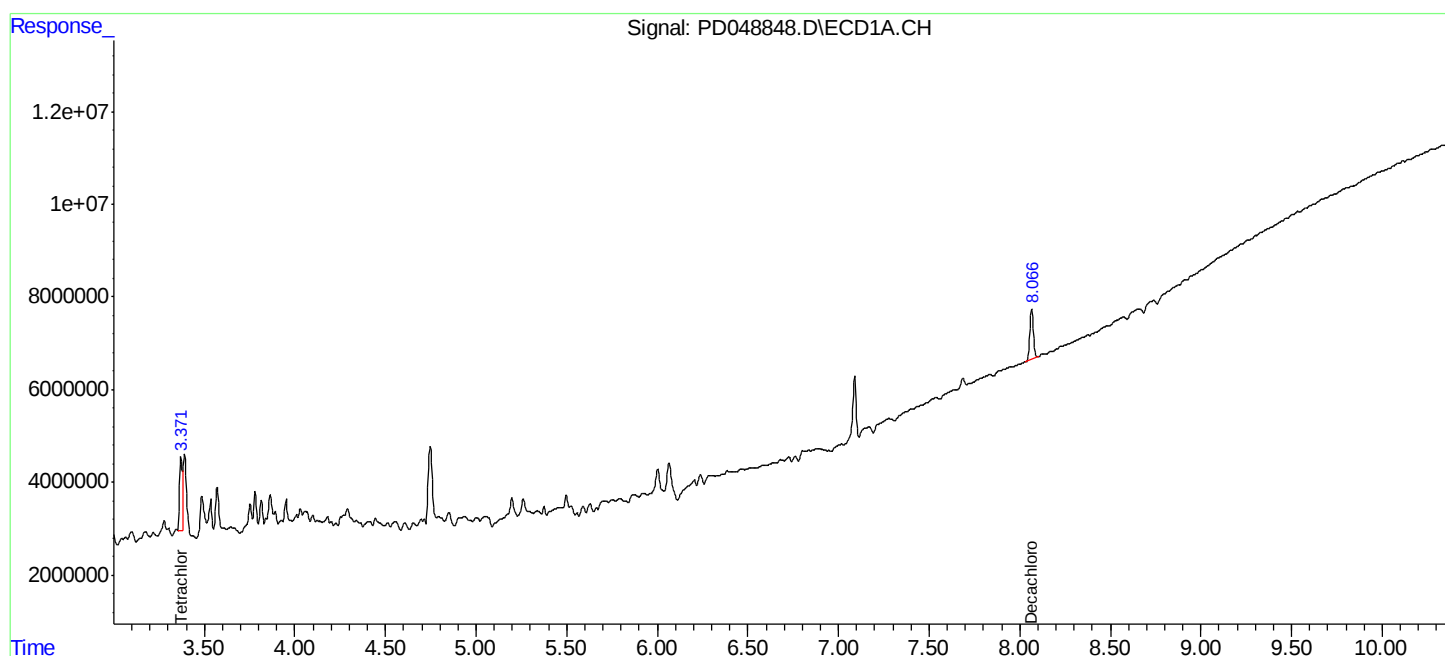

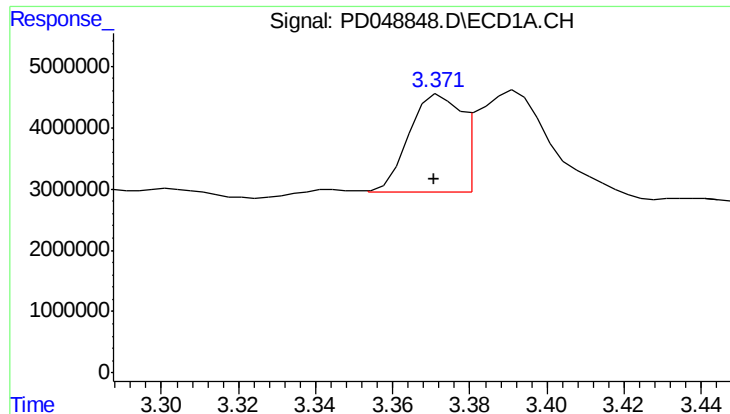


#1 Tetrachloro-m-xylene

R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 13694816
Conc: 12.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
2018-NYSEG-CLARK-AREA-9B


Manual Integrations
APPROVED

Sohil
8/13/2018 12:40:53 PM

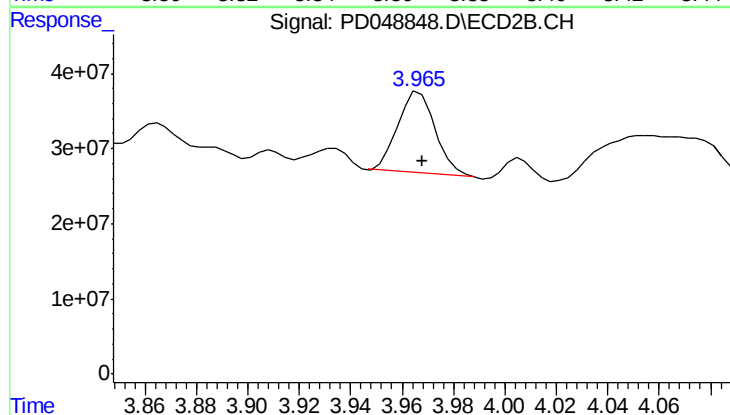


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: -0.003 min
Response: 109309991
Conc: 8.14 ng/ml m

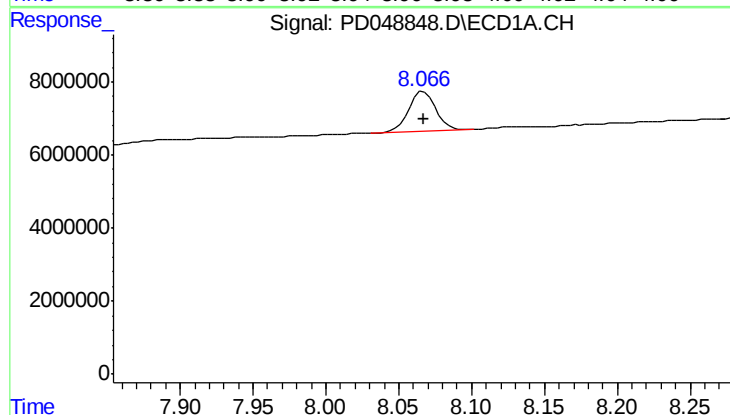

#28 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 13937605
Conc: 9.95 ng/ml

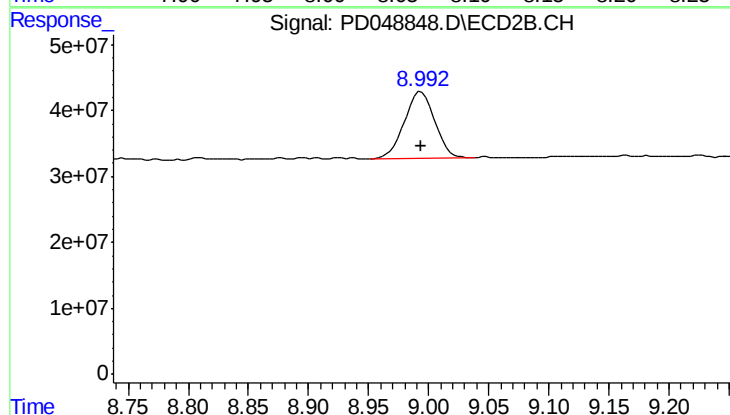

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 177814403
Conc: 11.77 ng/ml