

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
 Data File : PD058909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 12:26
 Operator : DD\AJ
 Sample : L3612-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFP3

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:59:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:26:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.212	3.866	15919063	20769719	16.461	14.341
27) SA Decachlor...	7.847	8.862	29744384	32449102	28.239	23.661
Target Compounds						
12) B 4,4'-DDE	5.297	6.167	2315022	4284617	2.012m	2.704 #
13) MA Dieldrin	5.404	6.323	58669290	5662867	48.297m	3.383m#
14) MA Endrin	5.668	6.535	5152416	1551268	5.187m	1.143m#
16) A 4,4'-DDD	5.809	6.661	5780927	11946046	6.130m	9.113 #
17) MA 4,4'-DDT	6.037	6.963	5192665	4934918	5.774	3.740 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 12:26
Operator : DD\AJ
Sample : L3612-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:26:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

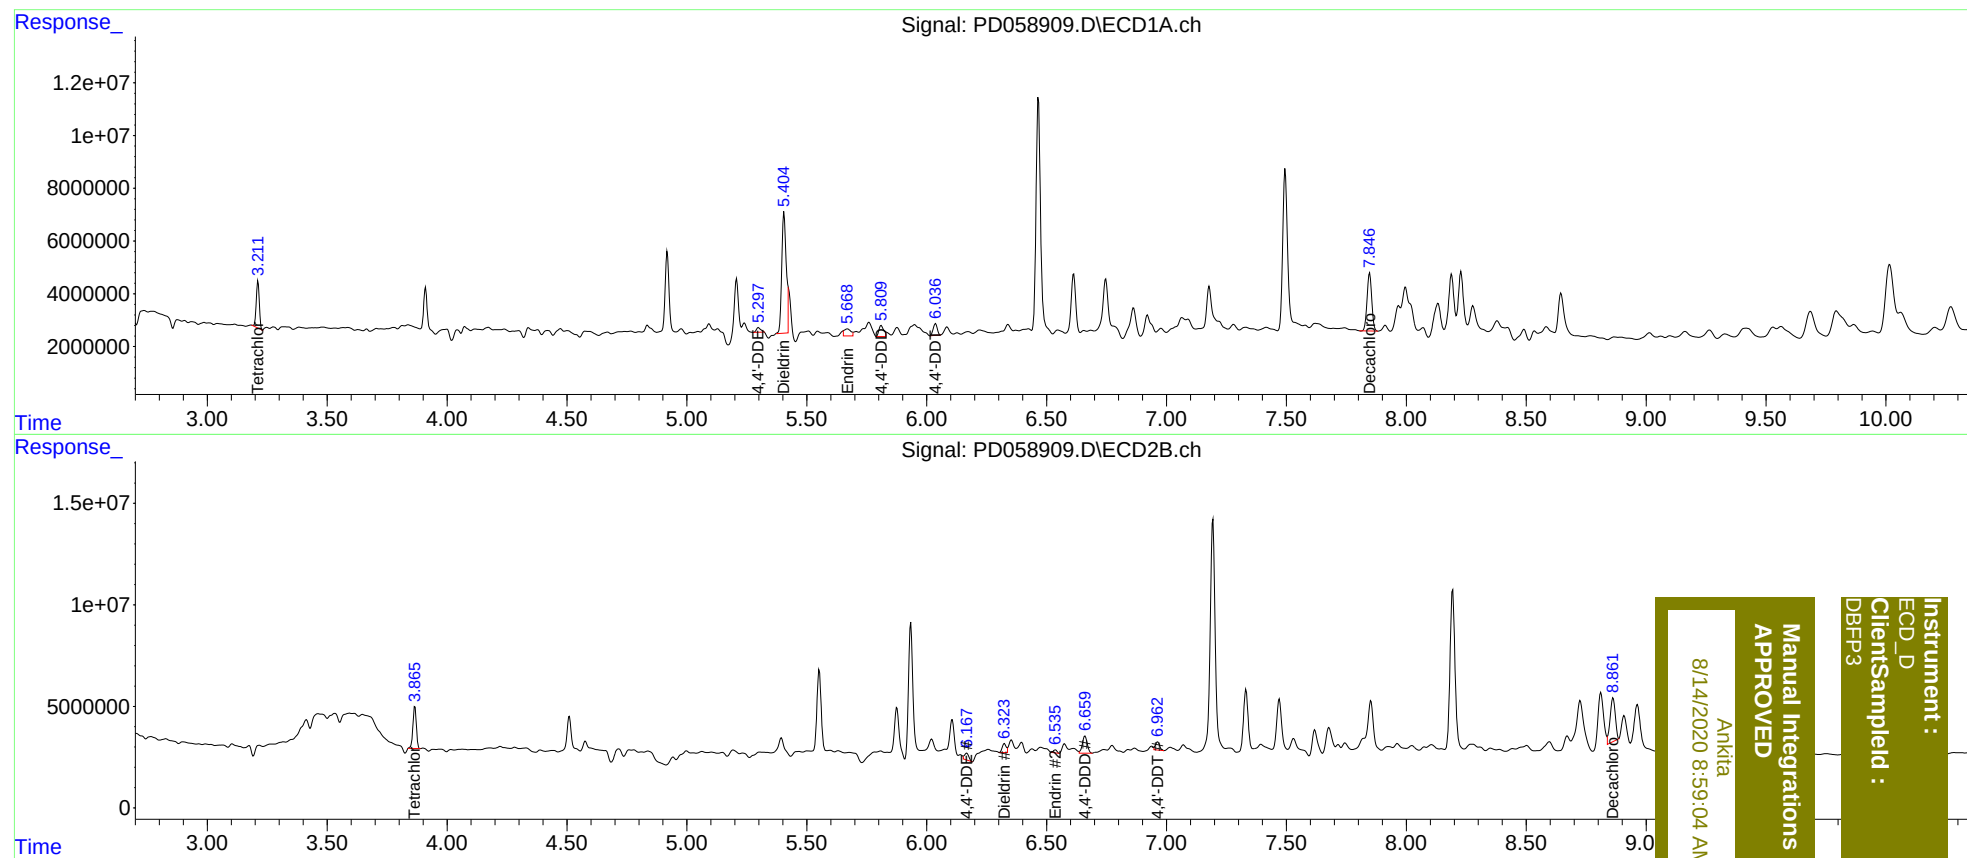

8/14/2020 8:59:04 AM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSample :
DBFP3