

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
 Data File : PD058926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 17:24
 Operator : DD\AJ
 Sample : L3612-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFP8

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:34:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 06:39:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.207	3.866	10230961	14261598	10.579	9.848
27)	SA Decachlor...	7.840	8.860	18486600	18217011	17.551	13.283
Target Compounds							
10)	B trans-Chl...	5.065	5.933	796644	4920921	0.689m	2.954m#
11)	B cis-Chlor...	5.121	6.017	806588	1785676	0.693m	1.061m#
16)	A 4,4'-DDD	5.801	6.661	1564208	2178636	1.659m	1.662

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 17:24
Operator : DD\AJ
Sample : L3612-22
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 06:39:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

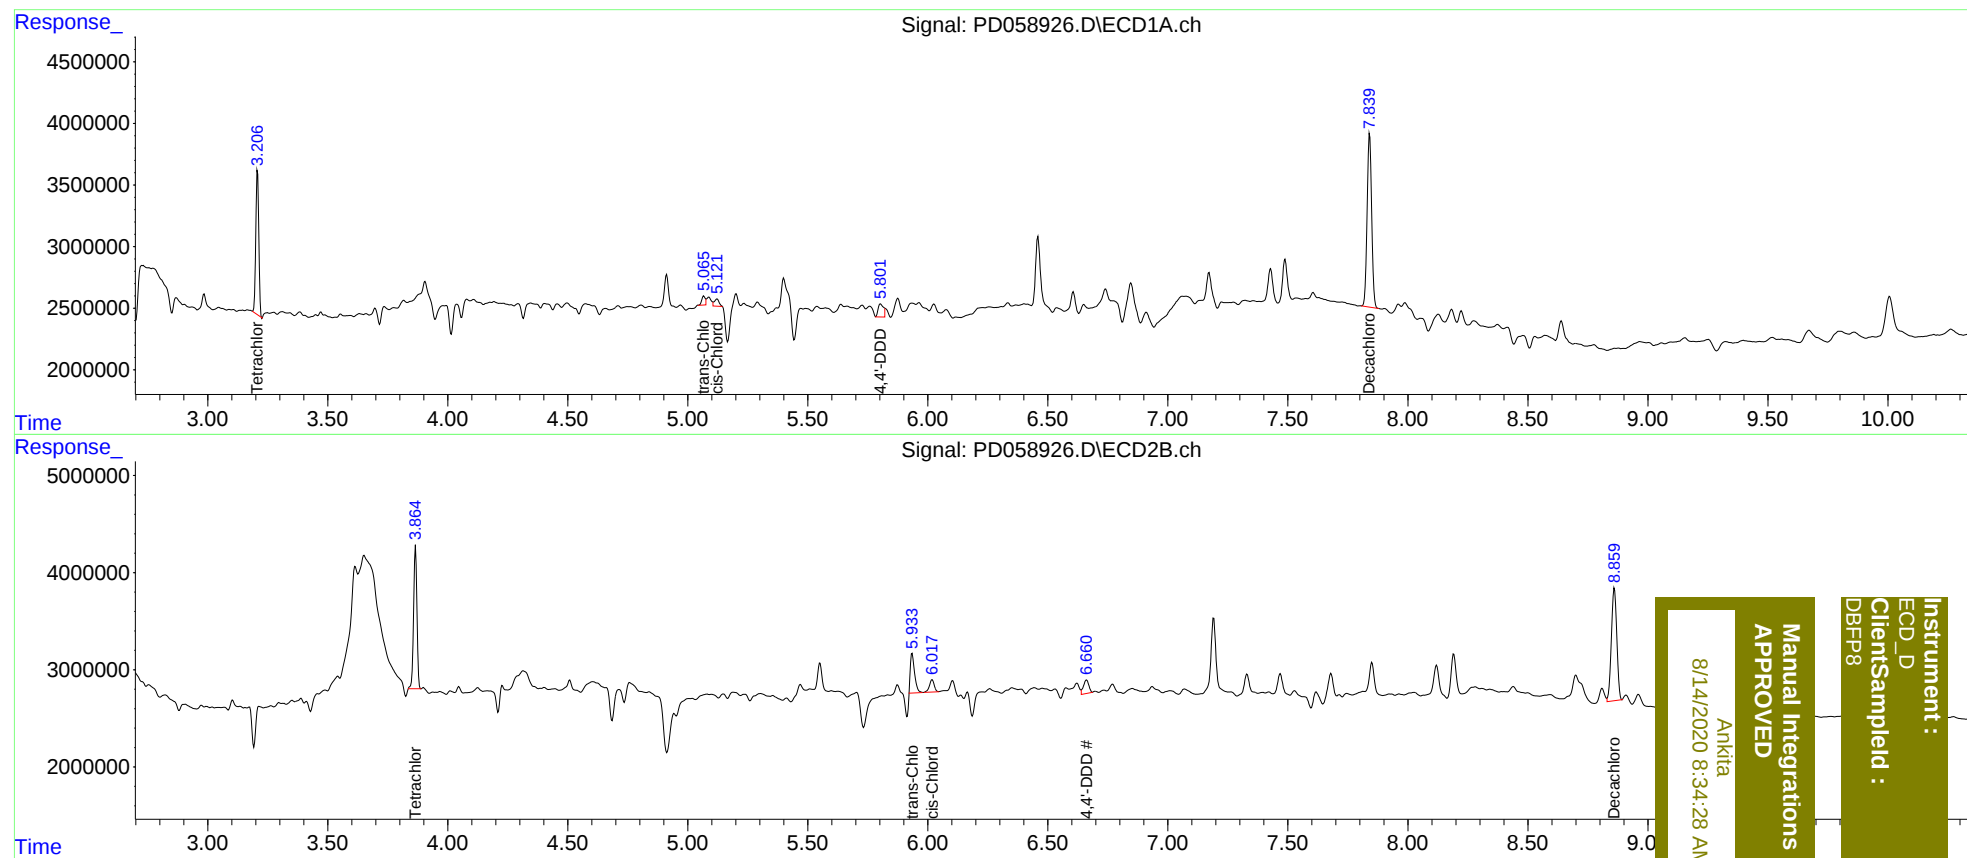

Manual Integrations
APPROVED

Ankita
8/14/2020 8:34:28 AM

Instrument :
ECD_D
Client Sampled :
DBFP8