

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
 Data File : PD058931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 18:35
 Operator : DD\AJ
 Sample : L3612-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFN0

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:34:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 07:08:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	9065683	13044475	9.374	9.007
27)	SA Decachlor...	7.841	8.860	16319879	20134106	15.494	14.681
Target Compounds							
10)	B trans-Chl...	5.065	5.932	781007	3677243	0.675m	2.207m#
11)	B cis-Chlor...	5.120	6.018	619901	1164206	0.533m	0.692 #
12)	B 4,4'-DDE	5.290	6.177	2579732	3534283	2.242	2.230
13)	MA Dieldrin	5.406	6.320	3644724	989467	3.000	0.591 #
16)	A 4,4'-DDD	5.798	6.666	1311690	2846944	1.391m	2.172 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 18:35
Operator : DD\AJ
Sample : L3612-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 07:08:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

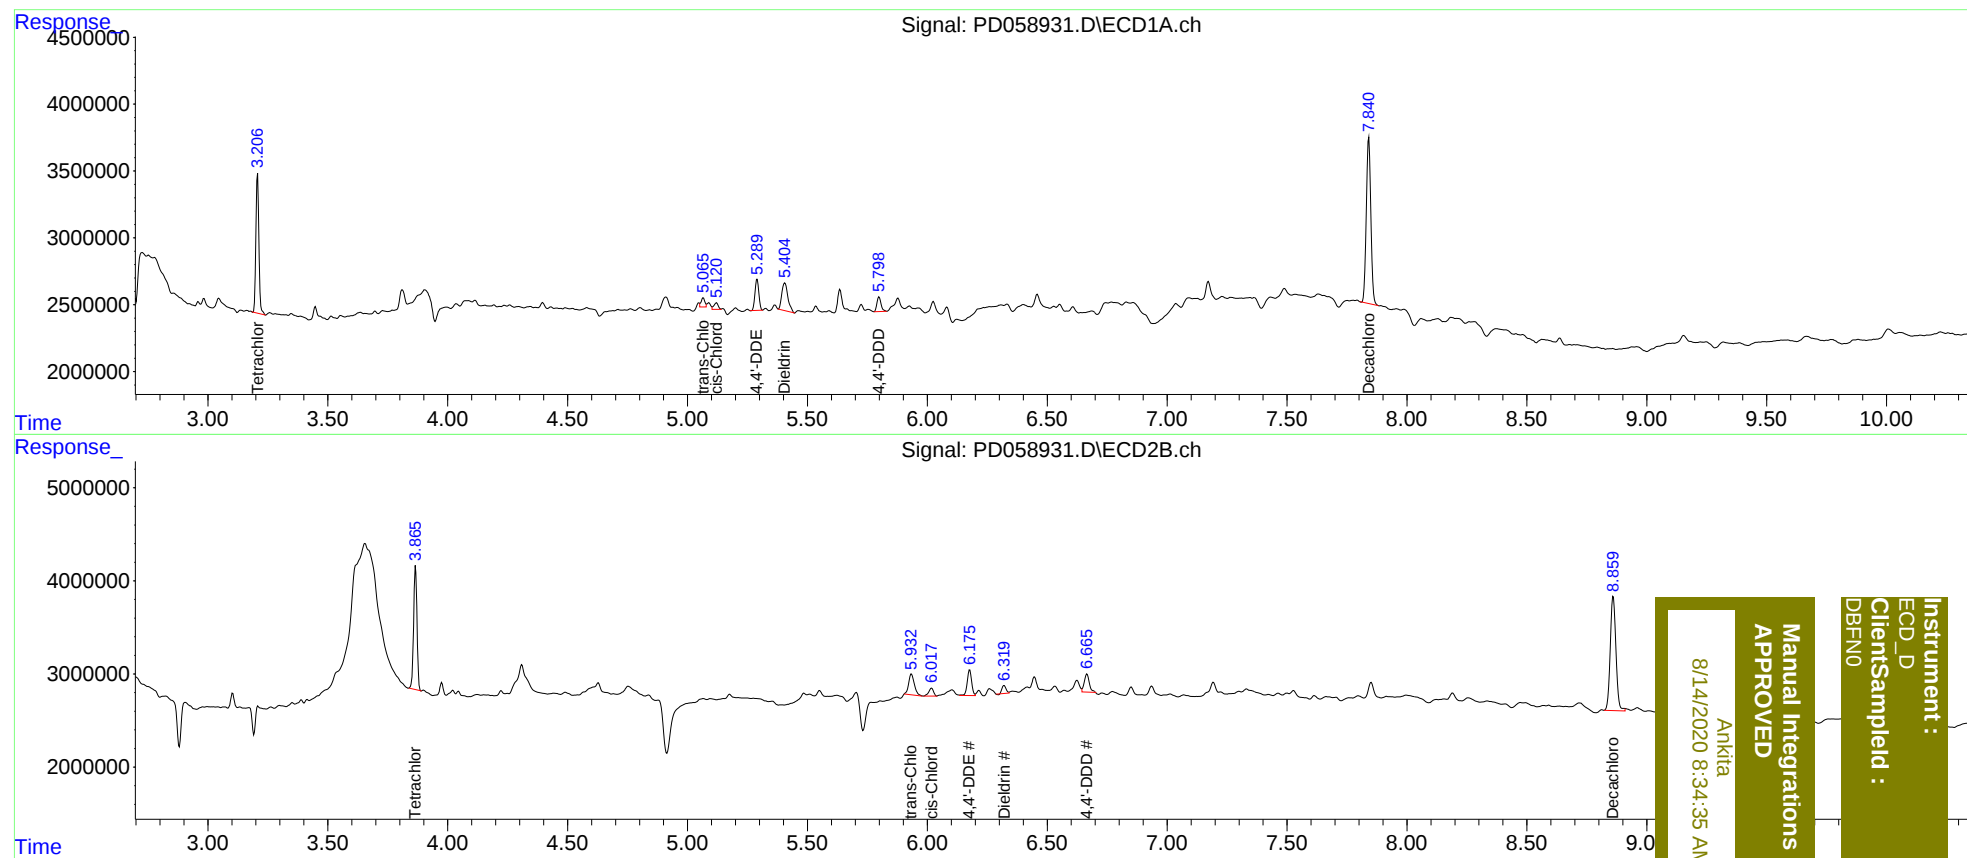

Instrument :
ECD_D
Client Sampled :
DBFNO

Manual Integrations
APPROVED
Ankita
8/14/2020 8:34:35 AM