

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 14:13
Operator : DD\AJ
Sample : PB130836BS
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS36

Manual Integrations
APPROVED

Ankita
8/14/2020 8:34:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:03:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

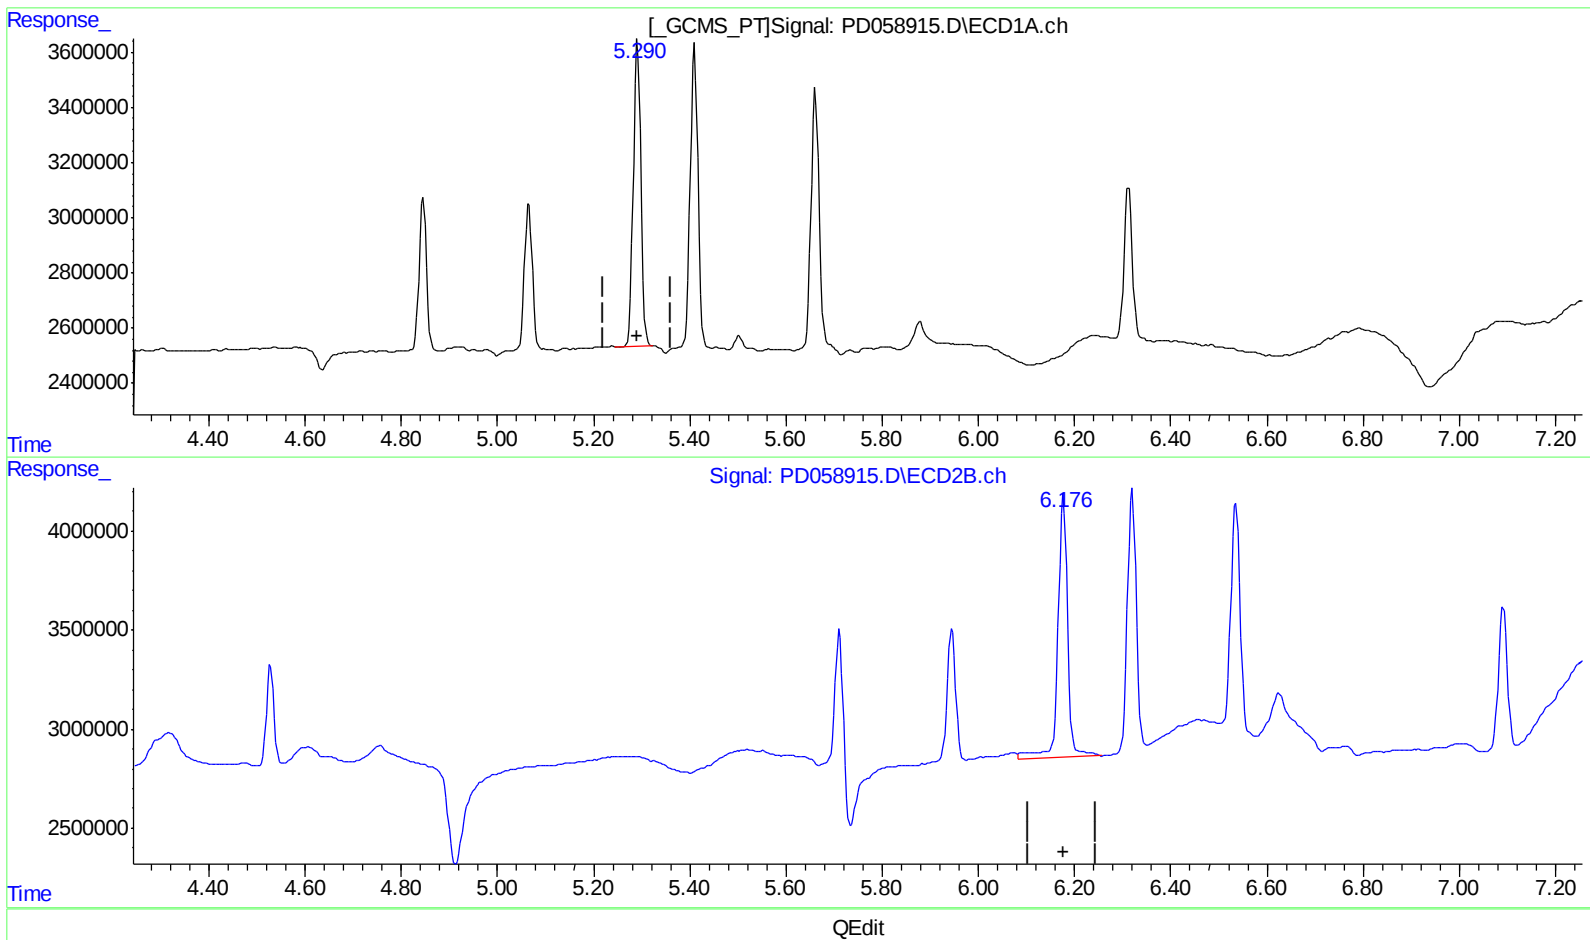

(12) 4,4'-DDE (B)
5.291min 10.501 ng/ml
response 12082760

(12) 4,4'-DDE #2 (B)
6.177min 11.823 ng/ml
response 18737051

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 14:13
Operator : DD\AJ
Sample : PB130836BS
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PLCS36

Manual Integrations
APPROVED

Ankita
8/14/2020 8:34:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:07:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

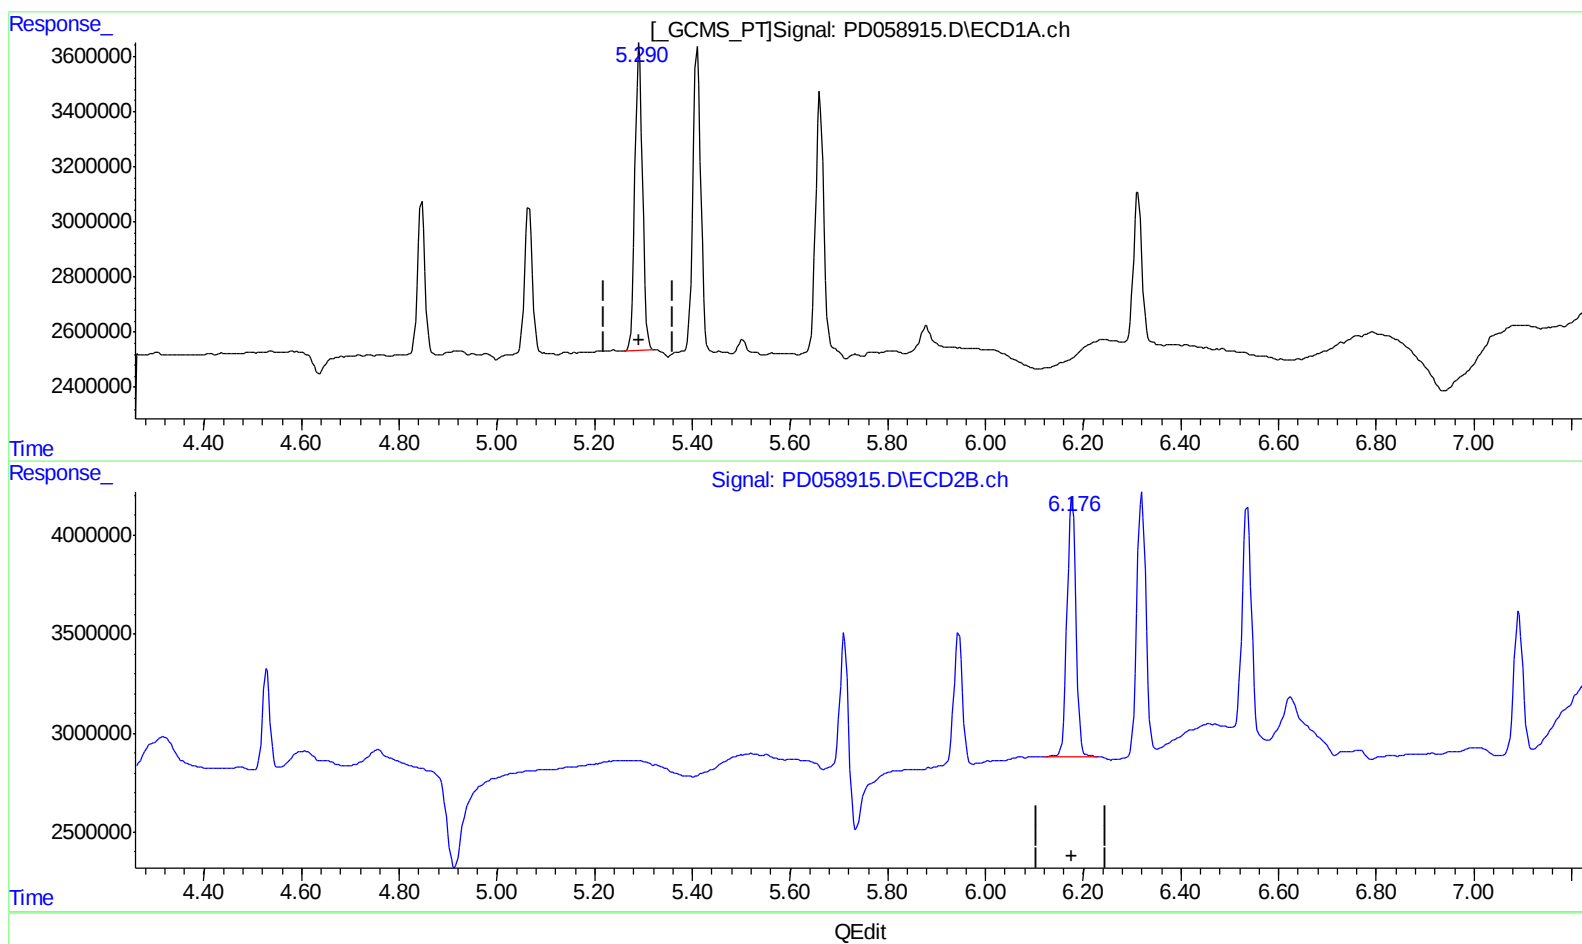

(12) 4,4'-DDE (B)
5.291min 10.576 ng/ml
response 12169403

(12) 4,4'-DDE #2 (B)
6.176min 10.403 ng/ml m
response 16486380

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
 Data File : PD058915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 14:13
 Operator : DD\AJ
 Sample : PB130836BS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS36

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:34:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:07:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.207	3.866	22439203	33049718	23.203	22.821
27) SA Decachlor...	7.841	8.861	45983183	57300735	43.656	41.782
Target Compounds						
3) MA gamma-BHC...	3.900	4.529	5299422	5301316	3.813	2.789 #
8) B Heptachlo...	4.846	5.711	5923496	10433139	5.243	6.266
10) B trans-Chl...	5.065	5.945	6115226	8050296	5.289	4.833
12) B 4,4'-DDE	5.291	6.176	12169403	16486380	10.576	10.403m
13) MA Dieldrin	5.410	6.320	12316849	16655178	10.139	9.950
14) MA Endrin	5.661	6.536	11625373	15023688	11.702	11.074
19) B Endosulfa...	6.312	7.092	6633059	9116033	6.482	6.343

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 08/18/20