

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
 Data File : PD058910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 12:40
 Operator : DD\AJ
 Sample : L3612-16
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DBFP4

Manual Integrations
 APPROVED

Ankita
 8/14/2020 8:59:06 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:37:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 06 11:29:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.208	3.866	13957721	19285011	14.433	13.316
27)	SA Decachlor...	7.841	8.860	30847946	27116089	29.287	19.772 #
Target Compounds							
8)	B Heptachlo...	4.845	5.709	2161093	5766232	1.913m	3.463 #
10)	B trans-Chl...	5.066	5.933	9483094	90023702	8.201m	54.042 #
11)	B cis-Chlor...	5.122	6.020	8403650	27026331	7.221m	16.053 #
12)	B 4,4'-DDE	5.291	6.170	4753366	6135329	4.131m	3.871
13)	MA Dieldrin	5.400	6.321	79704552	20431904	65.614	12.206 #
14)	MA Endrin	5.667	6.533	5109810	1477530	5.144m	1.089m#
16)	A 4,4'-DDD	5.803	6.660	5681473	18520456	6.025m	14.129 #
17)	MA 4,4'-DDT	6.031	6.962	10280031	7210867	11.431	5.464 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081220\
Data File : PD058910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 12:40
Operator : DD\AJ
Sample : L3612-16
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:37:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD080620CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 06 11:29:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

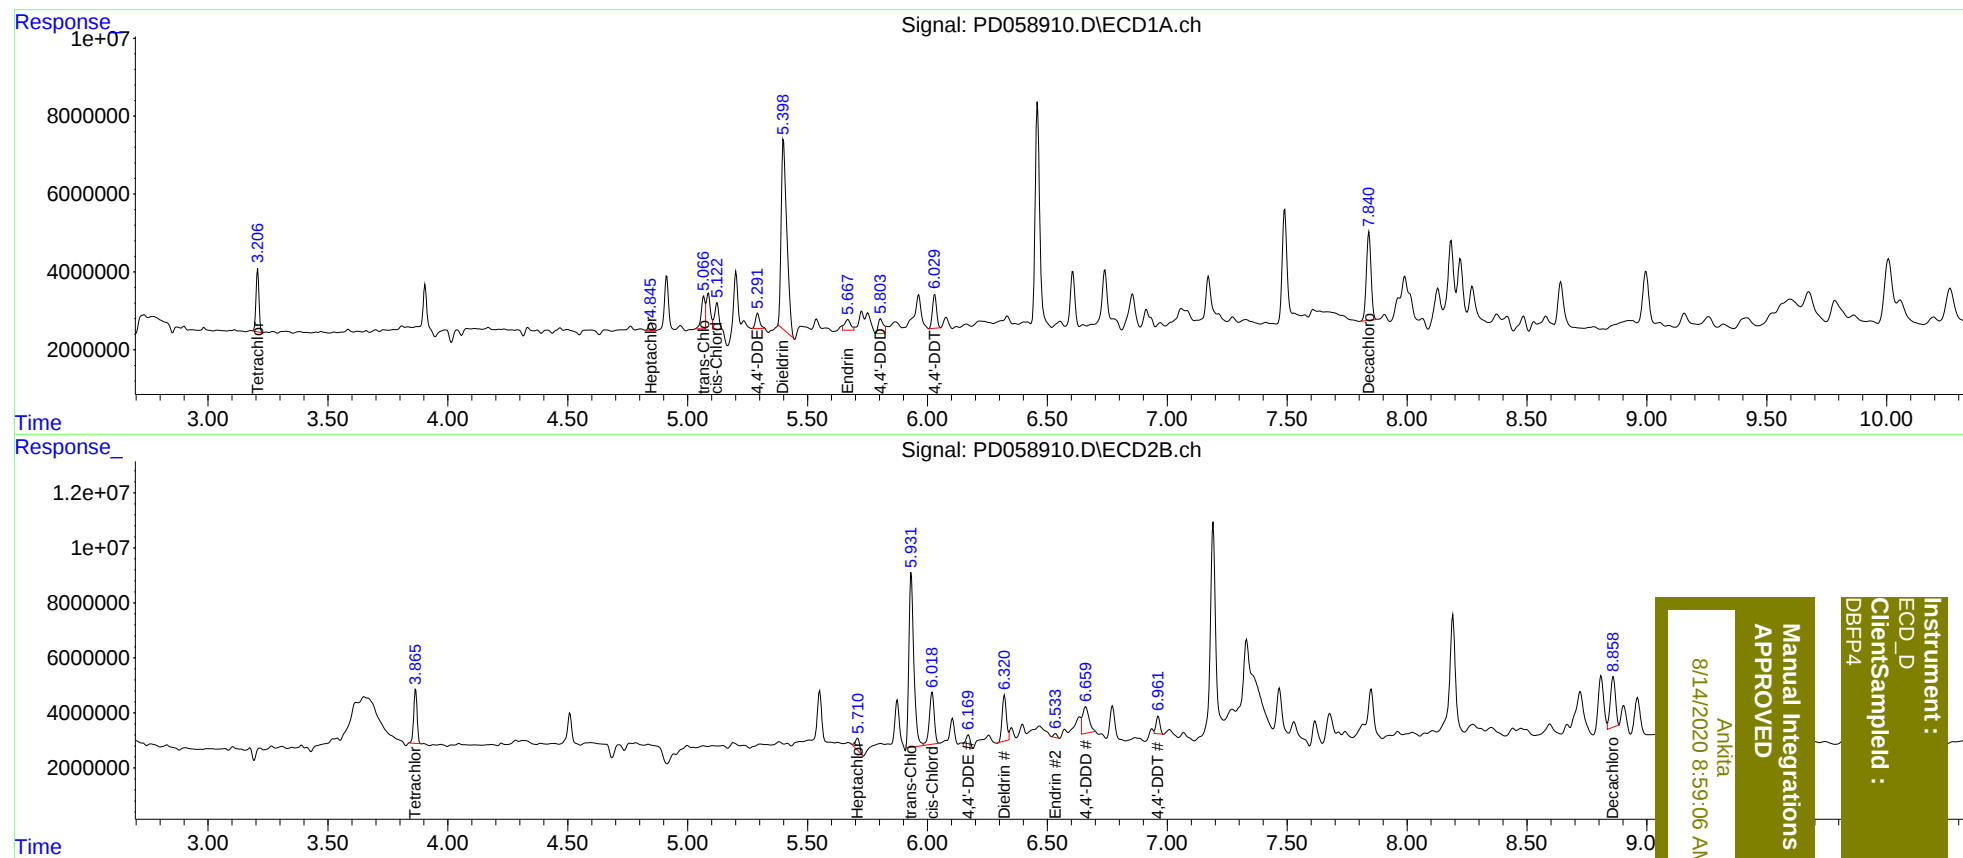

8/14/2020 8:59:06 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
ClientSampled :
DBFP4