

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081222\
 Data File : PD071536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 10:03
 Operator : AR\AJ
 Sample : N4015-02
 Misc : PEST MDL 1 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MDL-WATER-QT3-2022-06

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/15/2022
 Supervised By :Ankita Jodhani 08/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 22:22:38 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 11 04:21:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.807	3.564	49791910	557.3E6	17.455	17.003
27)	SA Decachlor...	8.000	9.090	95817600	356.7E6	34.128	37.206
Target Compounds							
2)	A alpha-BHC	3.316	4.030	3343173	43288024	0.813	1.025 #
3)	MA gamma-BHC...	3.650	4.366	3556657	38450028	0.904	1.094
4)	MA Heptachlor	3.995	4.943	3411347	28473640	0.839m	1.107 #
5)	MB Aldrin	4.280	5.286	3383280	23871083	0.816	1.067 #
6)	B beta-BHC	3.947	4.573	1368681	15144860	0.773m	1.048 #
7)	B delta-BHC	4.182	4.820	3056811	20999648	0.770	0.749
8)	B Heptachlo...	4.787	5.717	3231032	21514688	0.848	1.081 #
9)	A Endosulfan I	5.160	6.105	2970529	16450819	0.873m	1.020
10)	B trans-Chl...	5.040	5.972	3344925	17202035	0.841	0.941
11)	B cis-Chlor...	5.103	6.050	3300623	17512824	0.848m	0.980
12)	B 4,4'-DDE	5.296	6.223	2760995	16821121	0.777	1.069 #
13)	MA Dieldrin	5.428	6.382	3097746	18097271	0.817	1.092 #
14)	MA Endrin	5.705	6.615	2813910	15072989	0.858	1.188 #
15)	B Endosulfa...	6.000	6.841	3106008	13609149	0.996	1.041
16)	A 4,4'-DDD	5.854	6.747	2206133	14067416	0.811	1.155 #
17)	MA 4,4'-DDT	6.108	7.058	1783640	11198564	0.631	0.947 #
18)	B Endrin al...	6.181	6.972	2188783	9983741	0.816	0.908
19)	B Endosulfa...	6.405	7.204	2698808	12740058	0.877	1.039
20)	A Methoxychlor	6.687	7.534	1276300	6451160	0.884	1.226 #
21)	B Endrin ke...	6.915	7.696	2400774	14062499	0.702	1.072 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081222\
Data File : PD071536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 10:03
Operator : AR\AJ
Sample : N4015-02
Misc : PEST MDL 1 PPB
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 22:22:38 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081122CLP.M
Quant Title : GC Extractables
QLast Update : Thu Aug 11 04:21:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

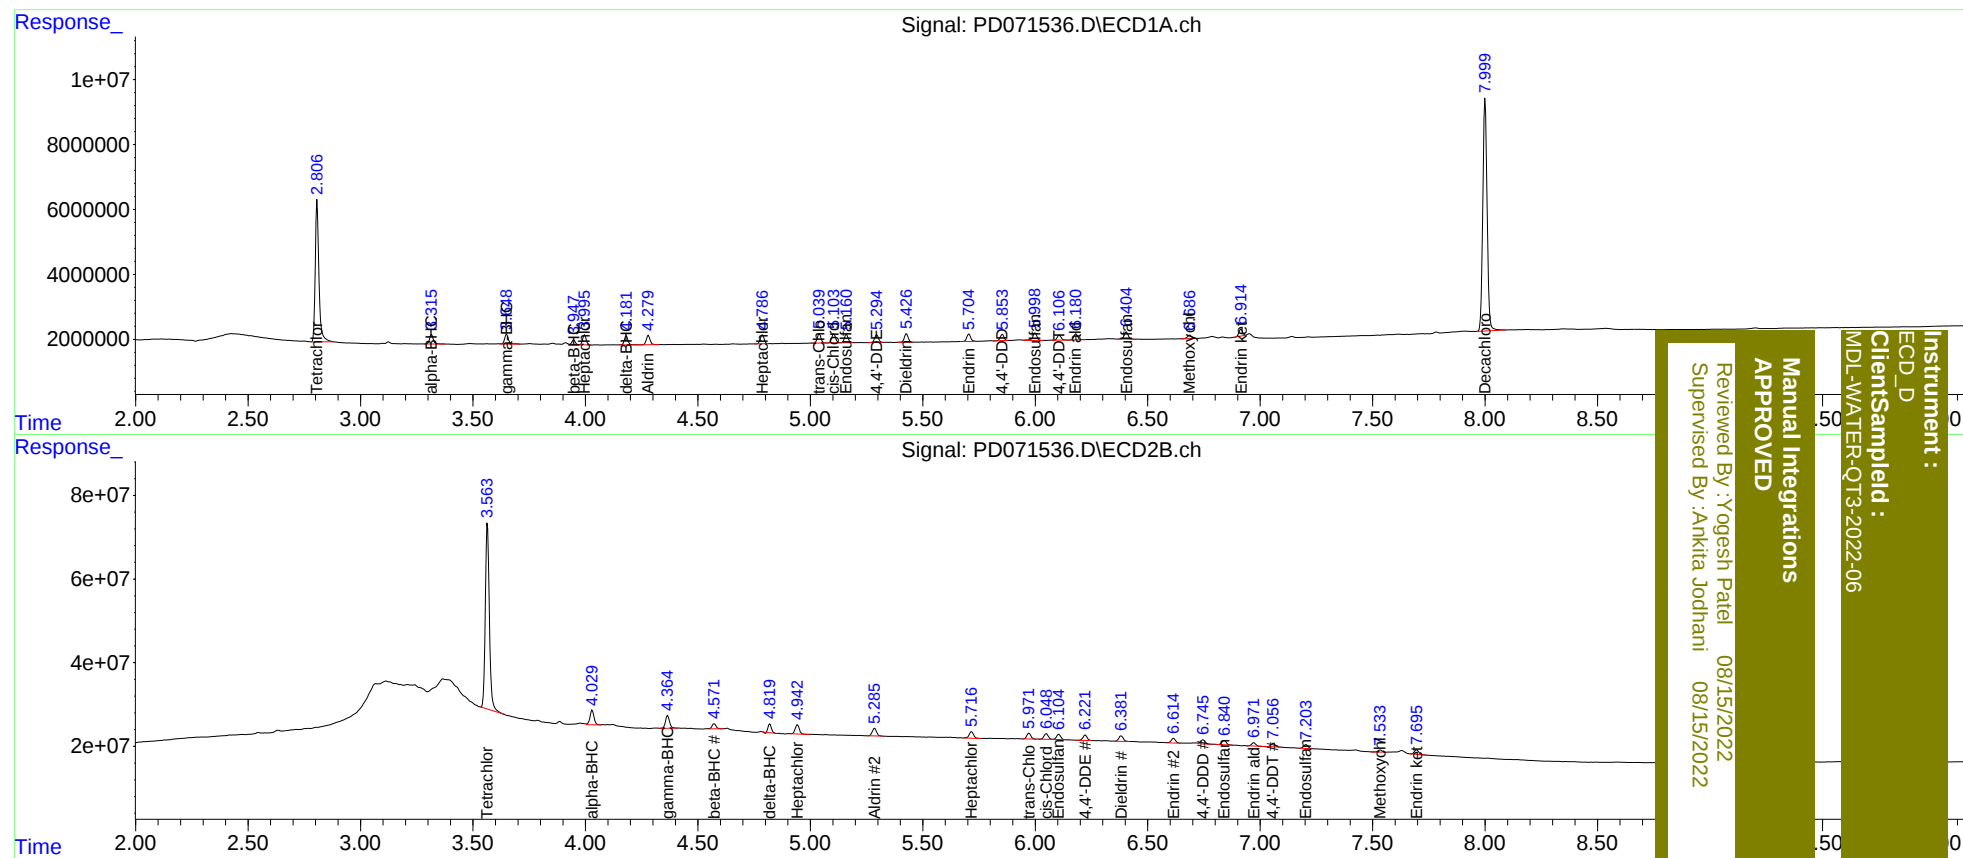

Reviewed By : Yogesh Patel 08/15/2022
Supervised By : Ankita Jodhani 08/15/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
MDL-WATER-QT3-2022-06