

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048866.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 15:05
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:15:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.369	3.968	28228449	330.5E6	25.463	24.622
28)	SA Decachlor...	8.066	8.994	106.4E6	260.5E6	75.971	17.250 #
Target Compounds							
2)	A alpha-BHC	3.788	4.371	3628025	1768362	1.894	0.078 #
3)	MA gamma-BHC...	4.073	4.694f	9320649	33389101	5.138	1.615 #
12)	B 4,4'-DDE	5.519	0.000	11296125	0	7.240	N.D. #
14)	MA Endrin	5.895	0.000	5415405	0	3.391	N.D. #
15)	B Endosulfa...	6.087f	0.000	6711562	0	4.657	N.D. #
19)	B Endosulfa...	6.569f	0.000	20638812	0	15.594	N.D. #
20)	A Methoxychlor	6.863f	0.000	18235170	0	23.410	N.D. #
23)	Chlordane-1	4.257	0.000	4776215	0	94.717	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048866.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 15:05
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:15:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

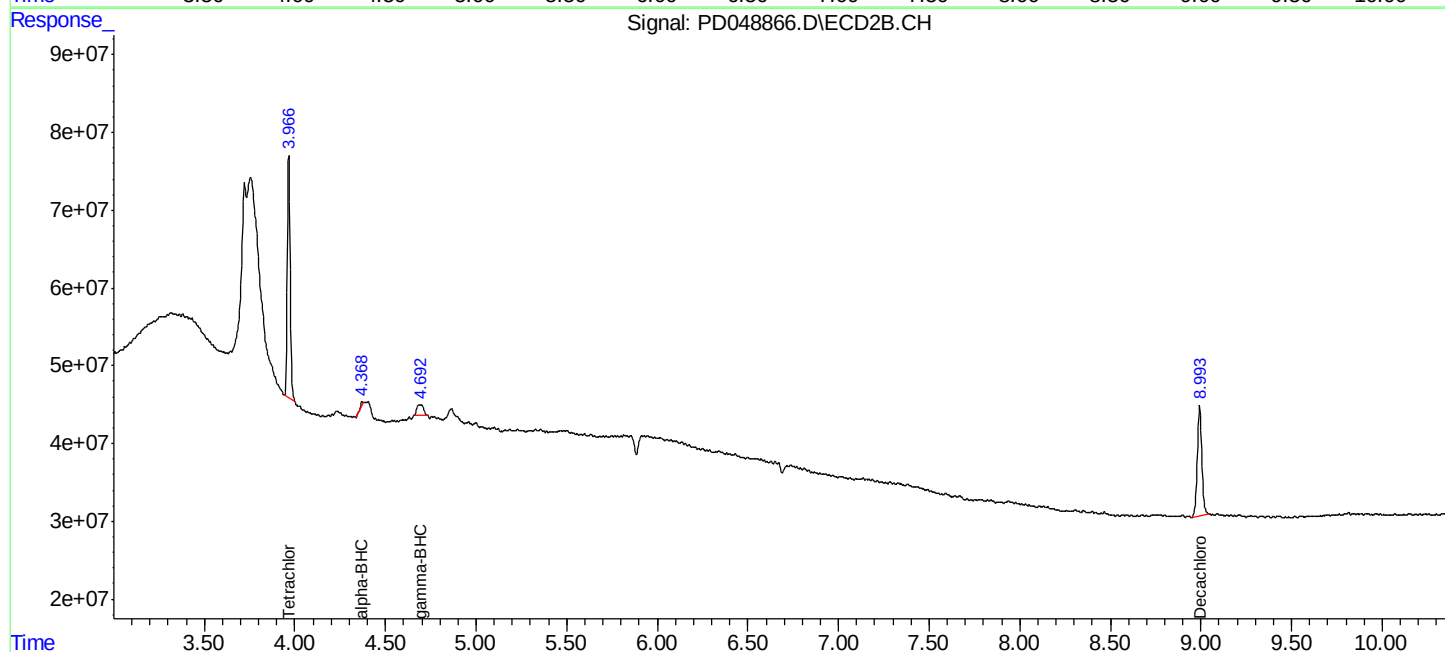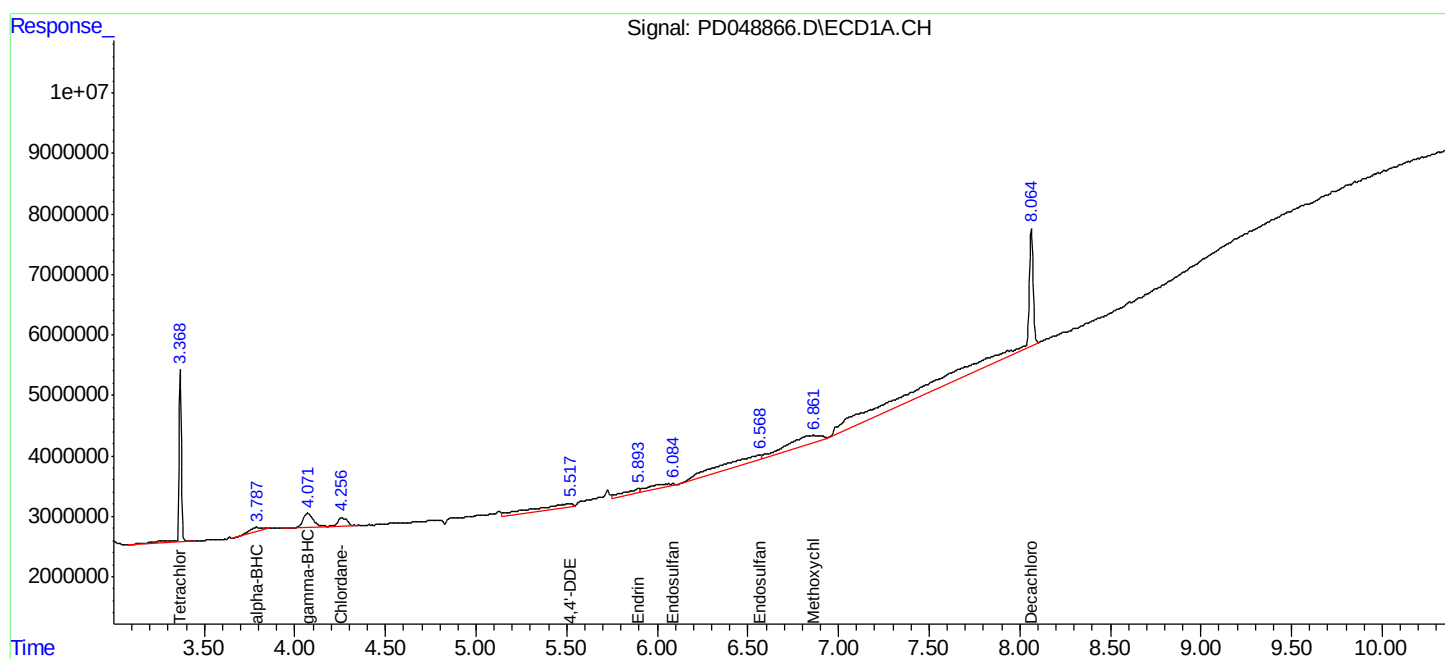


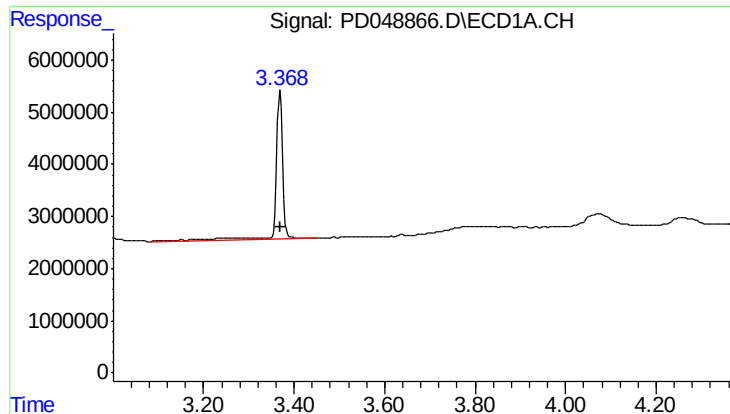

#1 Tetrachloro-m-xylene


R.T.: 3.369 min
Delta R.T.: -0.001 min
Response: 28228449
Conc: 25.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

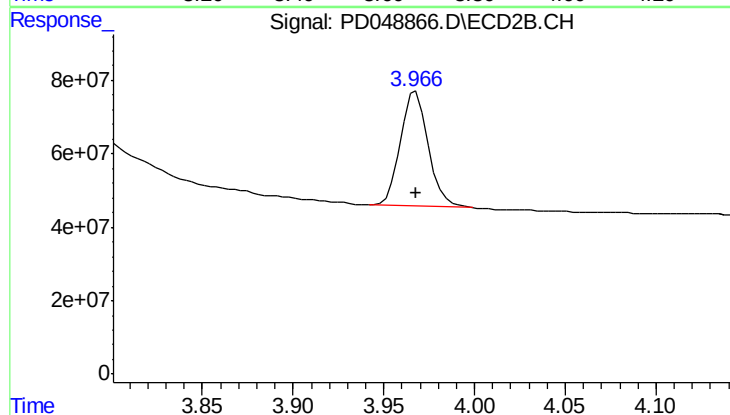


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 330520597
Conc: 24.62 ng/ml

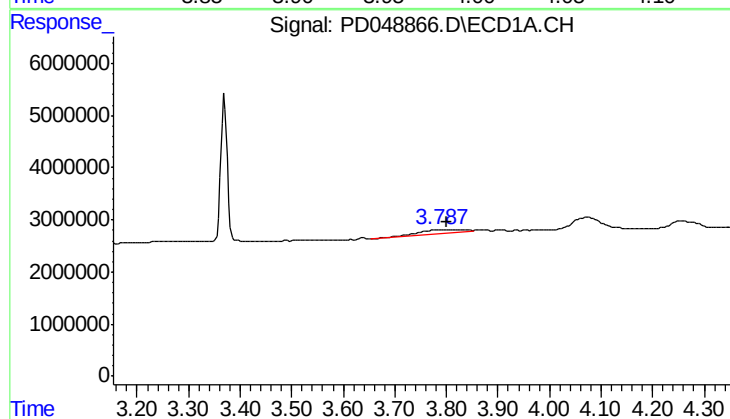


#2 alpha-BHC

R.T.: 3.788 min
Delta R.T.: -0.013 min
Response: 3628025
Conc: 1.89 ng/ml

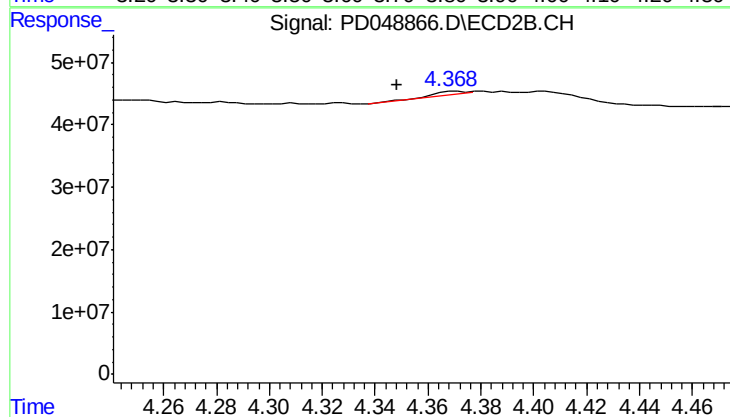

#2 alpha-BHC


R.T.: 4.371 min
Delta R.T.: 0.023 min
Response: 1768362
Conc: 0.08 ng/ml

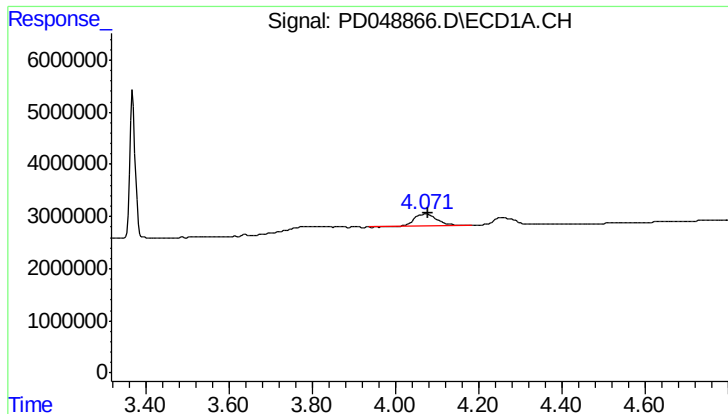

#3 gamma-BHC (Lindane)


R.T.: 4.073 min
Delta R.T.: -0.006 min
Response: 9320649
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

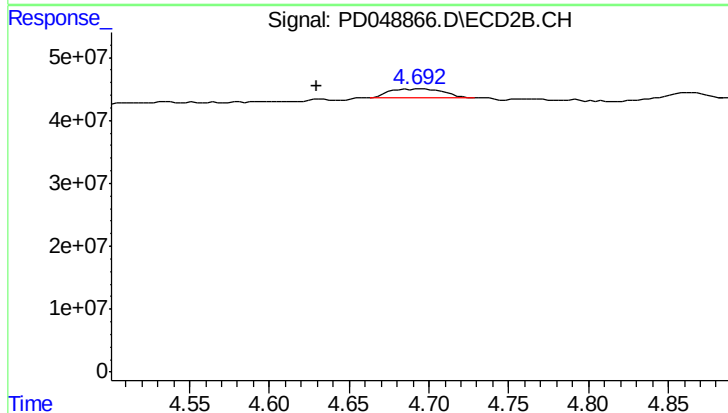


#3 gamma-BHC (Lindane)

R.T.: 4.694 min
Delta R.T.: 0.065 min
Response: 33389101
Conc: 1.61 ng/ml

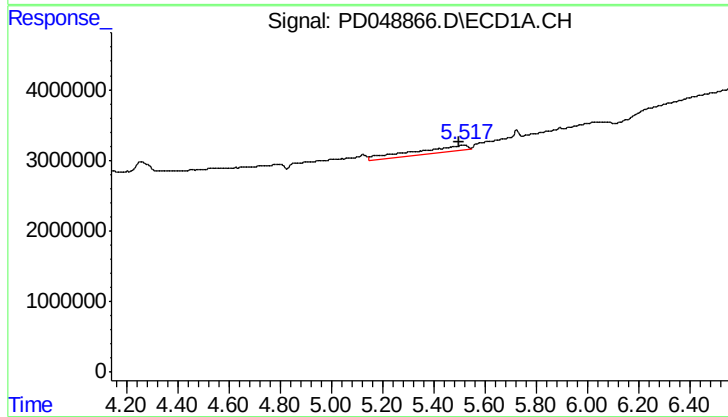


#12 4,4'-DDE

R.T.: 5.519 min
Delta R.T.: 0.022 min
Response: 11296125
Conc: 7.24 ng/ml

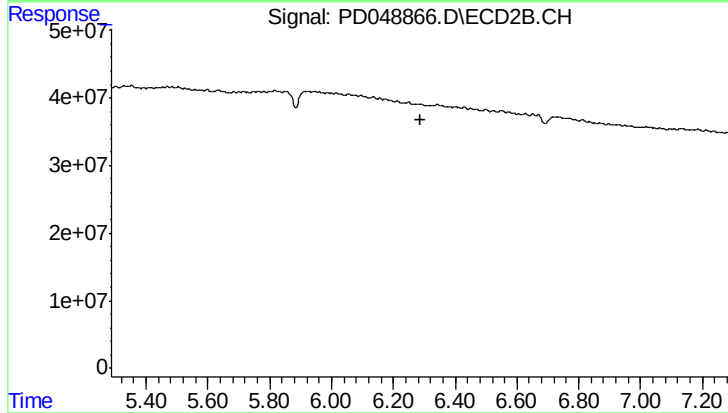

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

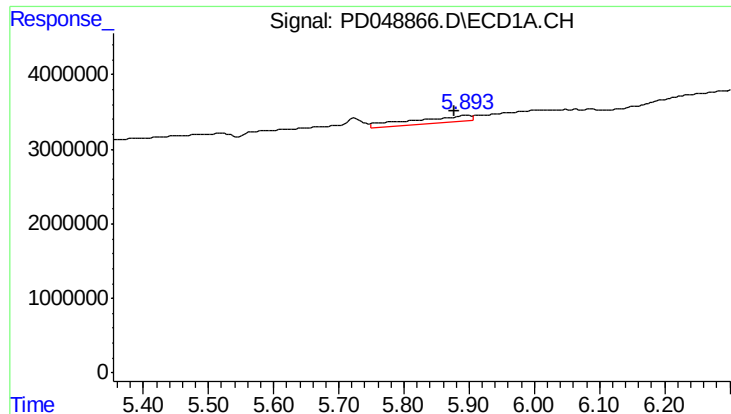

#14 Endrin


R.T.: 5.895 min
Delta R.T.: 0.017 min
Response: 5415405
Conc: 3.39 ng/ml

Instrument :
ECD_D
ClientSampleId :

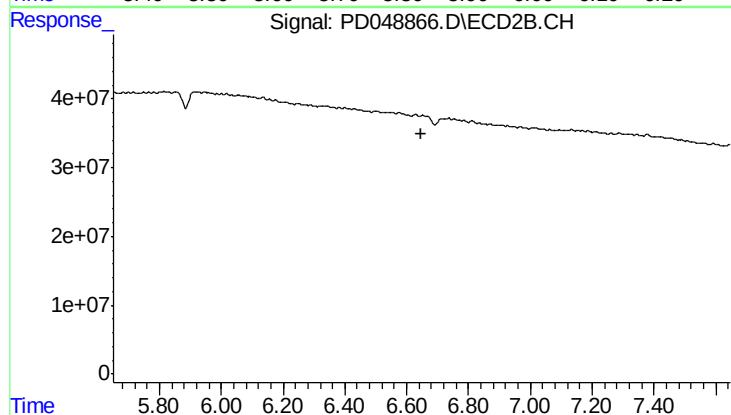


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.649 min
Response: 0
Conc: N.D.

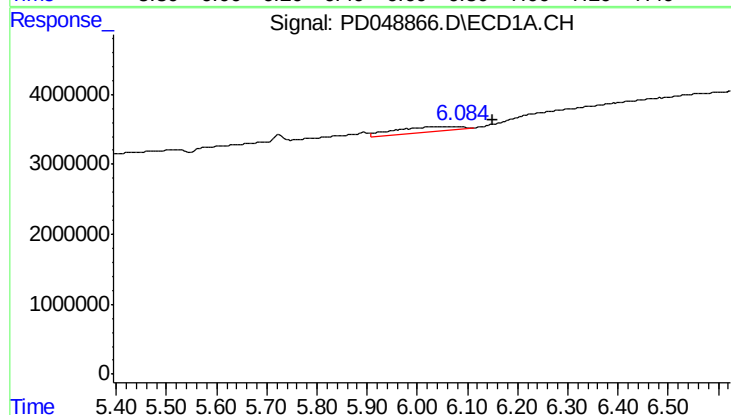


#15 Endosulfan II

R.T.: 6.087 min
Delta R.T.: -0.064 min
Response: 6711562
Conc: 4.66 ng/ml

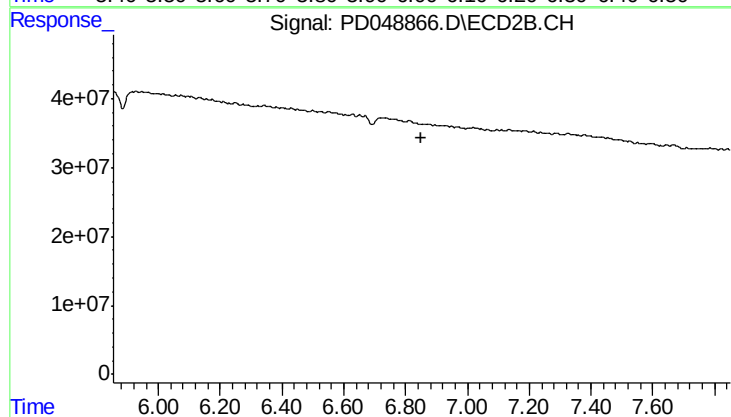

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.851 min
Response: 0
Conc: N.D.

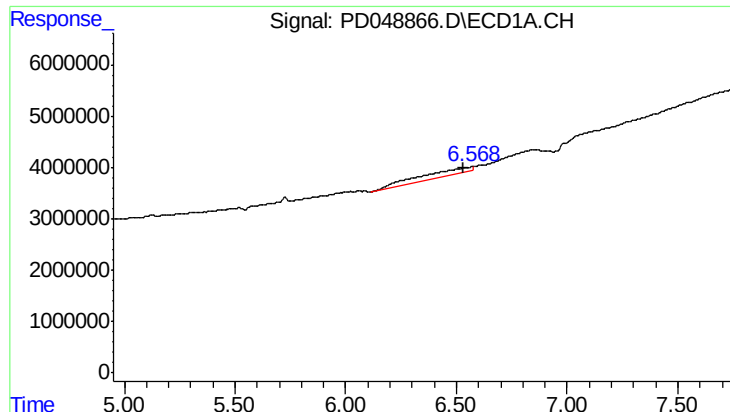

#19 Endosulfan Sulfate


R.T.: 6.569 min
Delta R.T.: 0.039 min
Response: 20638812
Conc: 15.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

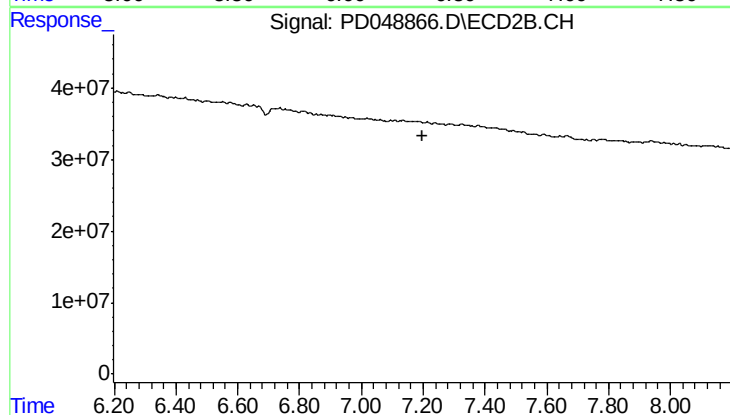


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.196 min
Response: 0
Conc: N.D.

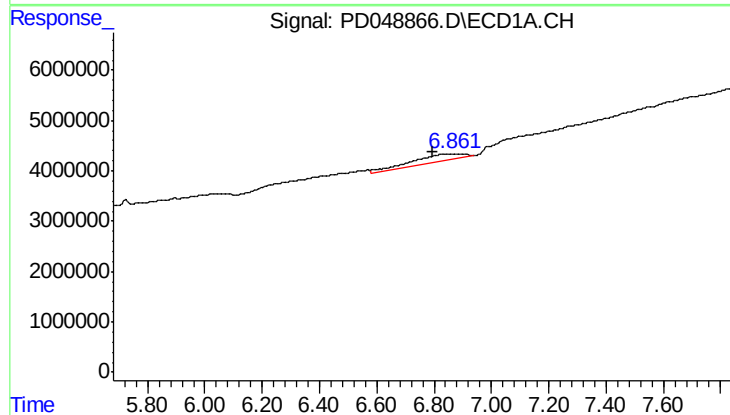


#20 Methoxychlor

R.T.: 6.863 min
Delta R.T.: 0.068 min
Response: 18235170
Conc: 23.41 ng/ml

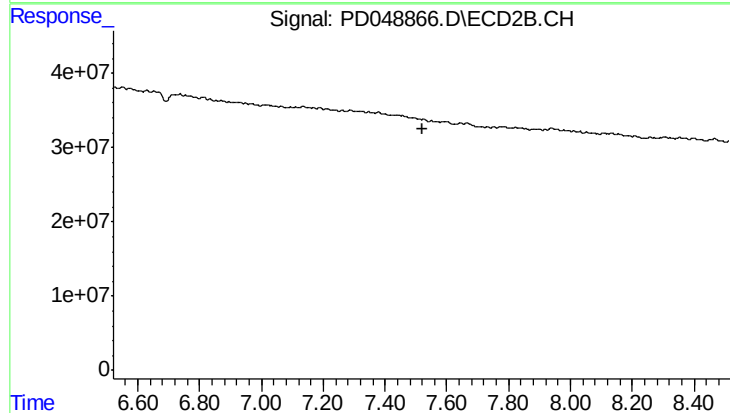

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

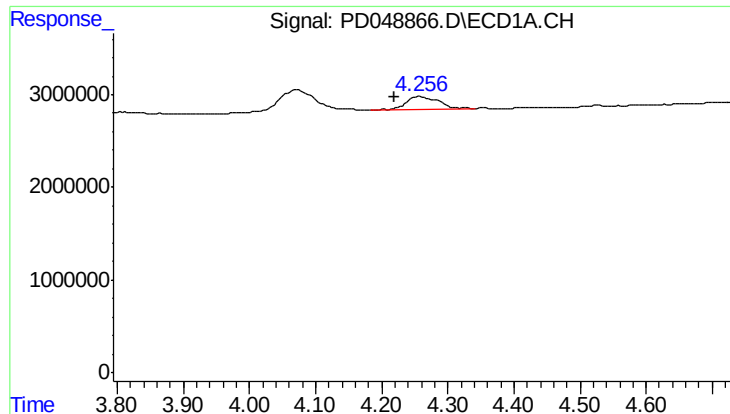

#23 Chlordane-1


R.T.: 4.257 min
Delta R.T.: 0.037 min
Response: 4776215
Conc: 94.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

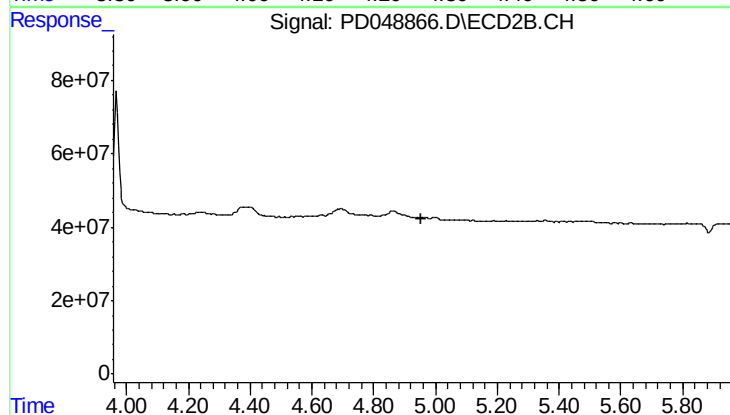


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.955 min
Response: 0
Conc: N.D.

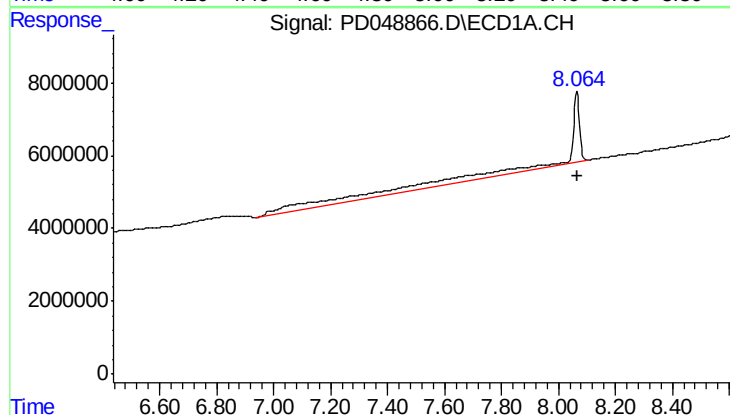

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 106381385
Conc: 75.97 ng/ml

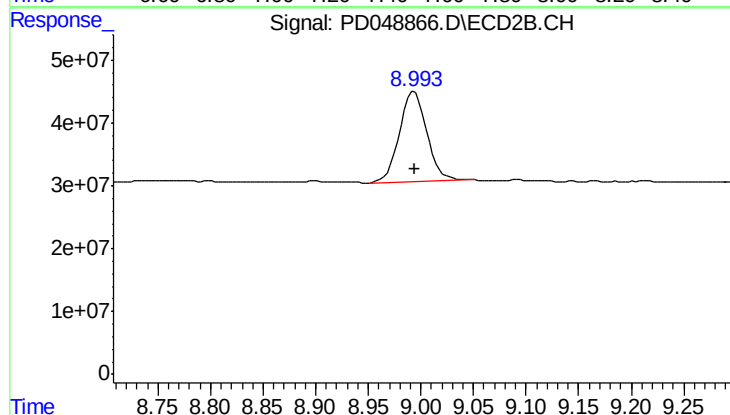

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 260531772
Conc: 17.25 ng/ml