

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048874.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 17:55
 Operator : AJ\SJ
 Sample : J4442-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:17:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.969	24014657	312.4E6	21.662	23.269
28)	SA Decachlor...	8.069	8.996	31662731	268.1E6	22.612	17.751
Target Compounds							
2)	A alpha-BHC	3.785	0.000	2635551	0	1.376	N.D. #
3)	MA gamma-BHC...	4.076	0.000	6683509	0	3.685	N.D. #
6)	B beta-BHC	4.291f	0.000	3166638	0	4.437	N.D. #
7)	B delta-BHC	0.000	4.998	0	20110575	N.D.	1.073 #
8)	B Heptachlo...	5.111f	0.000	550130	0	0.359	N.D. #
14)	MA Endrin	5.904	0.000	957930	0	0.600	N.D. #
20)	A Methoxychlor	6.853f	0.000	19658258	0	25.237	N.D. #
23)	Chlordane-1	4.258	4.998	2021001	20110575	40.078	27.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048874.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 17:55
Operator : AJ\SJ
Sample : J4442-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:17:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

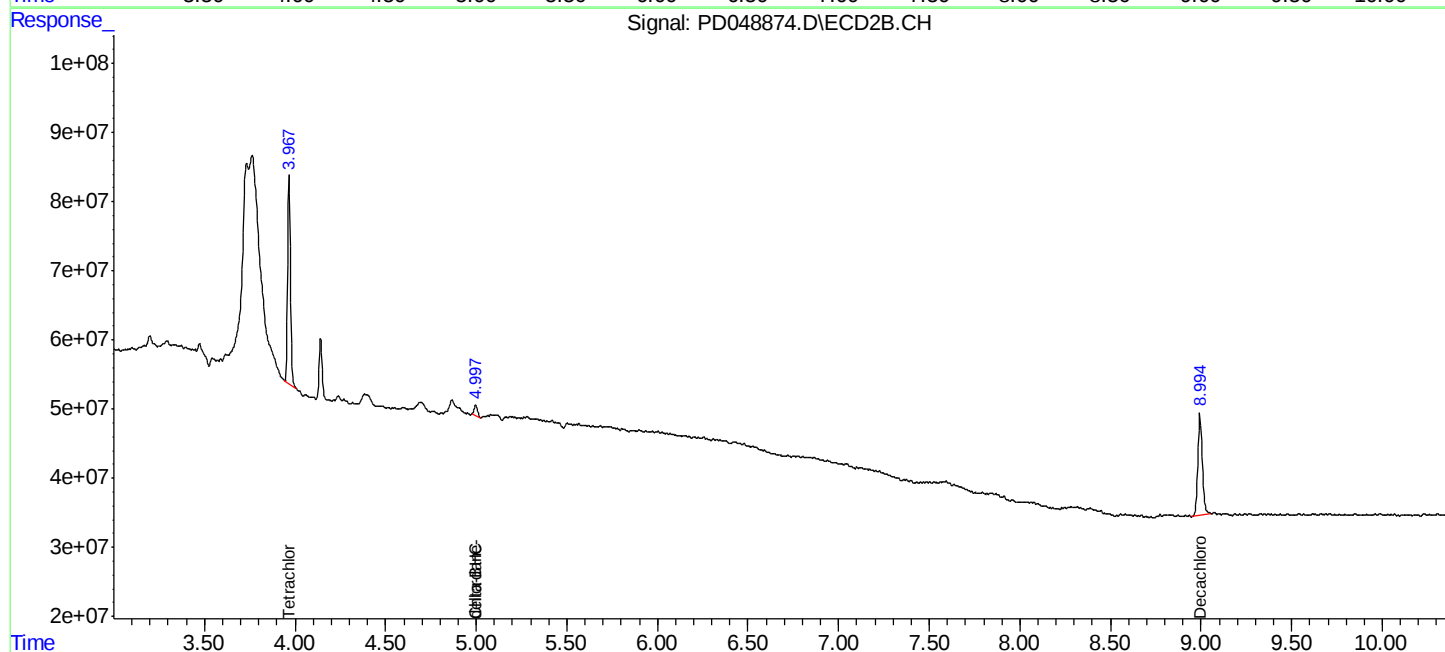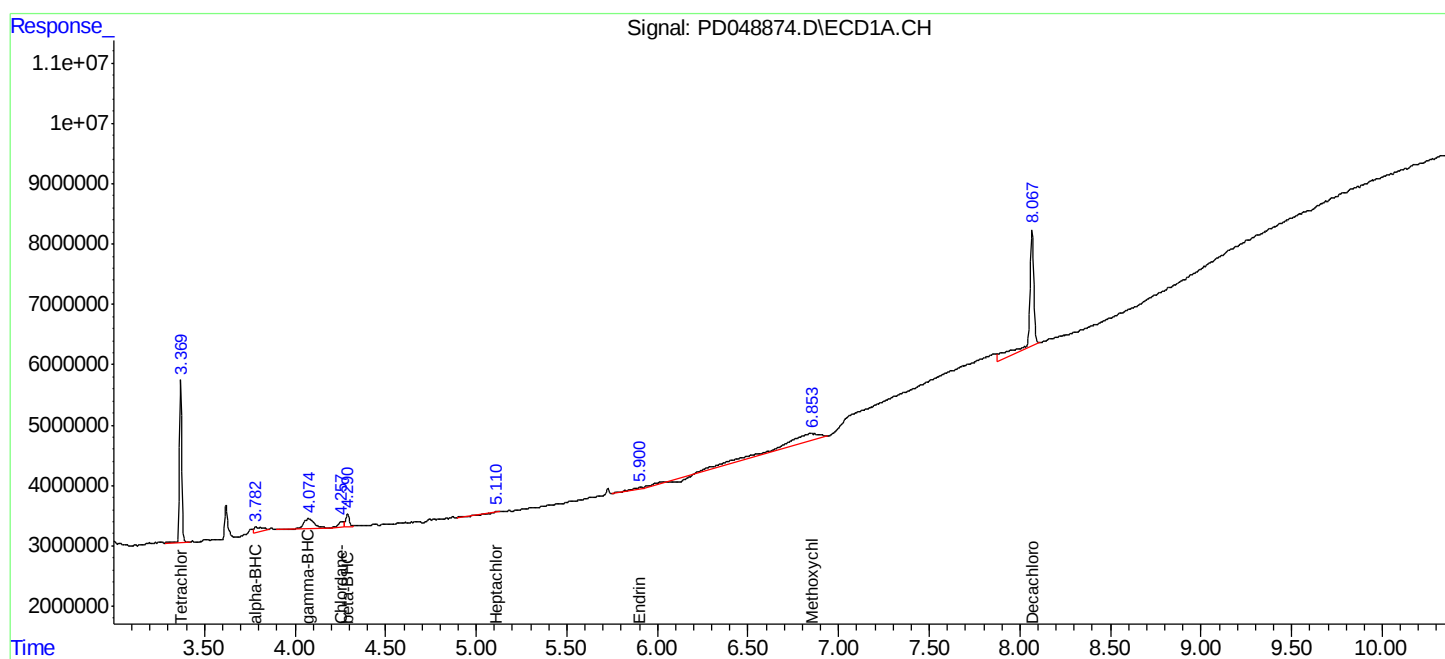


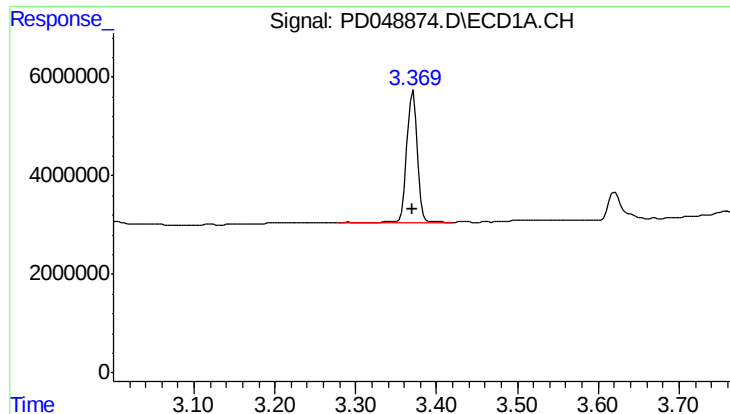

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 24014657
Conc: 21.66 ng/ml

Instrument :
ECD_D
ClientSampleId :

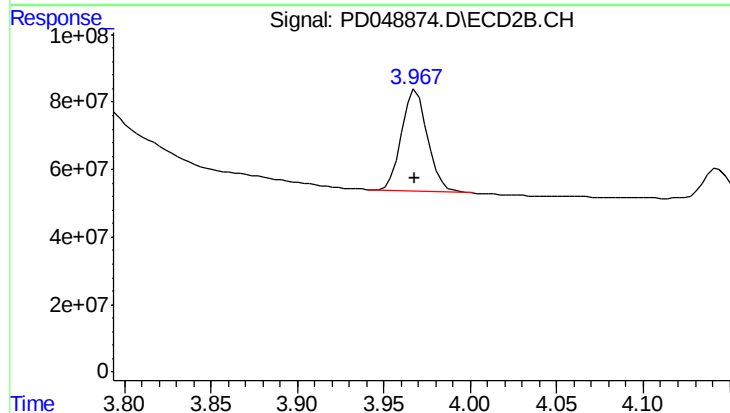


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 312352513
Conc: 23.27 ng/ml

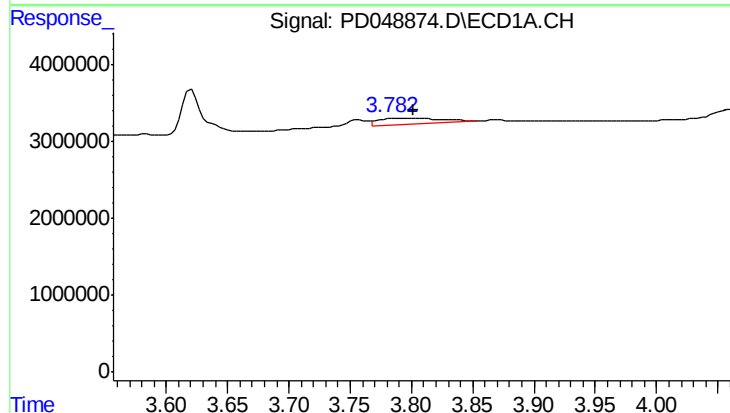


#2 alpha-BHC

R.T.: 3.785 min
Delta R.T.: -0.017 min
Response: 2635551
Conc: 1.38 ng/ml

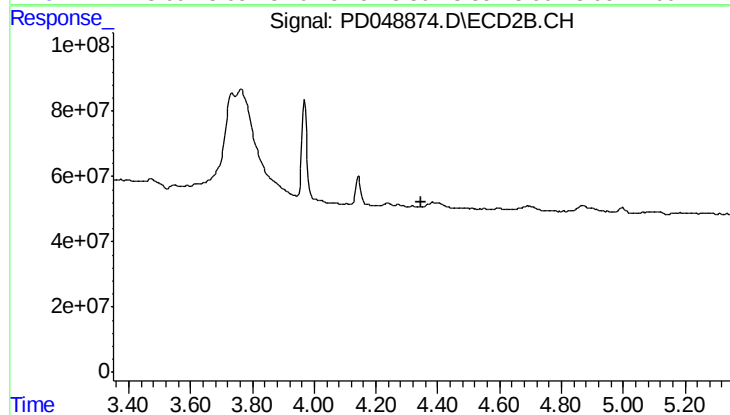

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

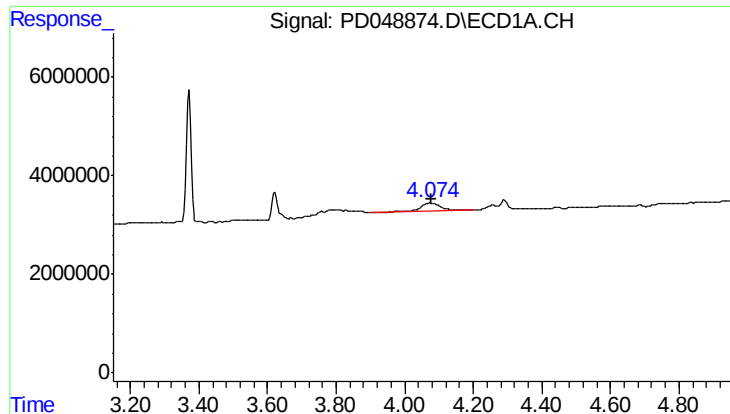

#3 gamma-BHC (Lindane)


R.T.: 4.076 min
Delta R.T.: -0.004 min
Response: 6683509
Conc: 3.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

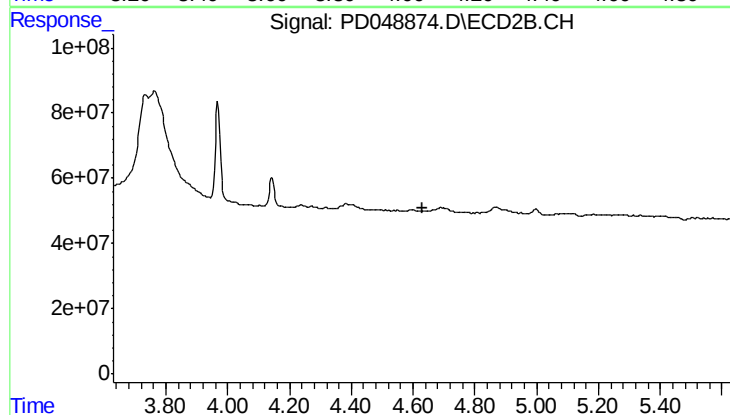


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.630 min
Response: 0
Conc: N.D.

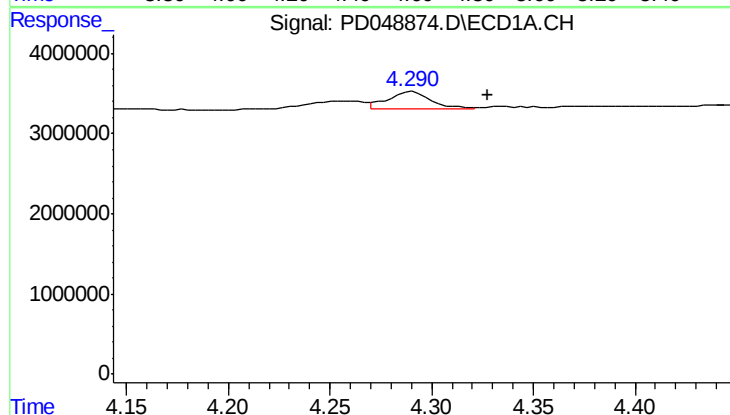


#6 beta-BHC

R.T.: 4.291 min
Delta R.T.: -0.037 min
Response: 3166638
Conc: 4.44 ng/ml

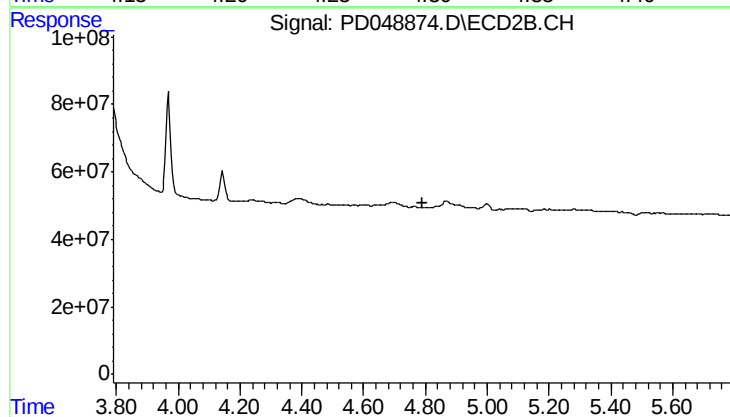

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

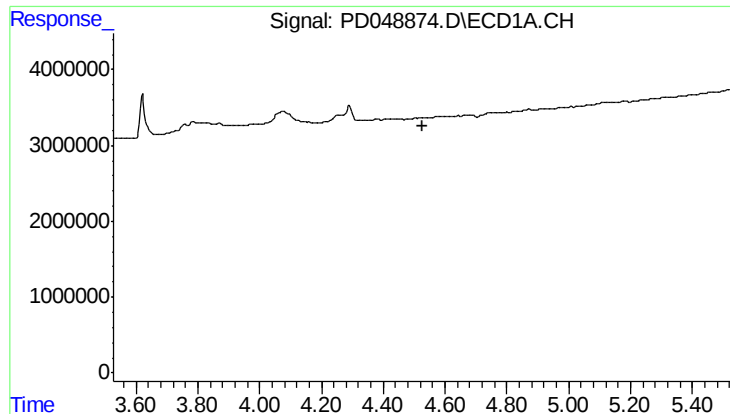

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

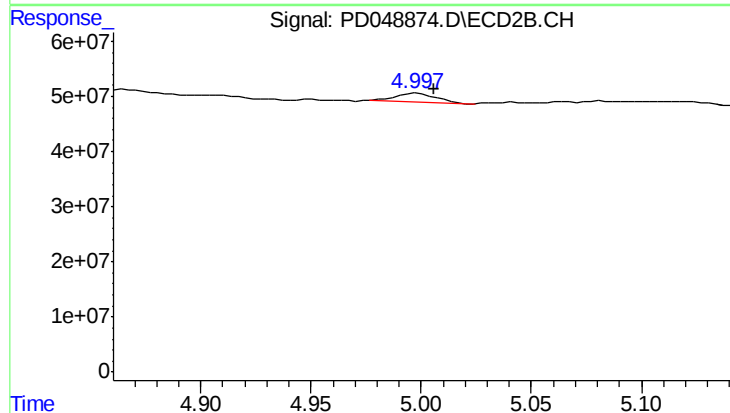


#7 delta-BHC

R.T.: 4.998 min
Delta R.T.: -0.008 min
Response: 20110575
Conc: 1.07 ng/ml

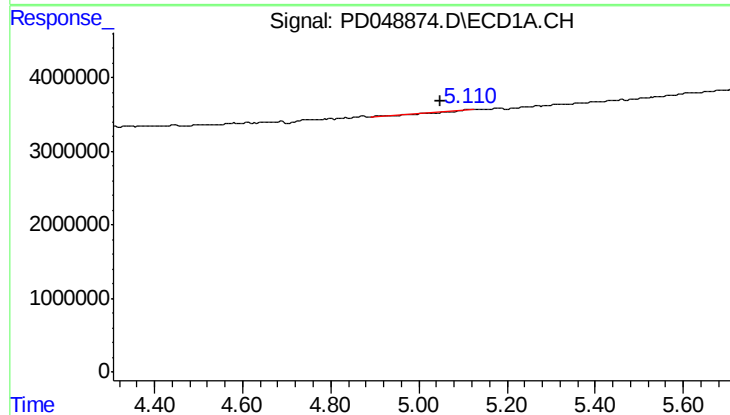


#8 Heptachlor epoxide

R.T.: 5.111 min
Delta R.T.: 0.062 min
Response: 550130
Conc: 0.36 ng/ml

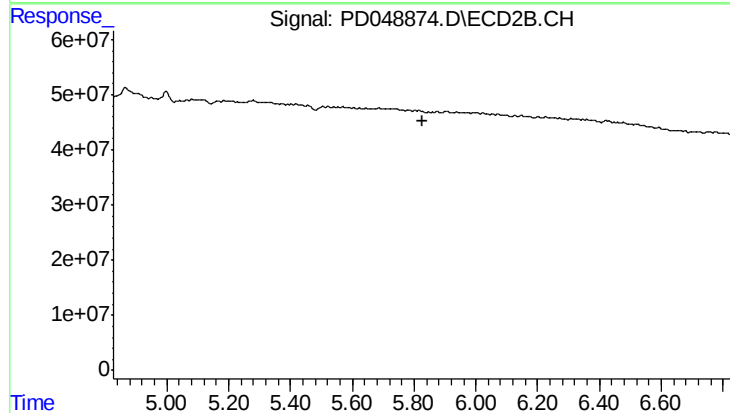

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.826 min
Response: 0
Conc: N.D.

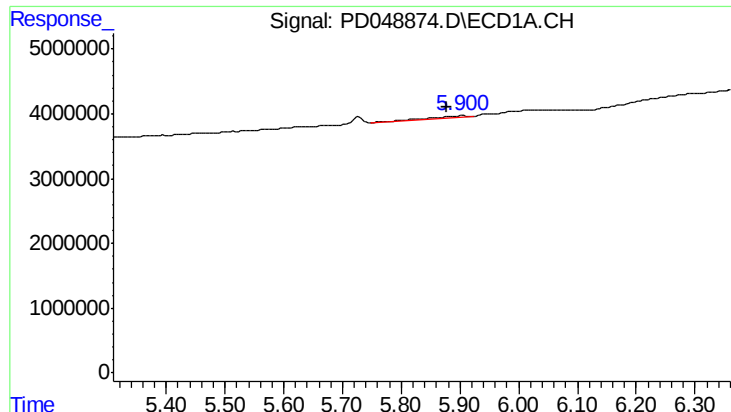

#14 Endrin


R.T.: 5.904 min
Delta R.T.: 0.026 min
Response: 957930
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

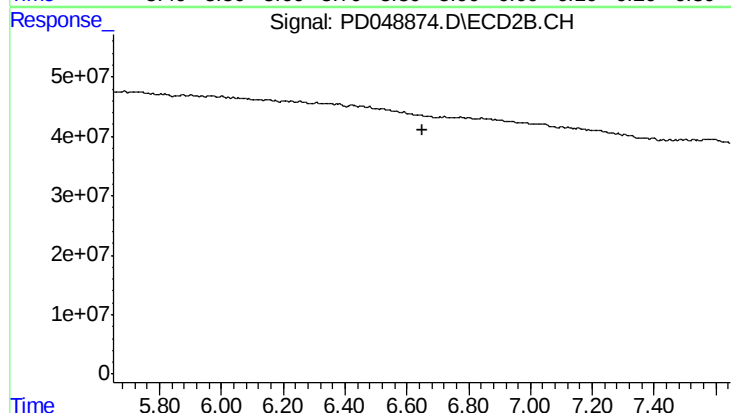


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.649 min
Response: 0
Conc: N.D.

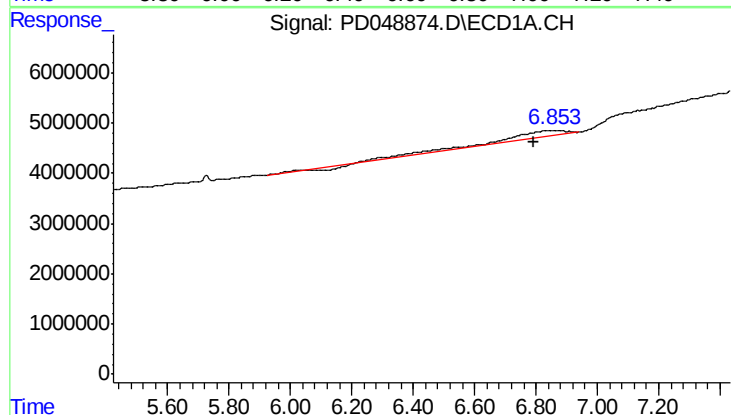


#20 Methoxychlor

R.T.: 6.853 min
Delta R.T.: 0.058 min
Response: 19658258
Conc: 25.24 ng/ml

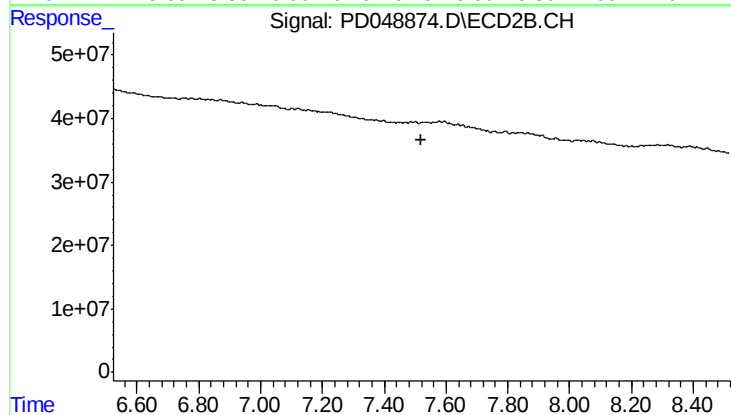

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

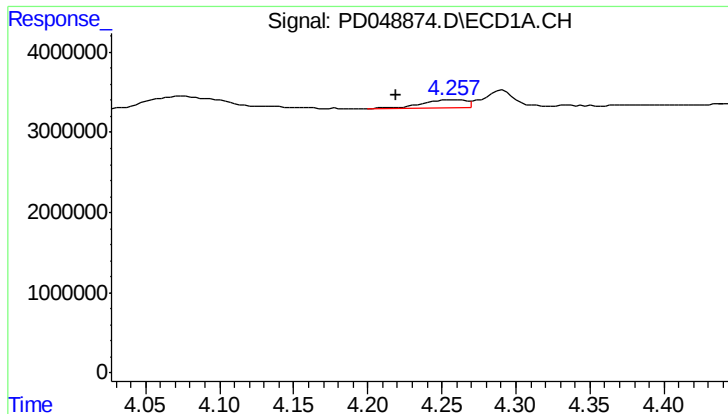

#23 Chlordane-1


R.T.: 4.258 min
Delta R.T.: 0.038 min
Response: 2021001
Conc: 40.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

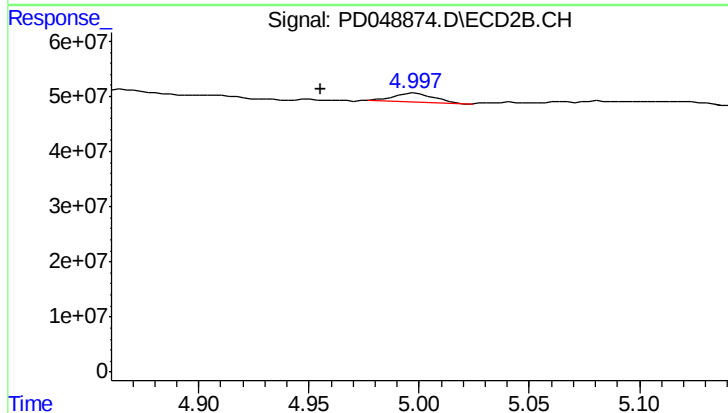


#23 Chlordane-1

R.T.: 4.998 min
Delta R.T.: 0.043 min
Response: 20110575
Conc: 27.39 ng/ml

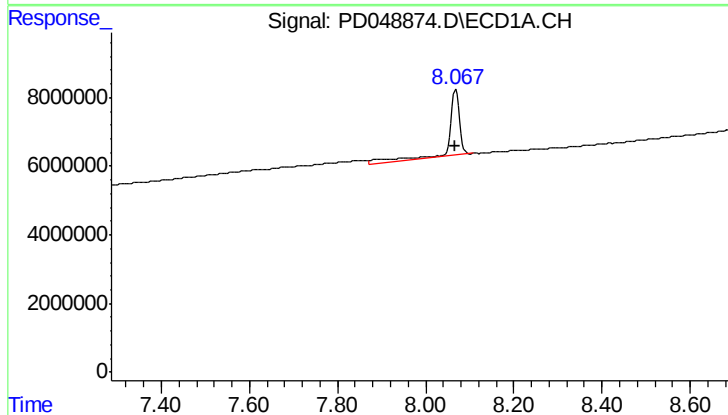

#28 Decachlorobiphenyl

R.T.: 8.069 min
Delta R.T.: 0.001 min
Response: 31662731
Conc: 22.61 ng/ml

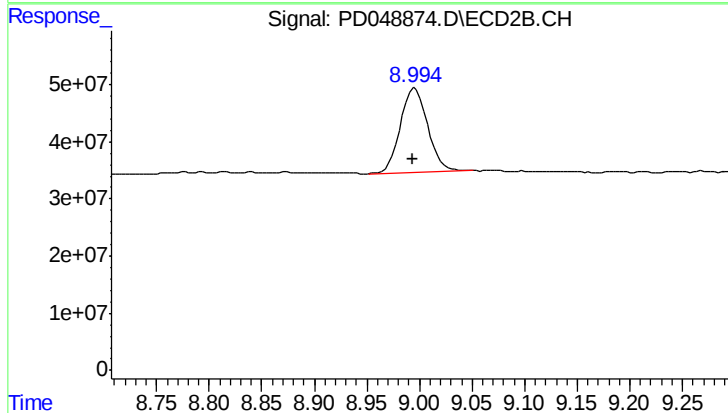

#28 Decachlorobiphenyl

R.T.: 8.996 min
Delta R.T.: 0.002 min
Response: 268089280
Conc: 17.75 ng/ml