

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048884.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 20:12
 Operator : AJ\SJ
 Sample : J4447-25
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:19:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.969	21081004	281.5E6	19.016	20.968
28)	SA Decachlor...	8.068	8.995	111.4E6	267.3E6	79.536	17.697 #
Target Compounds							
2)	A alpha-BHC	3.796	0.000	5393603	0	2.815	N.D. #
3)	MA gamma-BHC...	4.081	0.000	7917391	0	4.365	N.D. #
6)	B beta-BHC	4.291f	0.000	4496176	0	6.300	N.D. #
7)	B delta-BHC	0.000	4.997	0	20307716	N.D.	1.084 #
15)	B Endosulfa...	6.175	0.000	1469117	0	1.019	N.D. #
20)	A Methoxychlor	6.797	7.520	33170755	14971195	42.585	2.481 #
23)	Chlordane-1	0.000	4.997	0	20307716	N.D.	27.656 #
27)	Chlordane-5	6.175	0.000	1469117	0	26.760	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048884.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 20:12
Operator : AJ\SJ
Sample : J4447-25
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:19:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

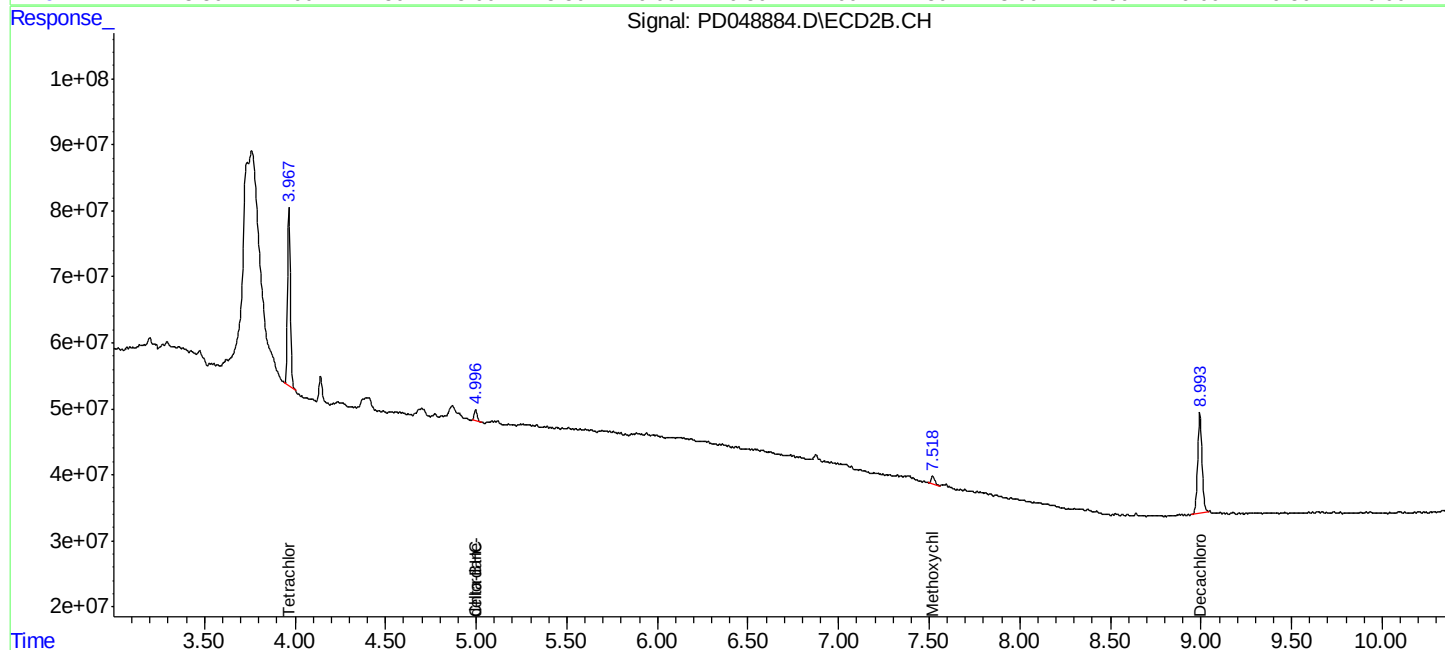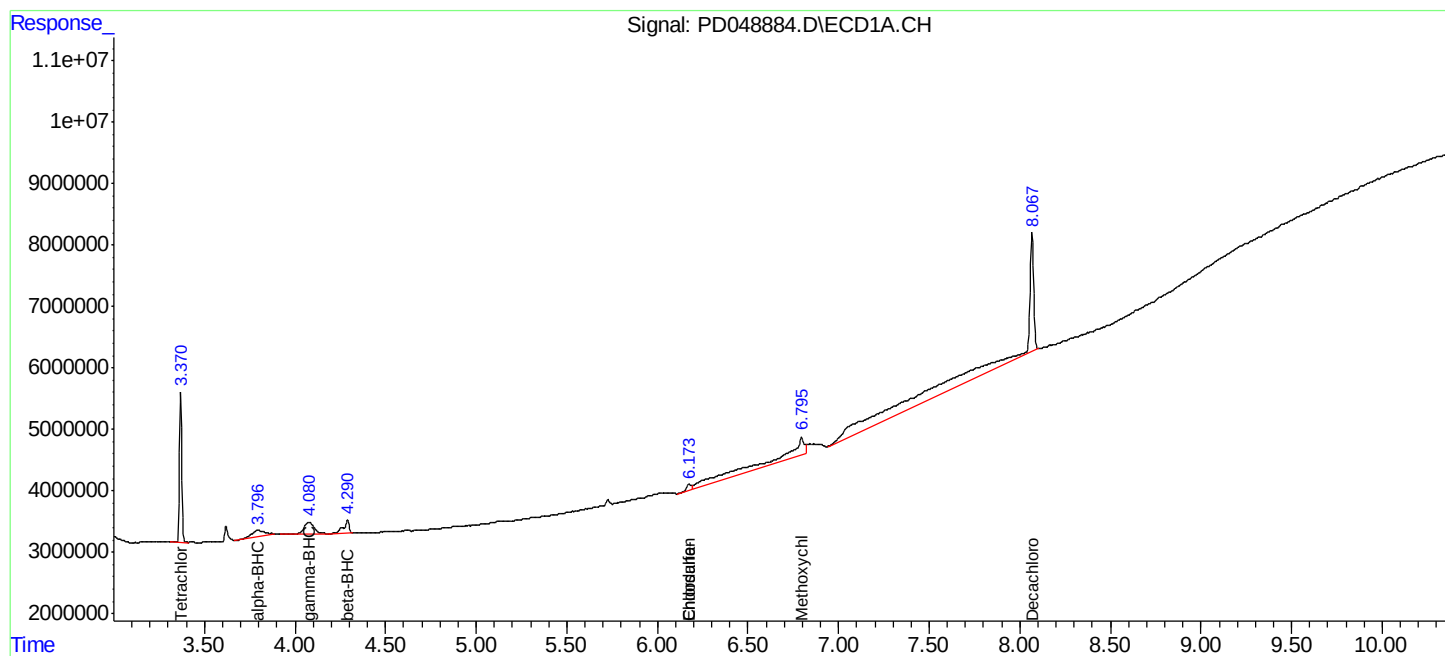


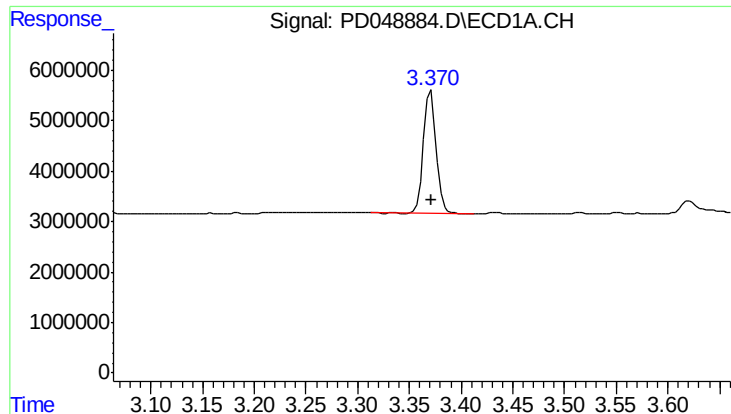

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 21081004
Conc: 19.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

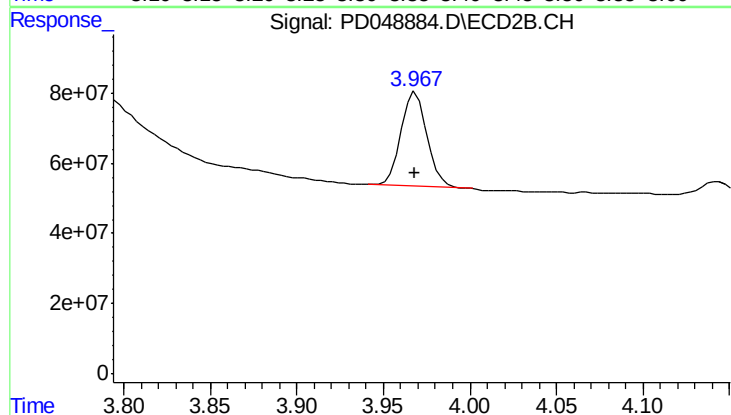


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 281472471
Conc: 20.97 ng/ml

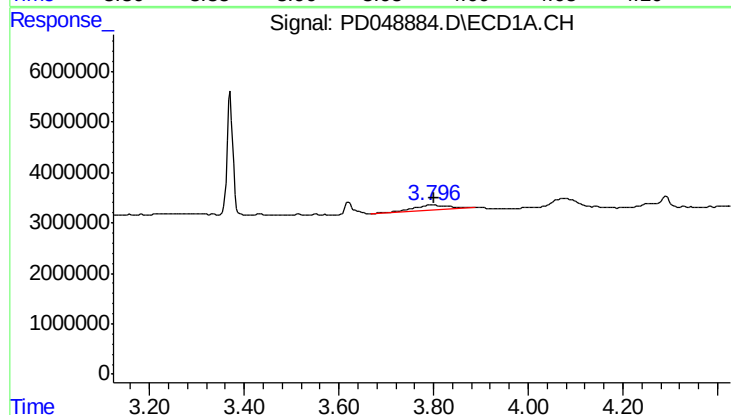


#2 alpha-BHC

R.T.: 3.796 min
Delta R.T.: -0.005 min
Response: 5393603
Conc: 2.82 ng/ml

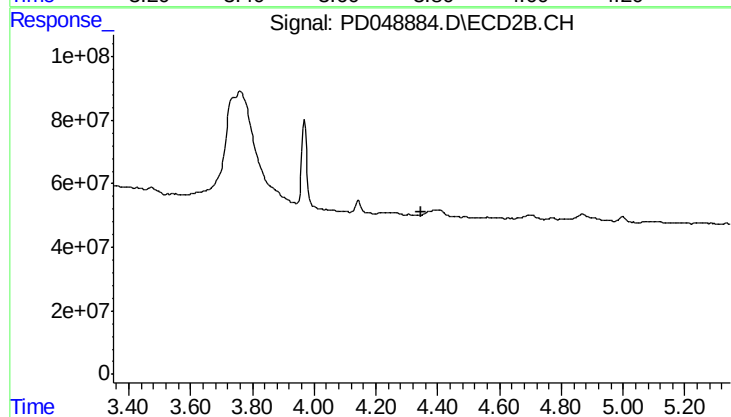

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

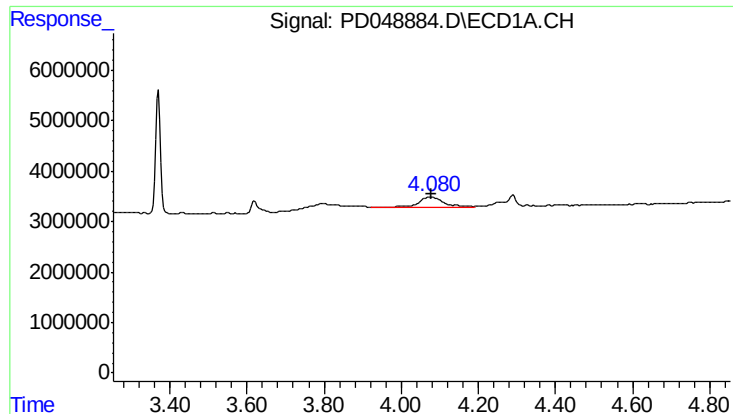

#3 gamma-BHC (Lindane)


R.T.: 4.081 min
Delta R.T.: 0.001 min
Response: 7917391
Conc: 4.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

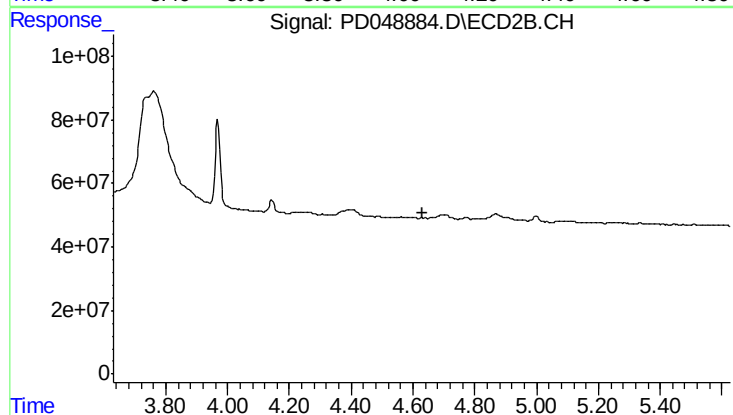


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.630 min
Response: 0
Conc: N.D.

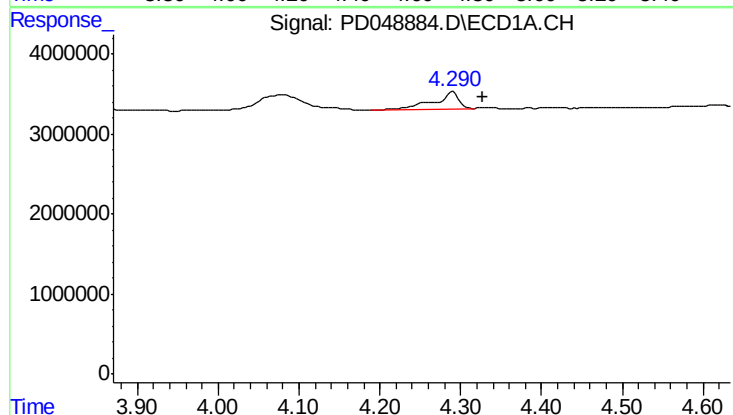


#6 beta-BHC

R.T.: 4.291 min
Delta R.T.: -0.037 min
Response: 4496176
Conc: 6.30 ng/ml

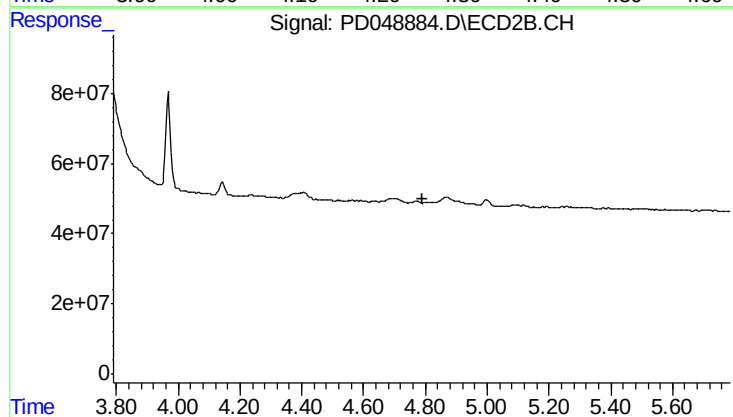

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

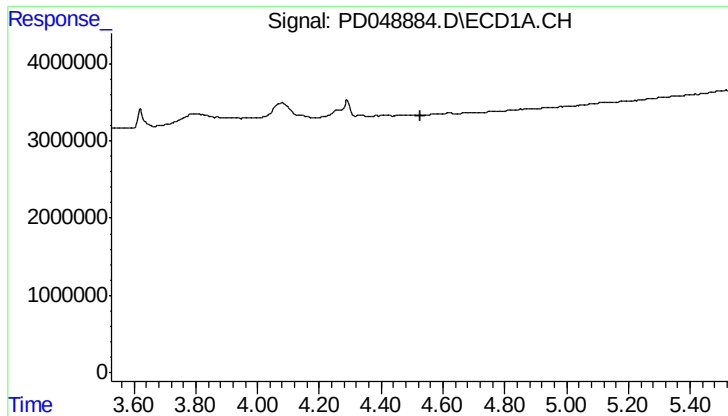

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

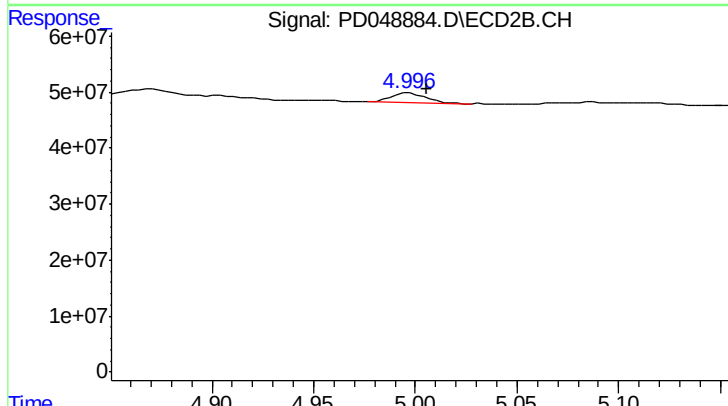


#7 delta-BHC

R.T.: 4.997 min
Delta R.T.: -0.009 min
Response: 20307716
Conc: 1.08 ng/ml

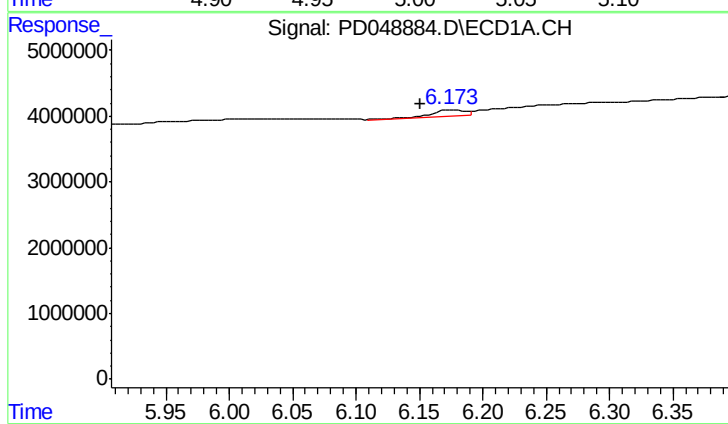


#15 Endosulfan II

R.T.: 6.175 min
Delta R.T.: 0.024 min
Response: 1469117
Conc: 1.02 ng/ml

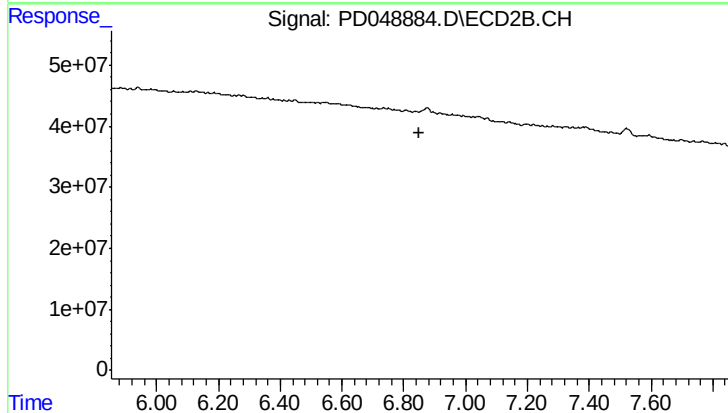

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.851 min
Response: 0
Conc: N.D.

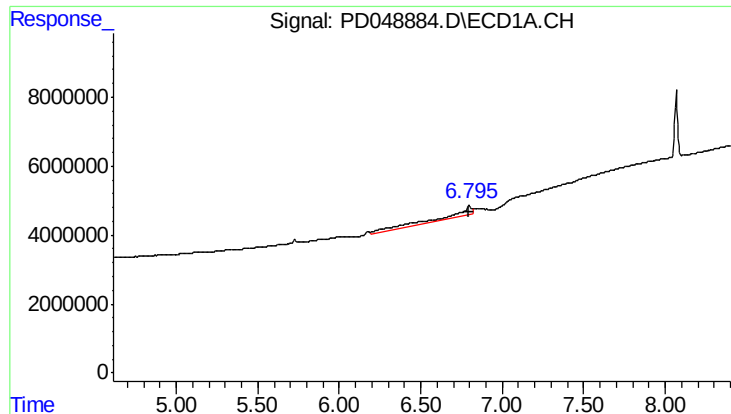

#20 Methoxychlor


R.T.: 6.797 min
Delta R.T.: 0.001 min
Response: 33170755
Conc: 42.58 ng/ml

Instrument :
ECD_D
ClientSampleId :

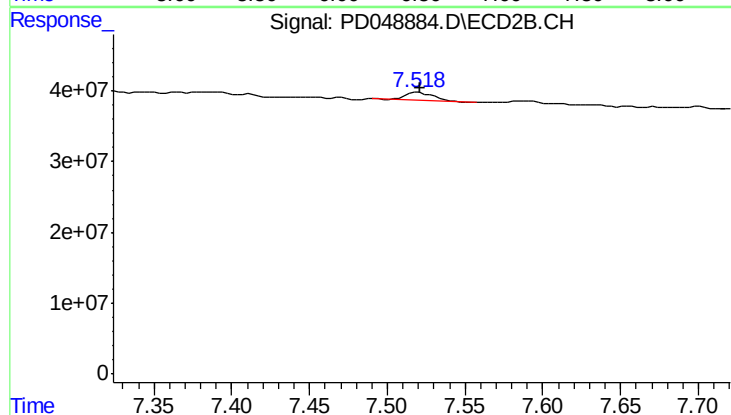


#20 Methoxychlor

R.T.: 7.520 min
Delta R.T.: 0.000 min
Response: 14971195
Conc: 2.48 ng/ml

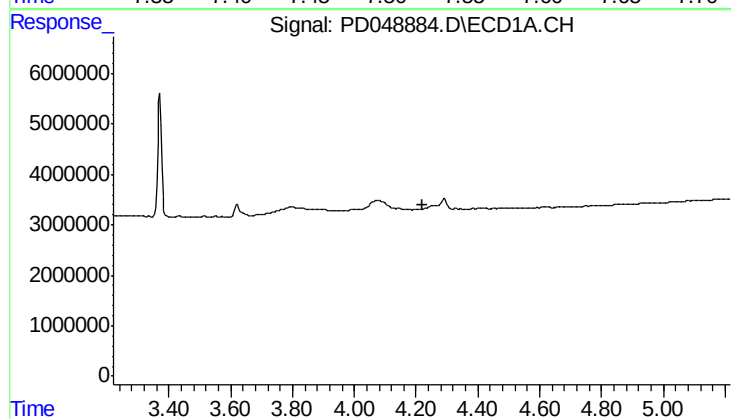


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.220 min
Response: 0
Conc: N.D.

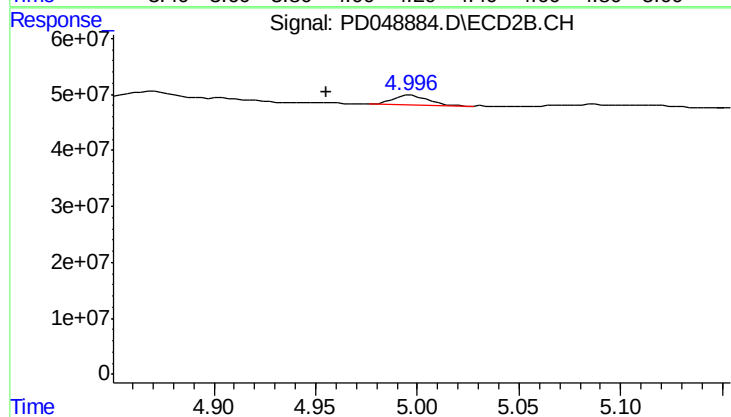

#23 Chlordane-1


R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 20307716
Conc: 27.66 ng/ml

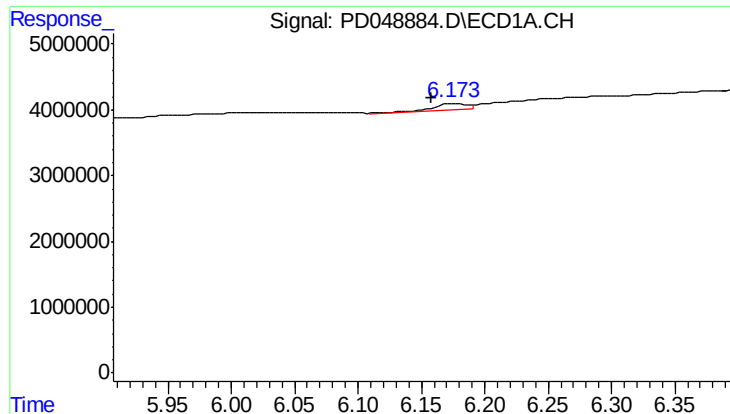

#27 Chlordane-5


R.T.: 6.175 min
Delta R.T.: 0.017 min
Response: 1469117
Conc: 26.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

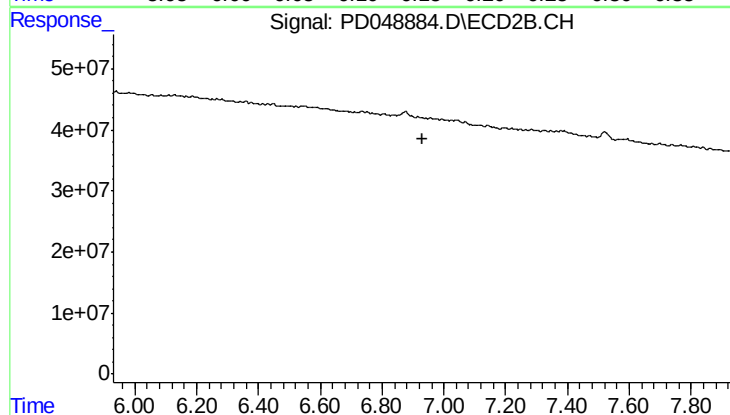


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.929 min
Response: 0
Conc: N.D.

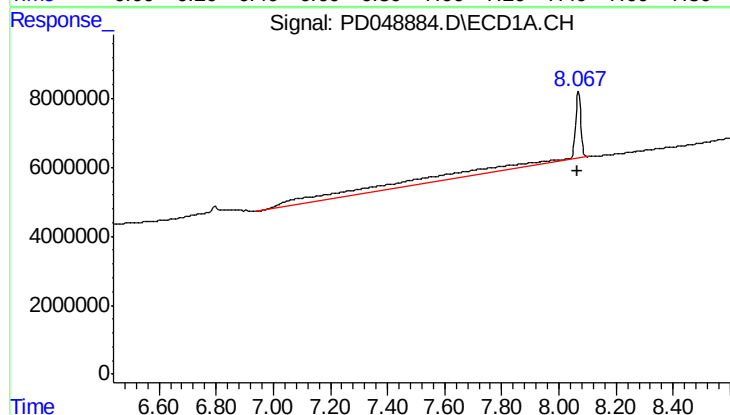

#28 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.001 min
Response: 111372752
Conc: 79.54 ng/ml

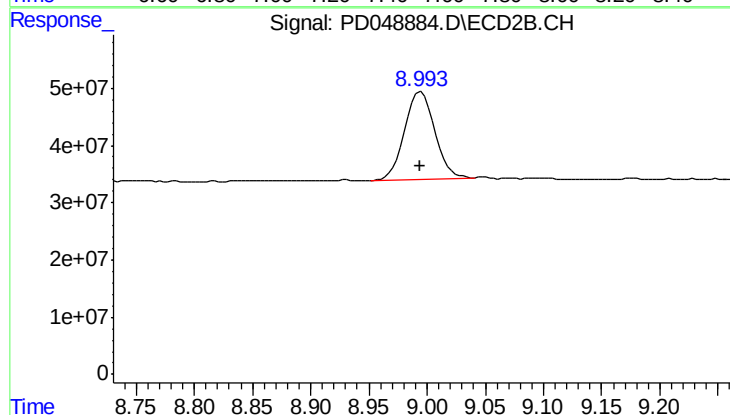

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 267281186
Conc: 17.70 ng/ml