

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048885.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 20:26
 Operator : AJ\SJ
 Sample : J4447-45
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:19:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.969	23011713	289.0E6	20.757	21.530
28)	SA Decachlor...	8.068	8.995	113.7E6	271.7E6	81.176	17.987 #
Target Compounds							
2)	A alpha-BHC	3.798	0.000	5394136	0	2.815	N.D. #
3)	MA gamma-BHC...	4.080	0.000	7736549	0	4.265	N.D. #
6)	B beta-BHC	4.290f	0.000	4895956	0	6.860	N.D. #
7)	B delta-BHC	0.000	5.000	0	23361140	N.D.	1.247 #
15)	B Endosulfa...	6.176	0.000	1231097	0	0.854	N.D. #
16)	A 4,4'-DDD	6.065f	0.000	5288757	0	3.772	N.D. #
20)	A Methoxychlor	6.796	7.522	32666082	17540185	41.937	2.907 #
23)	Chlordane-1	0.000	5.000	0	23361140	N.D.	31.814 #
27)	Chlordane-5	6.176	0.000	1231097	0	22.425	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048885.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 20:26
Operator : AJ\SJ
Sample : J4447-45
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:19:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

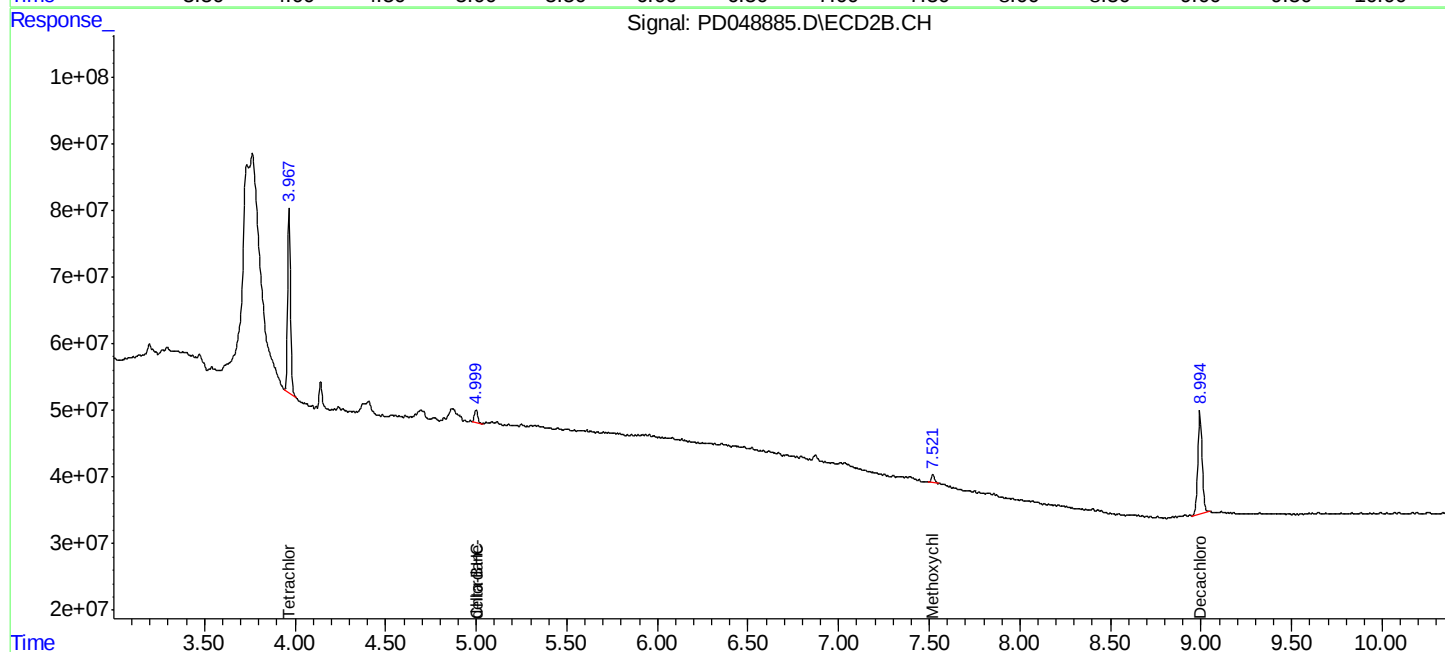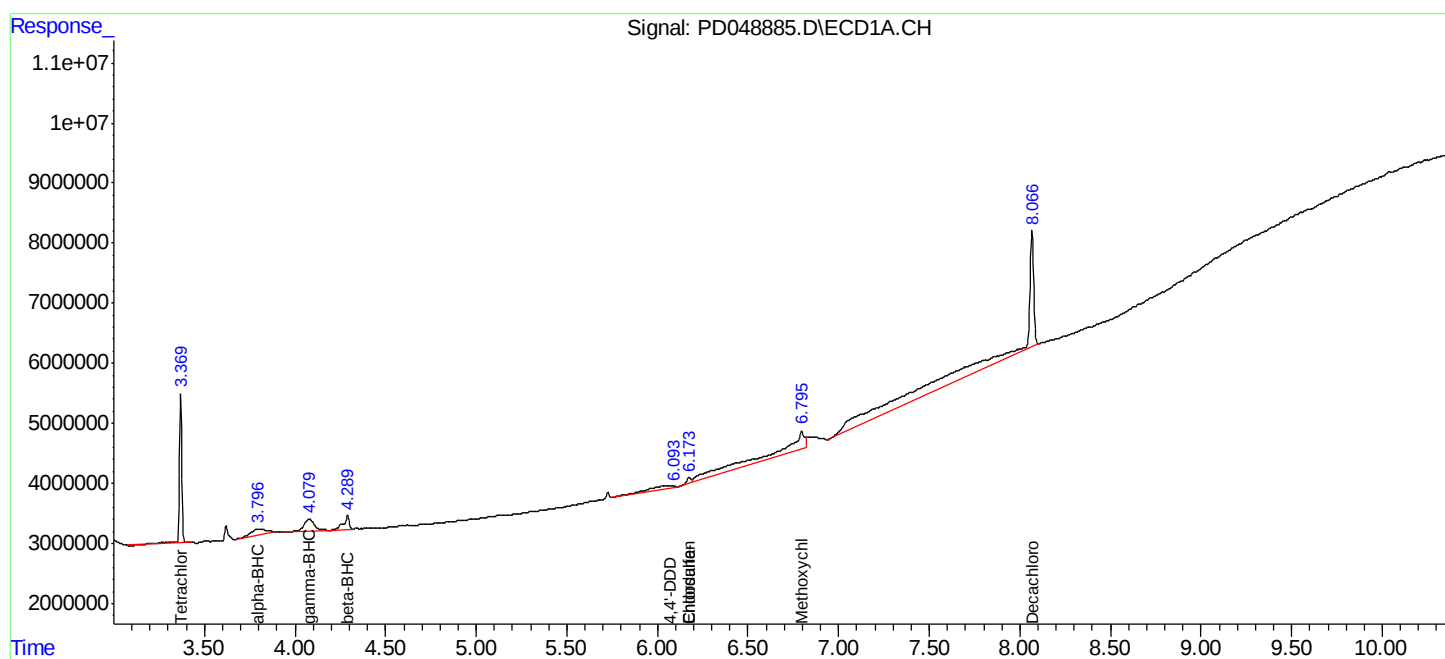


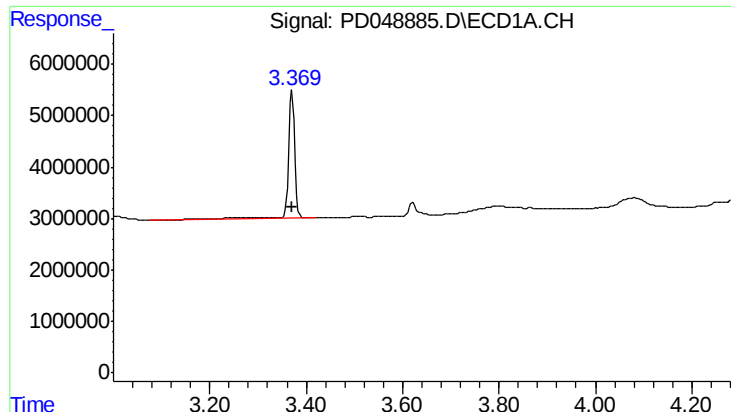

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 23011713
Conc: 20.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

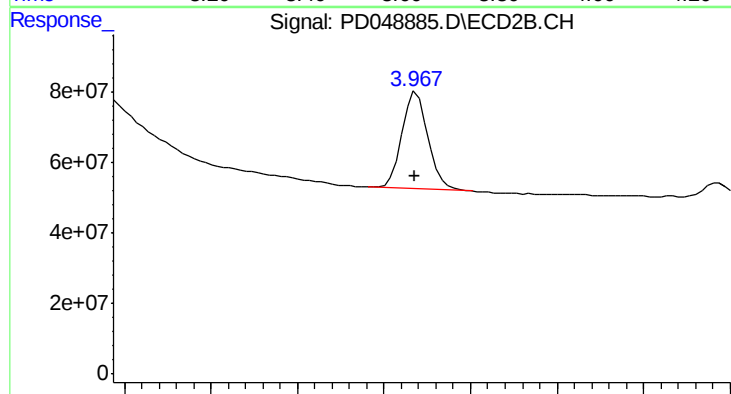


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 289020351
Conc: 21.53 ng/ml

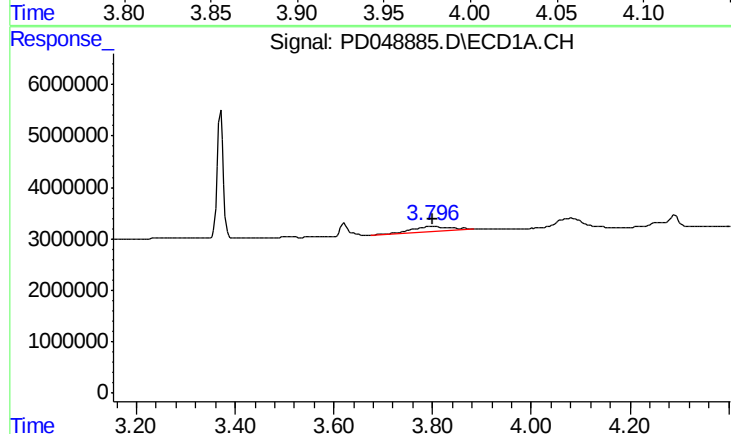


#2 alpha-BHC

R.T.: 3.798 min
Delta R.T.: -0.003 min
Response: 5394136
Conc: 2.82 ng/ml

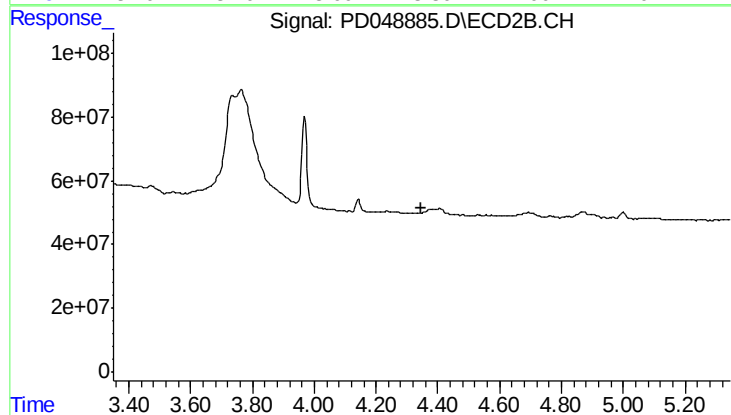

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

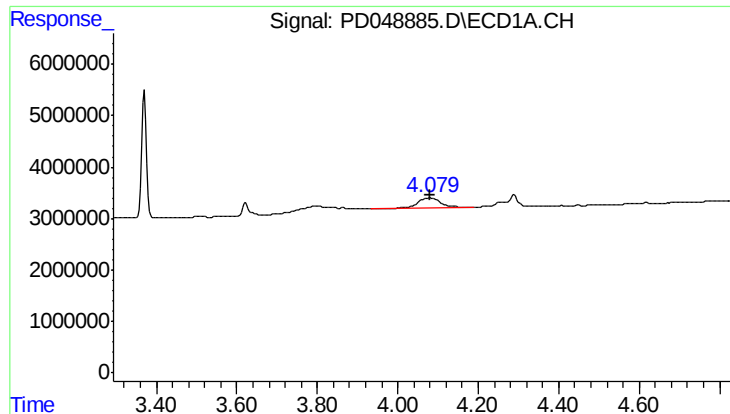

#3 gamma-BHC (Lindane)


R.T.: 4.080 min
Delta R.T.: 0.001 min
Response: 7736549
Conc: 4.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

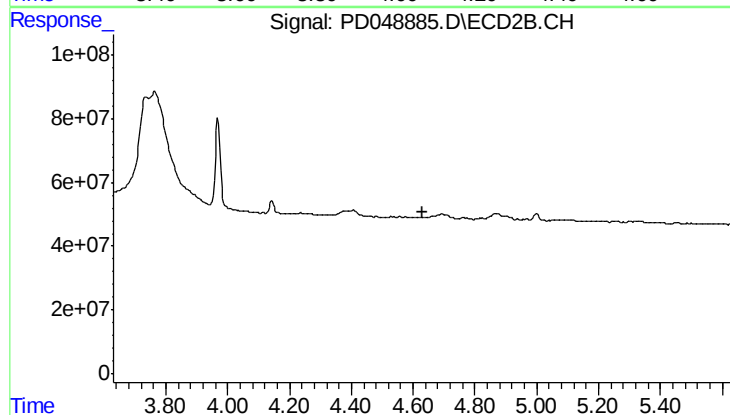


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.630 min
Response: 0
Conc: N.D.

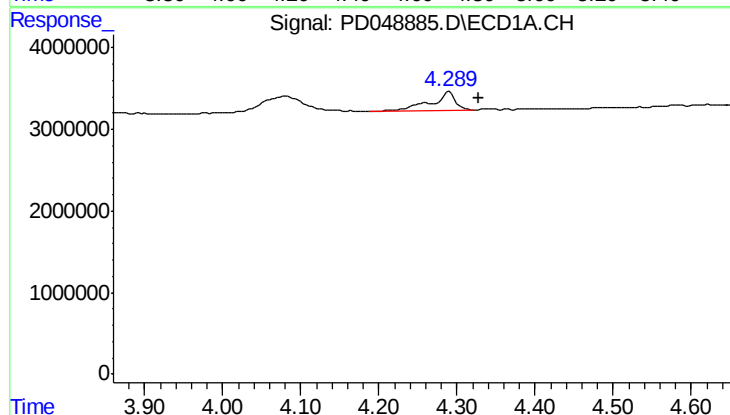


#6 beta-BHC

R.T.: 4.290 min
Delta R.T.: -0.037 min
Response: 4895956
Conc: 6.86 ng/ml

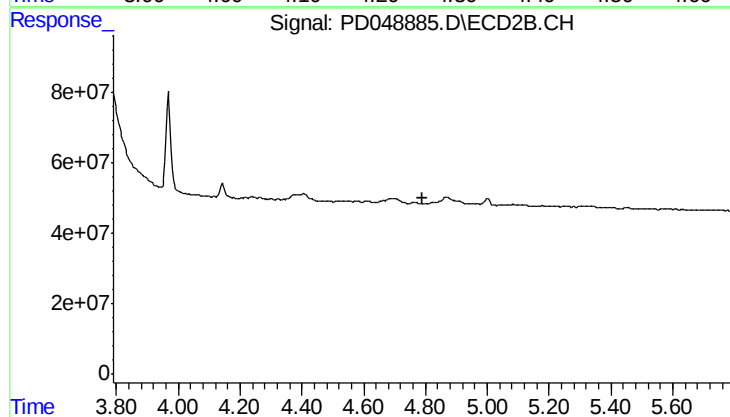

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

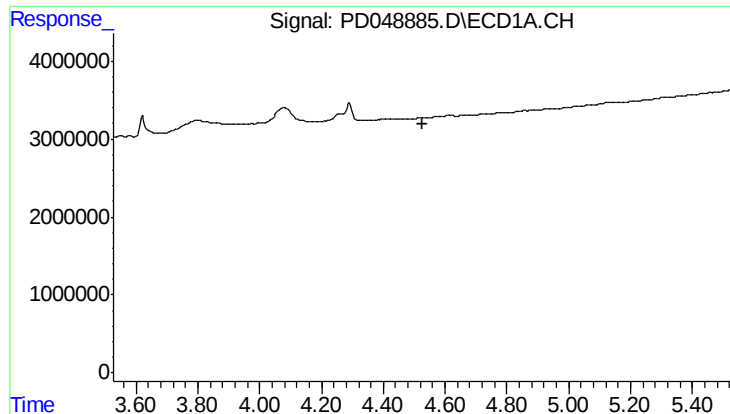

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

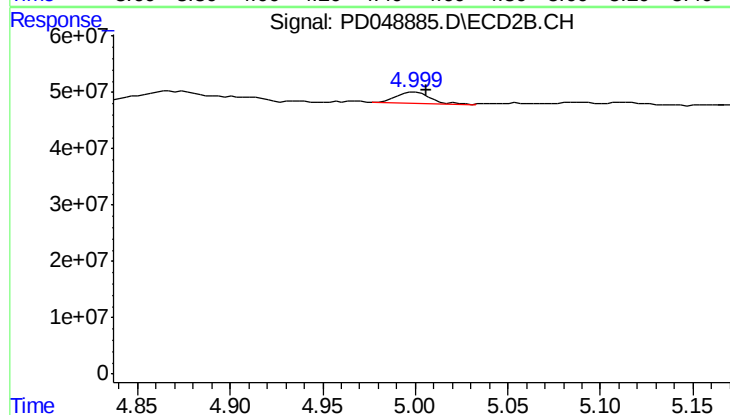


#7 delta-BHC

R.T.: 5.000 min
Delta R.T.: -0.005 min
Response: 23361140
Conc: 1.25 ng/ml

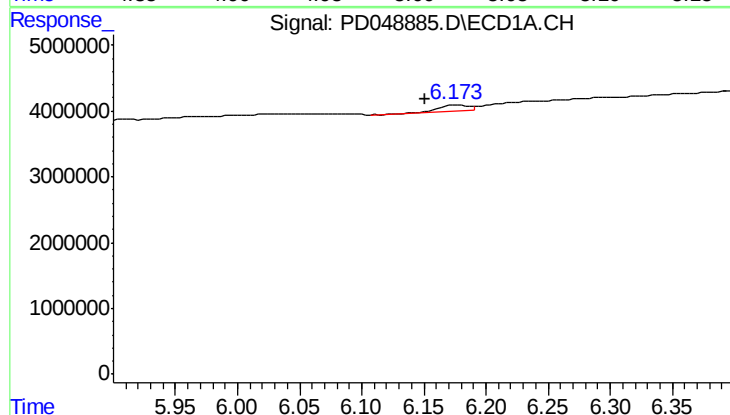


#15 Endosulfan II

R.T.: 6.176 min
Delta R.T.: 0.025 min
Response: 1231097
Conc: 0.85 ng/ml

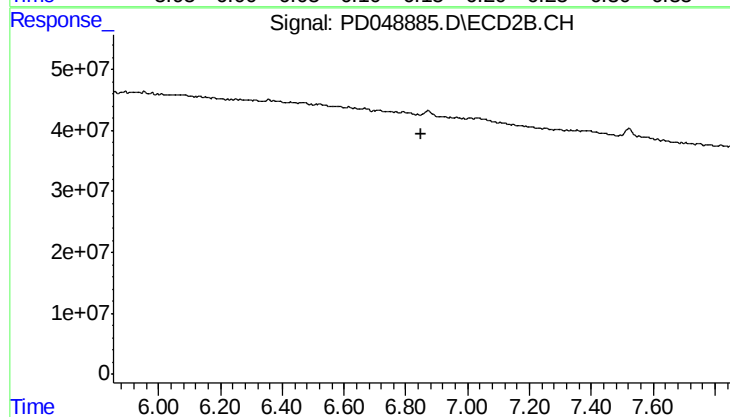

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.851 min
Response: 0
Conc: N.D.

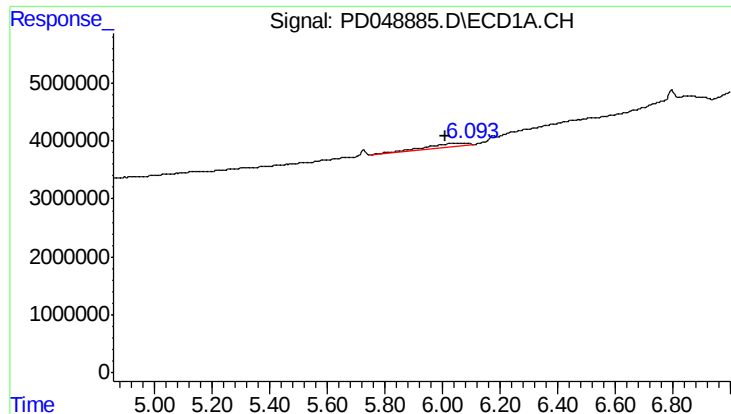

#16 4,4'-DDD


R.T.: 6.065 min
Delta R.T.: 0.056 min
Response: 5288757
Conc: 3.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

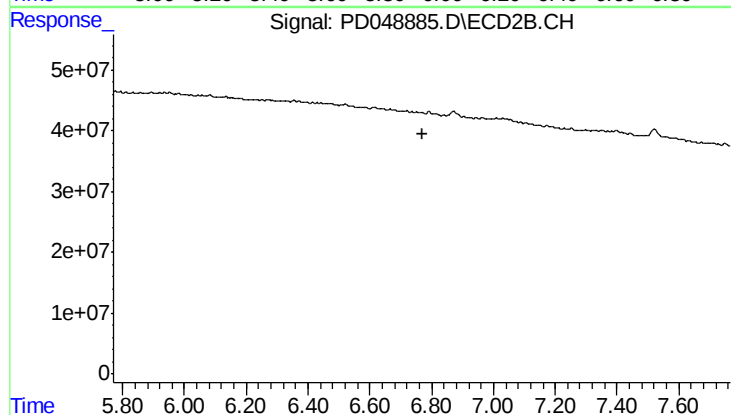


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

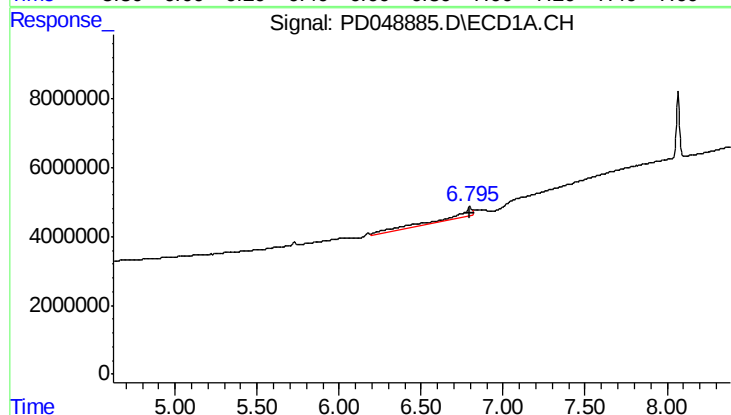


#20 Methoxychlor

R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 32666082
Conc: 41.94 ng/ml

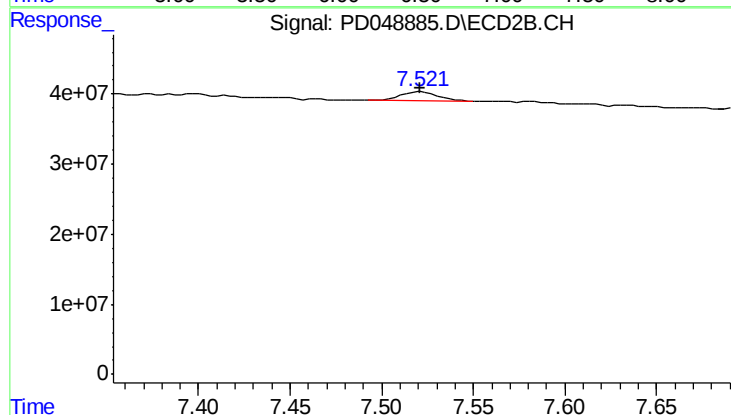

#20 Methoxychlor


R.T.: 7.522 min
Delta R.T.: 0.001 min
Response: 17540185
Conc: 2.91 ng/ml

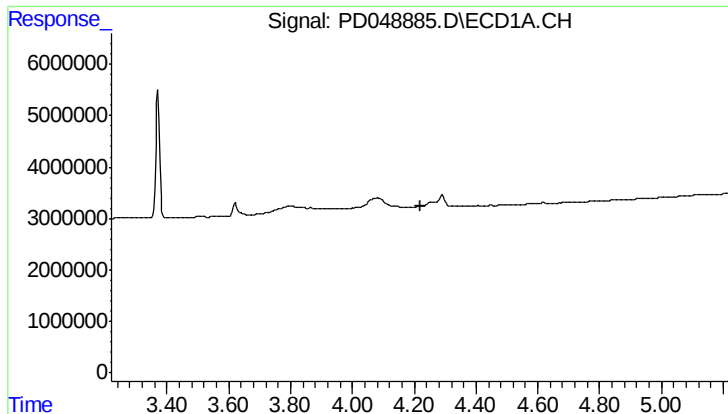

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

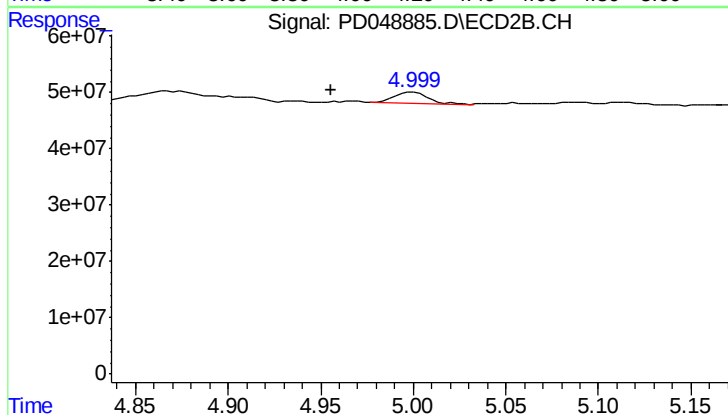


#23 Chlordane-1

R.T.: 5.000 min
Delta R.T.: 0.045 min
Response: 23361140
Conc: 31.81 ng/ml

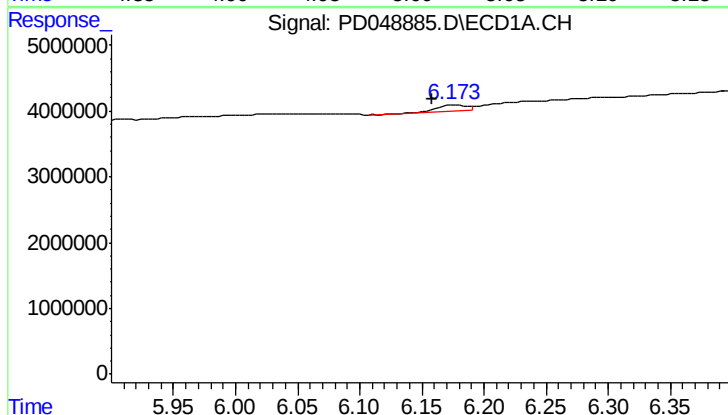


#27 Chlordane-5

R.T.: 6.176 min
Delta R.T.: 0.018 min
Response: 1231097
Conc: 22.42 ng/ml

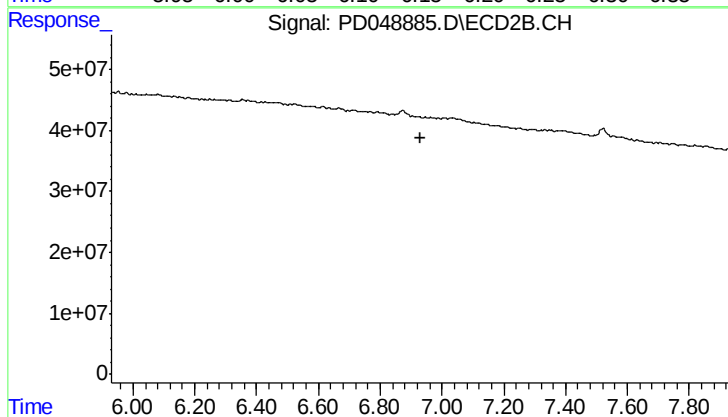

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.929 min
Response: 0
Conc: N.D.

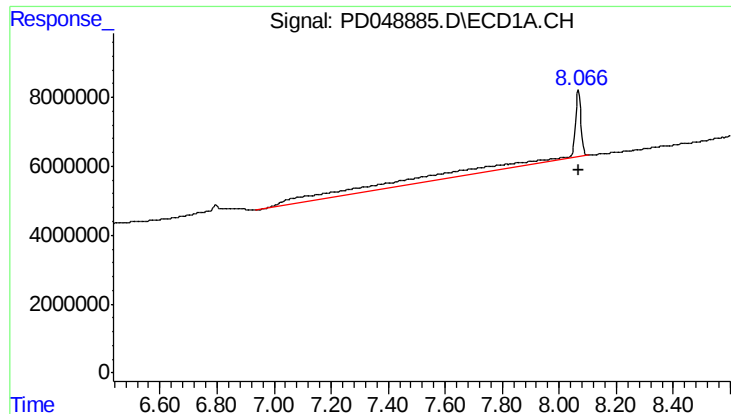

#28 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 113669313
Conc: 81.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

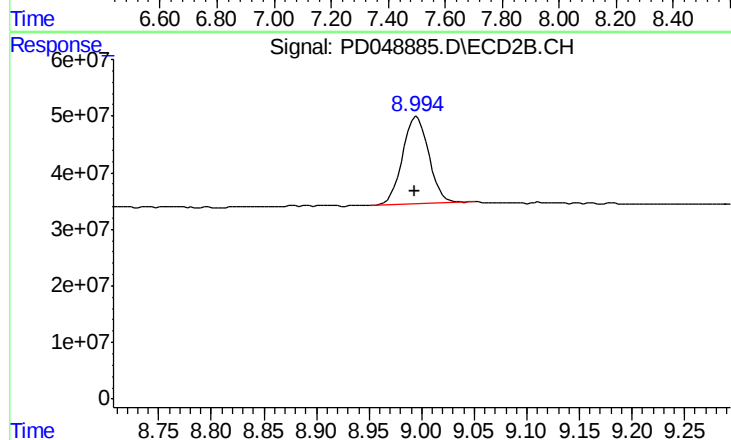

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.001 min
Response: 271657708
Conc: 17.99 ng/ml