

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 20:39
 Operator : AJ\SJ
 Sample : J4405-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:20:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.969	23503123	294.1E6	21.200	21.906
28)	SA Decachlor...	8.068	8.995	32721039	276.9E6	23.367	18.336
Target Compounds							
2)	A alpha-BHC	3.794	0.000	6282061	0	3.279	N.D. #
3)	MA gamma-BHC...	4.080	0.000	7653896	0	4.219	N.D. #
6)	B beta-BHC	4.291f	0.000	5386457	0	7.547	N.D. #
7)	B delta-BHC	0.000	4.999	0	20825341	N.D.	1.111 #
15)	B Endosulfa...	6.175	0.000	1081975	0	0.751	N.D. #
20)	A Methoxychlor	6.796	7.521	33804322	13689806	43.398	2.269 #
23)	Chlordane-1	0.000	4.999	0	20825341	N.D.	28.360 #
27)	Chlordane-5	6.175	0.000	1081975	0	19.708	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 20:39
Operator : AJ\SJ
Sample : J4405-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:20:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

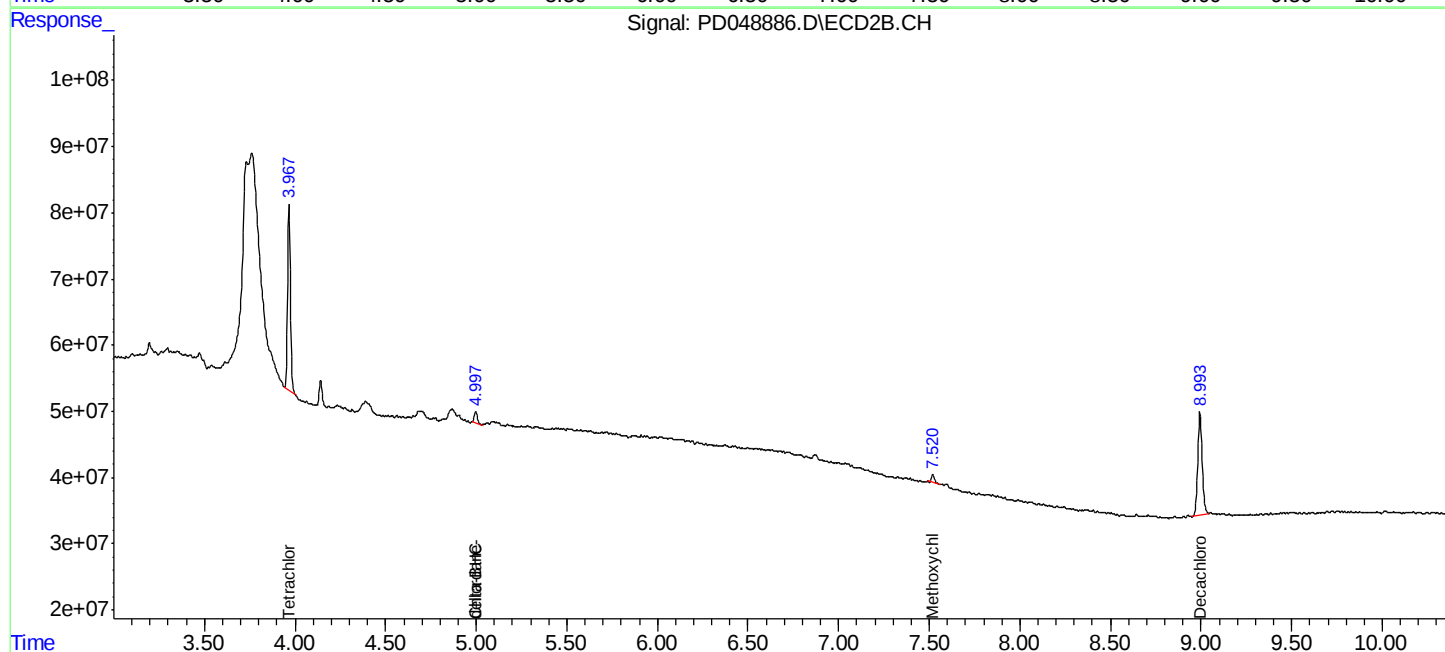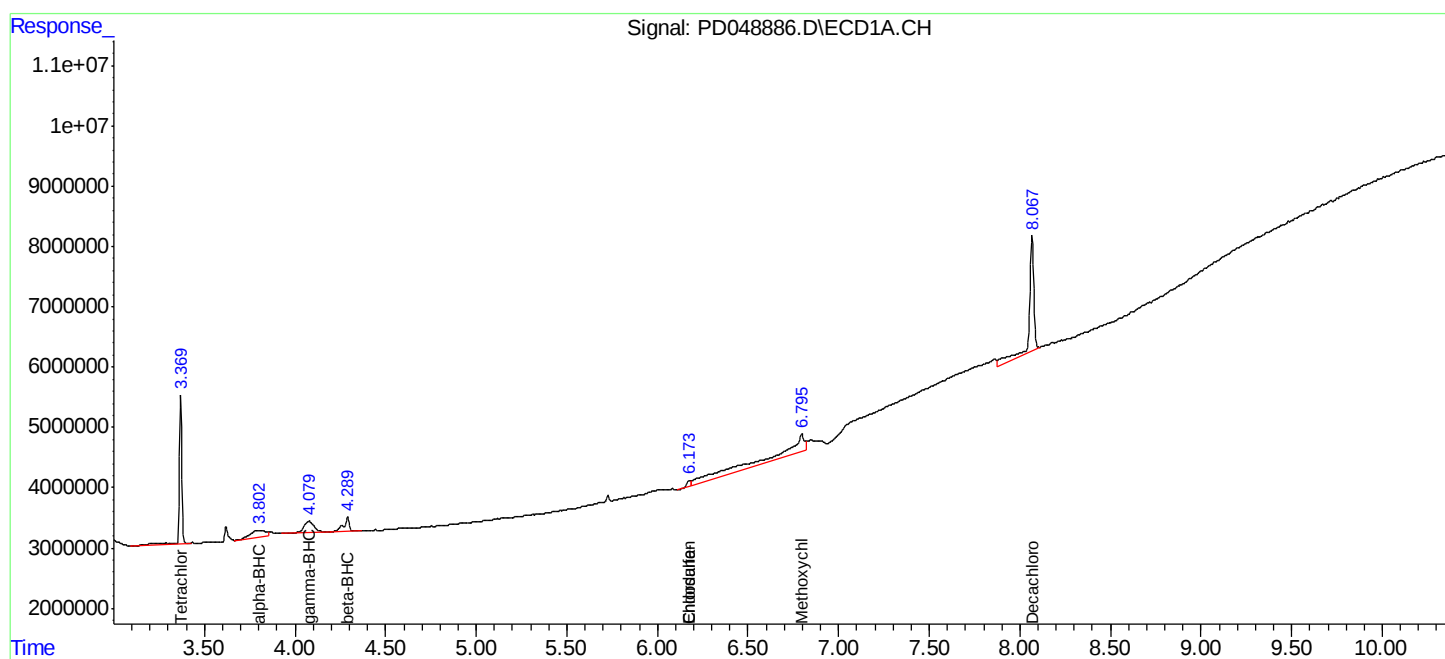


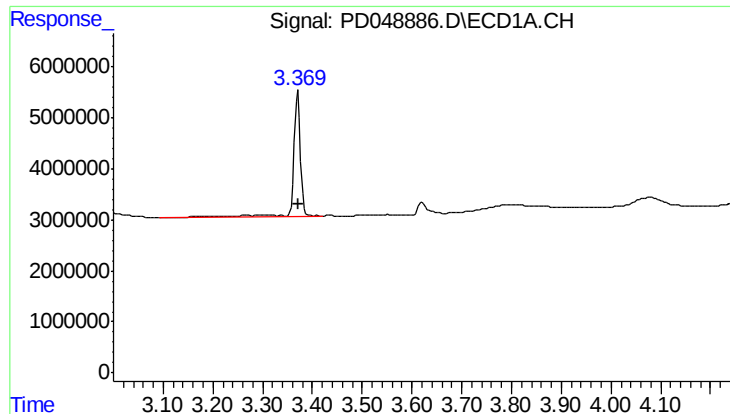

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 23503123
Conc: 21.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

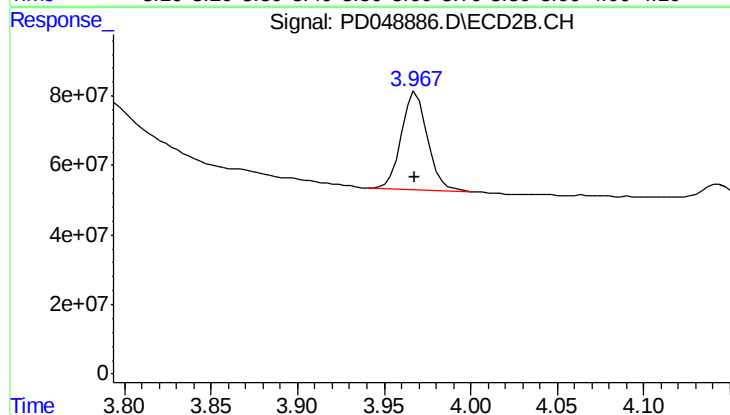


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 294066725
Conc: 21.91 ng/ml

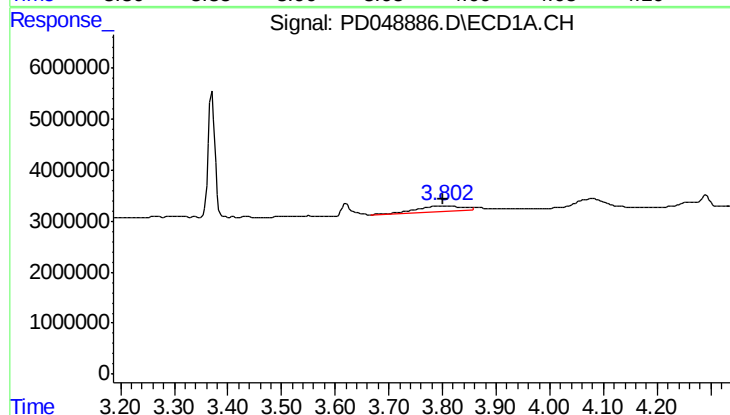


#2 alpha-BHC

R.T.: 3.794 min
Delta R.T.: -0.008 min
Response: 6282061
Conc: 3.28 ng/ml

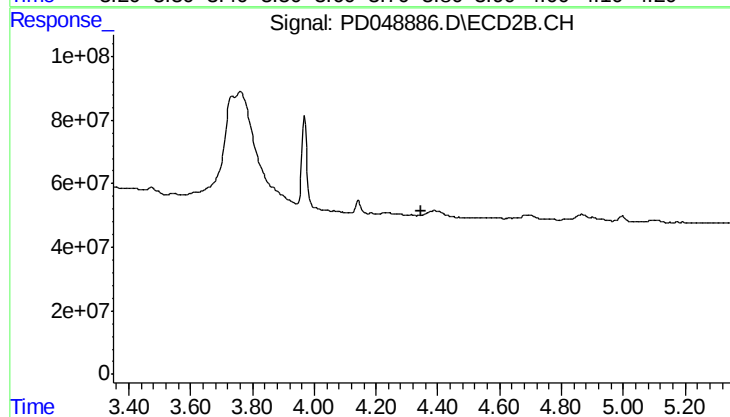

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.348 min
Response: 0
Conc: N.D.

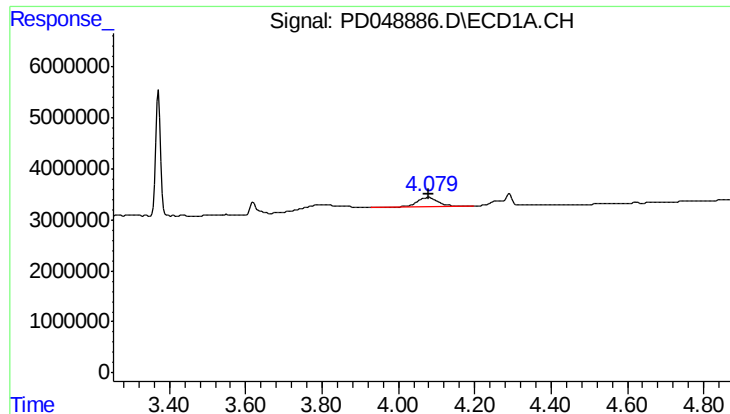

#3 gamma-BHC (Lindane)


R.T.: 4.080 min
Delta R.T.: 0.000 min
Response: 7653896
Conc: 4.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

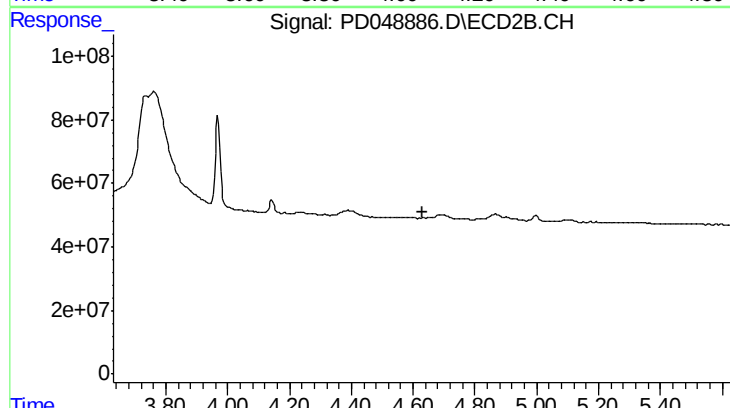


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.630 min
Response: 0
Conc: N.D.

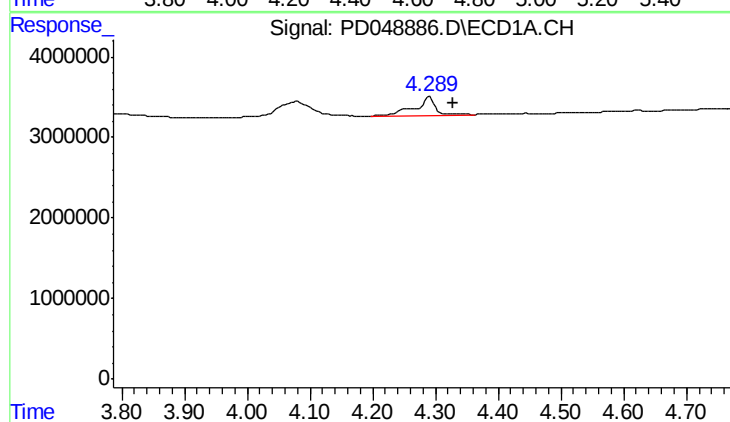


#6 beta-BHC

R.T.: 4.291 min
Delta R.T.: -0.037 min
Response: 5386457
Conc: 7.55 ng/ml

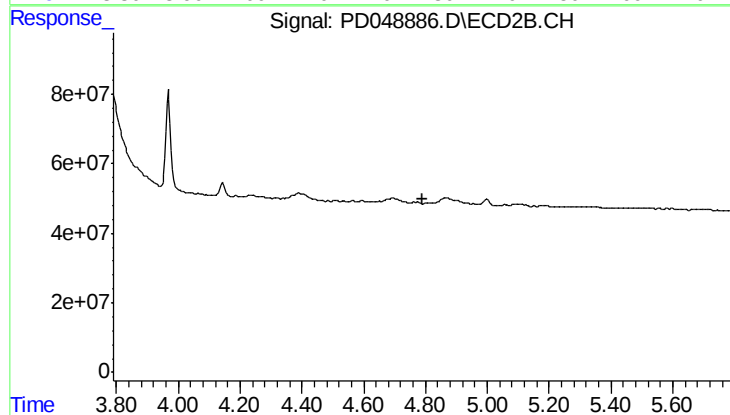

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.789 min
Response: 0
Conc: N.D.

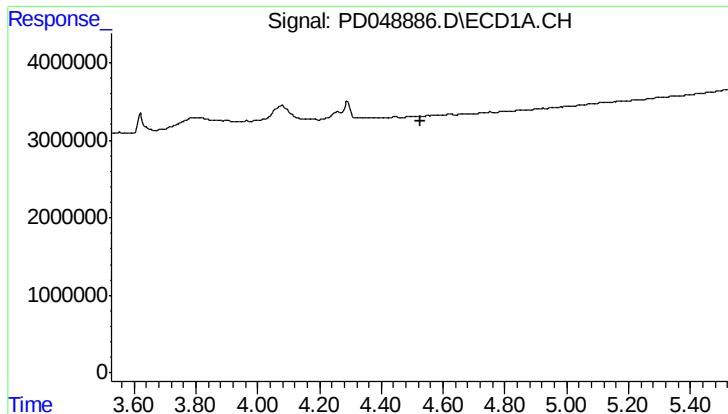

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.526 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

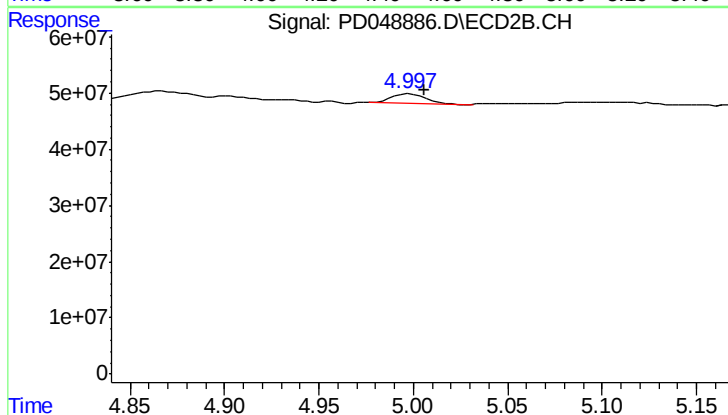


#7 delta-BHC

R.T.: 4.999 min
Delta R.T.: -0.007 min
Response: 20825341
Conc: 1.11 ng/ml

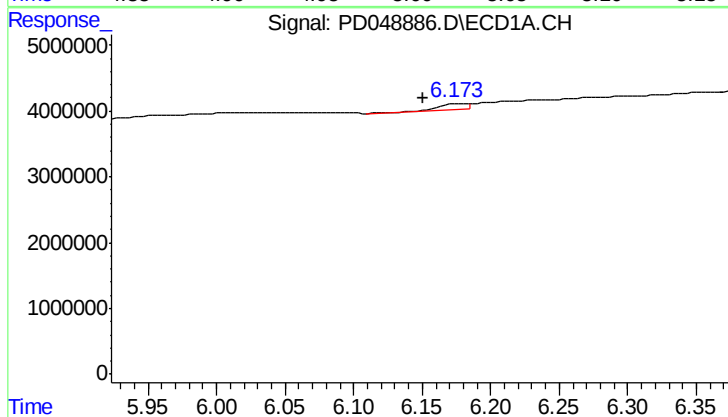


#15 Endosulfan II

R.T.: 6.175 min
Delta R.T.: 0.025 min
Response: 1081975
Conc: 0.75 ng/ml

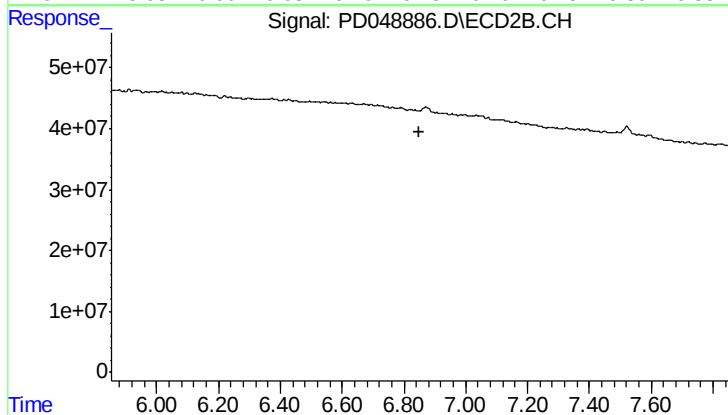

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.851 min
Response: 0
Conc: N.D.

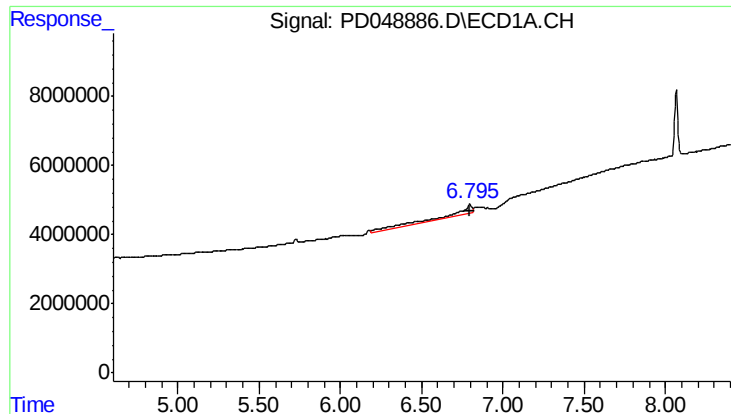

#20 Methoxychlor


R.T.: 6.796 min
Delta R.T.: 0.000 min
Response: 33804322
Conc: 43.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

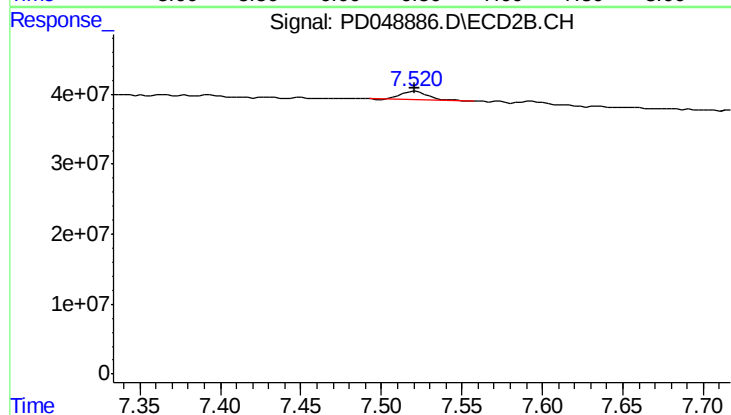


#20 Methoxychlor

R.T.: 7.521 min
Delta R.T.: 0.000 min
Response: 13689806
Conc: 2.27 ng/ml

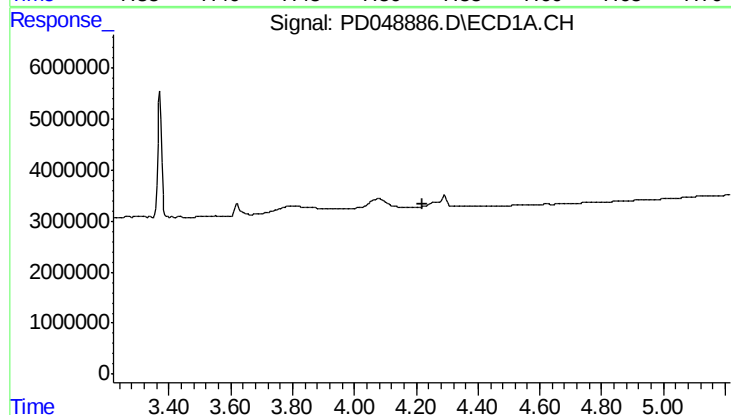


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.220 min
Response: 0
Conc: N.D.

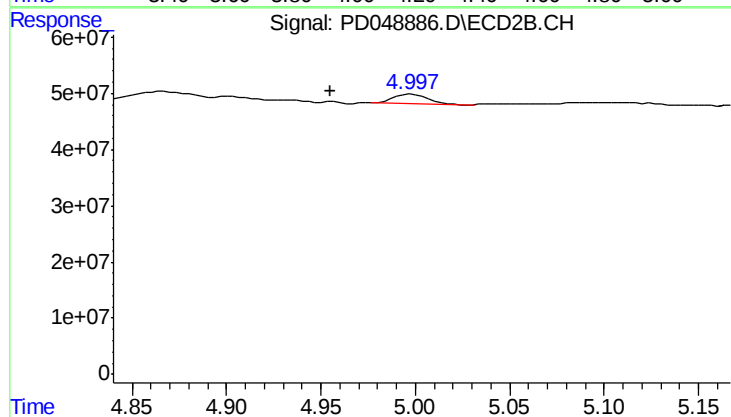

#23 Chlordane-1


R.T.: 4.999 min
Delta R.T.: 0.044 min
Response: 20825341
Conc: 28.36 ng/ml

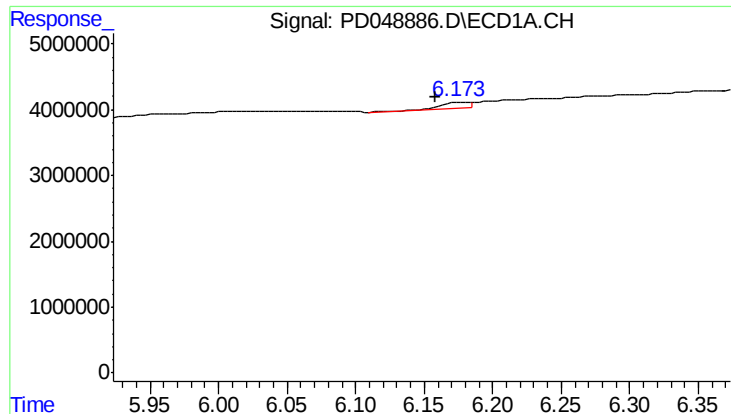

#27 Chlordane-5


R.T.: 6.175 min
Delta R.T.: 0.017 min
Response: 1081975
Conc: 19.71 ng/ml

Instrument :
ECD_D
ClientSampleId :

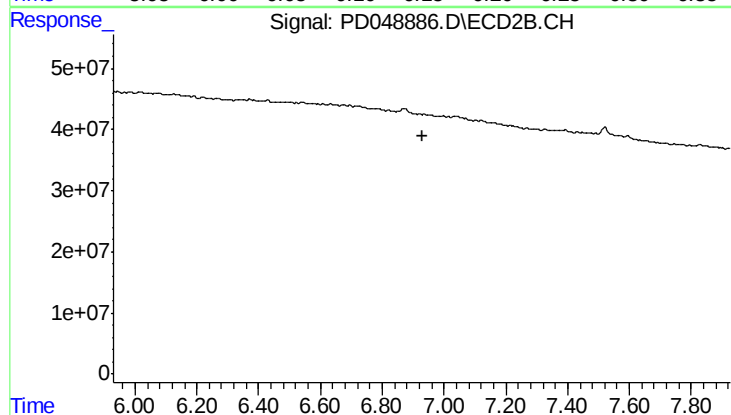


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.929 min
Response: 0
Conc: N.D.

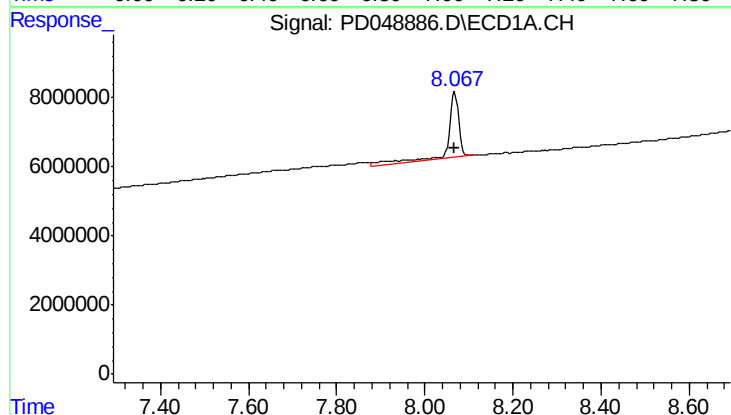

#28 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.001 min
Response: 32721039
Conc: 23.37 ng/ml

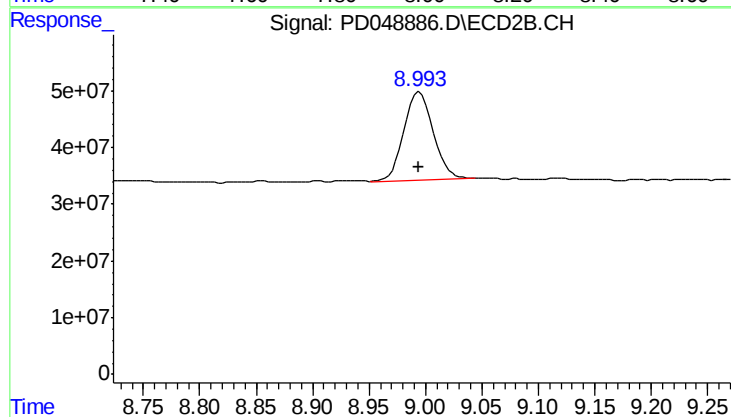

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 276931454
Conc: 18.34 ng/ml