

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048891.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2018 21:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:21:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.371	3.969	24953739	345.6E6	22.509	25.744
28)	SA Decachlor...	8.068	8.995	112.0E6	310.7E6	79.953	20.573 #
Target Compounds							
2)	A alpha-BHC	3.801	4.374	4928358	-2519261	2.572	N.D. #
3)	MA gamma-BHC...	4.078	4.684f	6248265	27847257	3.445	1.347 #
10)	B gamma-Chl...	0.000	6.050	0	1150737	N.D.	0.062 #
12)	B 4,4'-DDE	5.525	0.000	24481951	0	15.692	N.D. #
14)	MA Endrin	5.897	0.000	8742357	0	5.475	N.D. #
16)	A 4,4'-DDD	6.024	0.000	7723987	0	5.508	N.D. #
20)	A Methoxychlor	6.847f	0.000	38385280	0	49.279	N.D. #
25)	Chlordane-3	0.000	6.050	0	1150737	N.D.	0.472 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048891.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2018 21:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:21:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

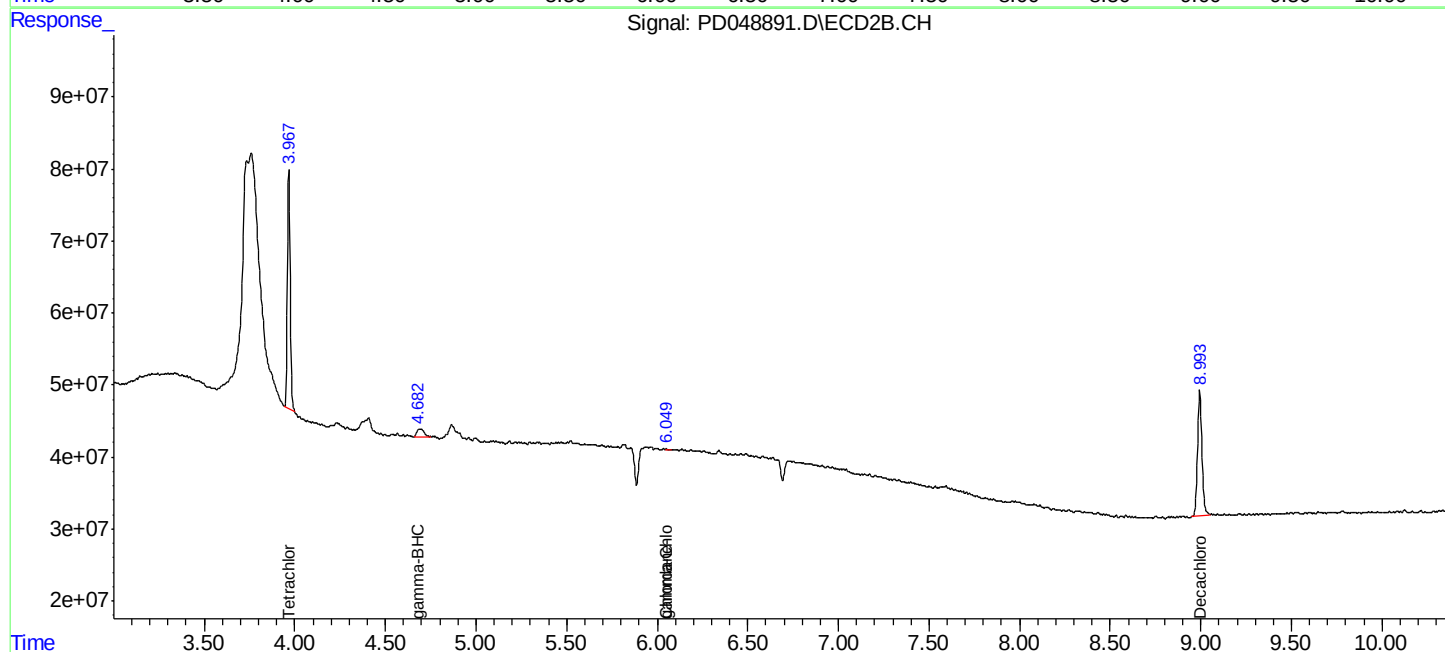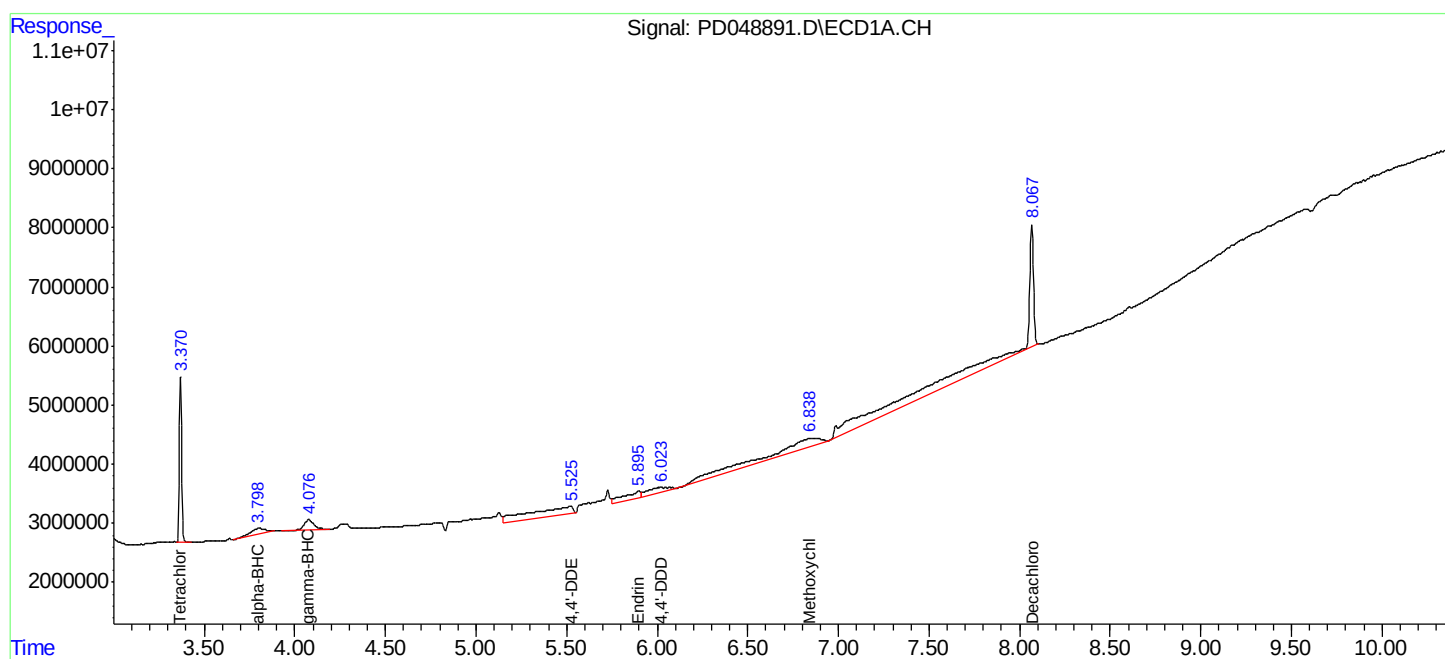


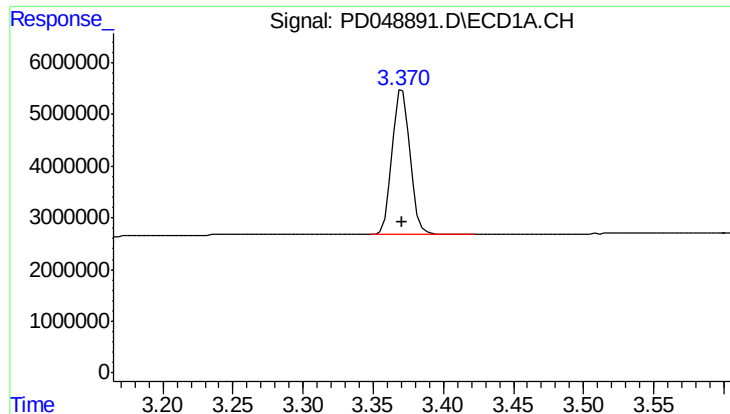

#1 Tetrachloro-m-xylene


R.T.: 3.371 min
Delta R.T.: 0.000 min
Response: 24953739
Conc: 22.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

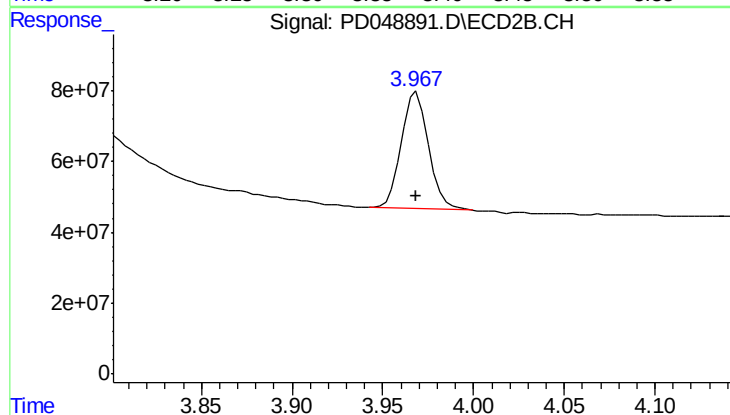


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 345585316
Conc: 25.74 ng/ml

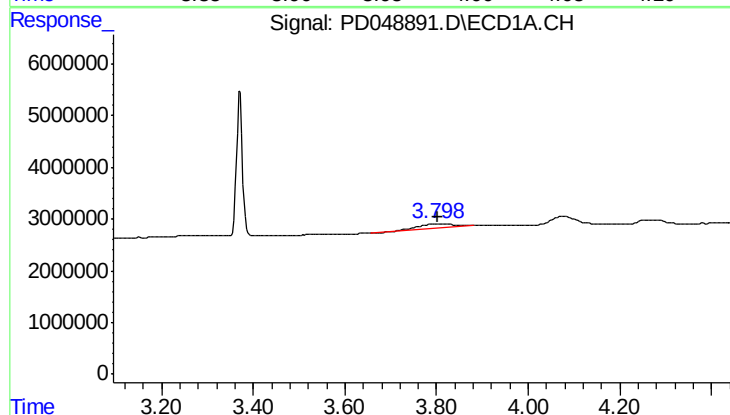


#2 alpha-BHC

R.T.: 3.801 min
Delta R.T.: 0.000 min
Response: 4928358
Conc: 2.57 ng/ml

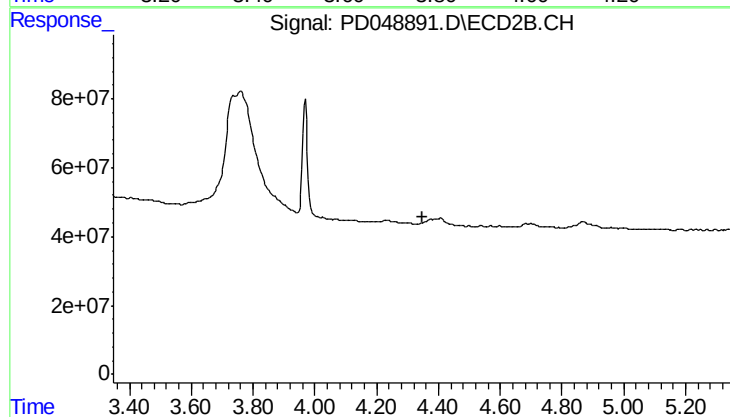

#2 alpha-BHC


R.T.: 4.374 min
Delta R.T.: 0.026 min
Response: -2519261
Conc: N.D.

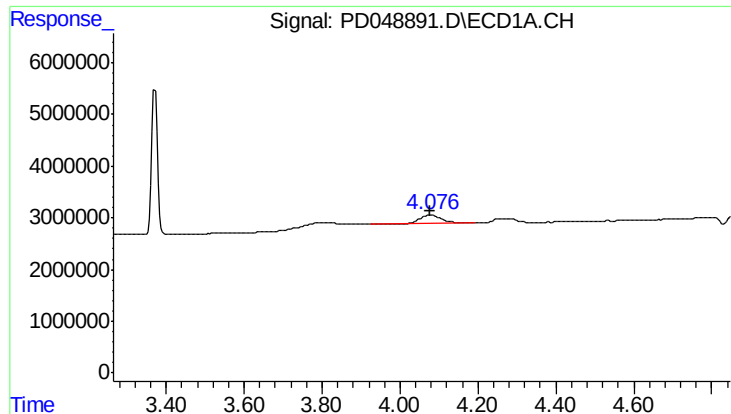

#3 gamma-BHC (Lindane)


R.T.: 4.078 min
Delta R.T.: -0.001 min
Response: 6248265
Conc: 3.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

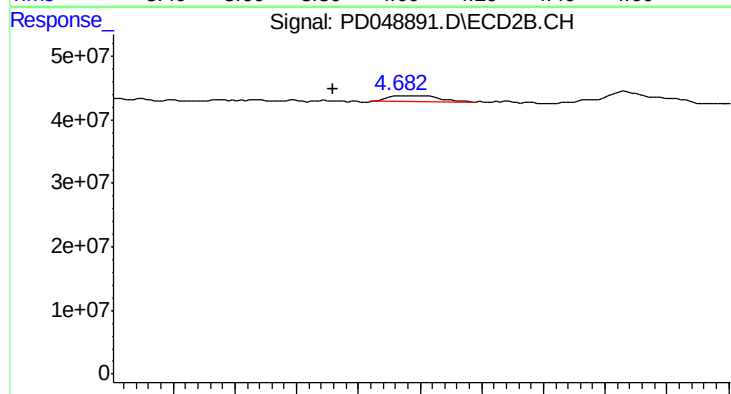


#3 gamma-BHC (Lindane)

R.T.: 4.684 min
Delta R.T.: 0.054 min
Response: 27847257
Conc: 1.35 ng/ml

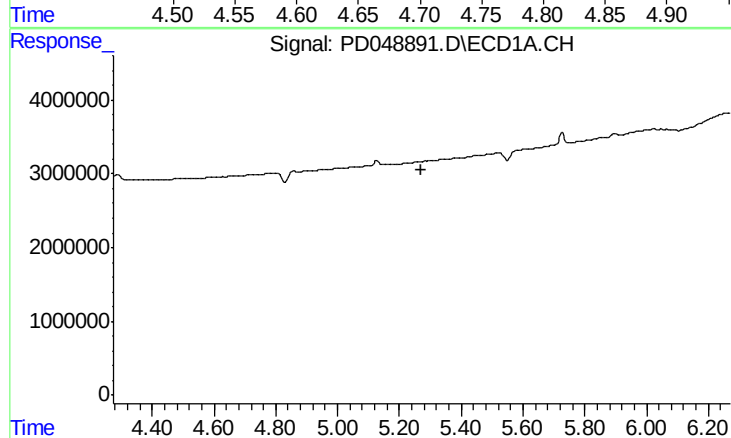


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.272 min
Response: 0
Conc: N.D.

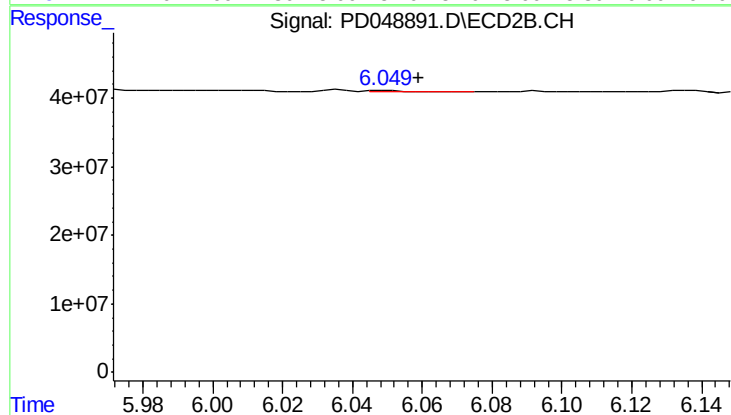

#10 gamma-Chlordane


R.T.: 6.050 min
Delta R.T.: -0.009 min
Response: 1150737
Conc: 0.06 ng/ml

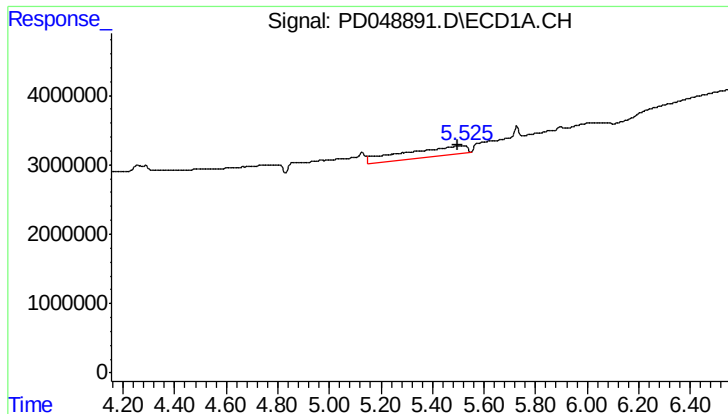

#12 4,4'-DDE


R.T.: 5.525 min
Delta R.T.: 0.029 min
Response: 24481951
Conc: 15.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

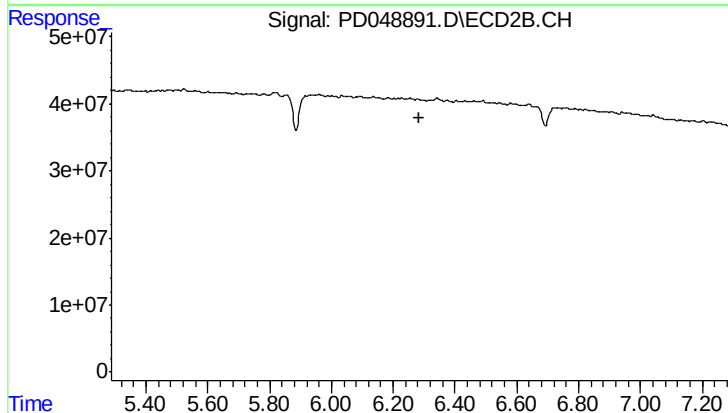


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

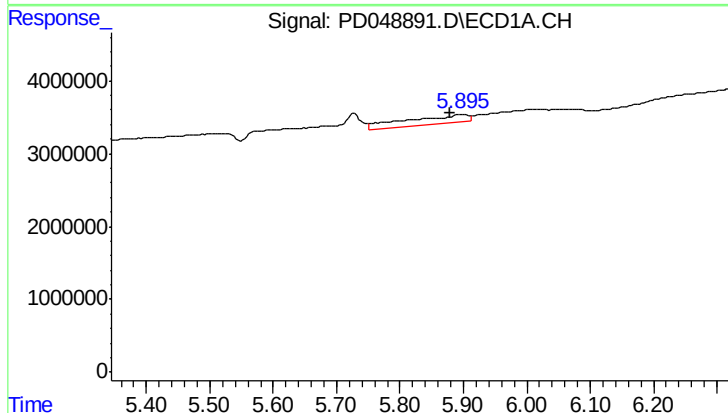


#14 Endrin

R.T.: 5.897 min
Delta R.T.: 0.019 min
Response: 8742357
Conc: 5.48 ng/ml

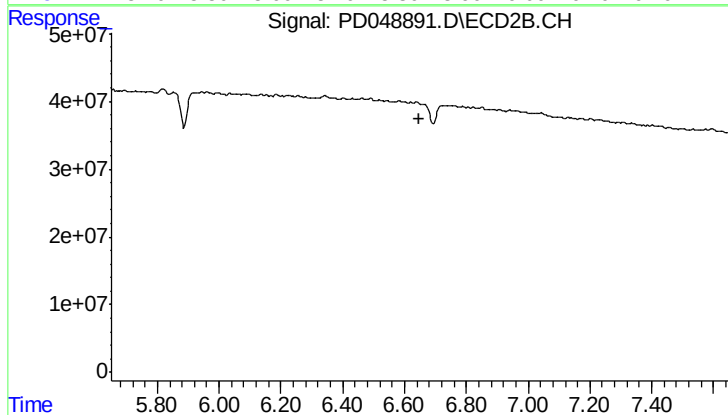

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.649 min
Response: 0
Conc: N.D.

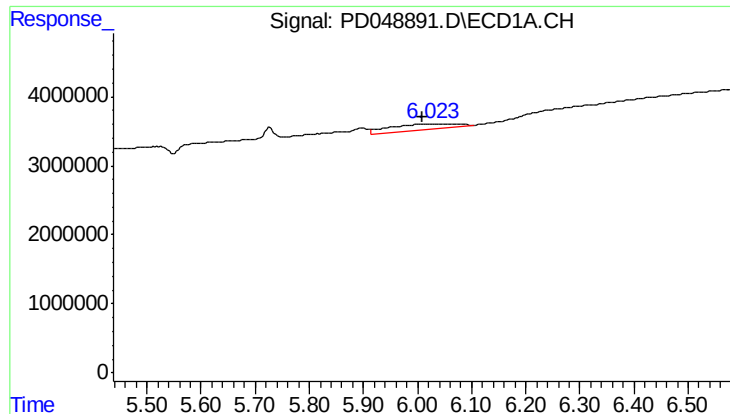

#16 4,4'-DDD


R.T.: 6.024 min
Delta R.T.: 0.015 min
Response: 7723987
Conc: 5.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

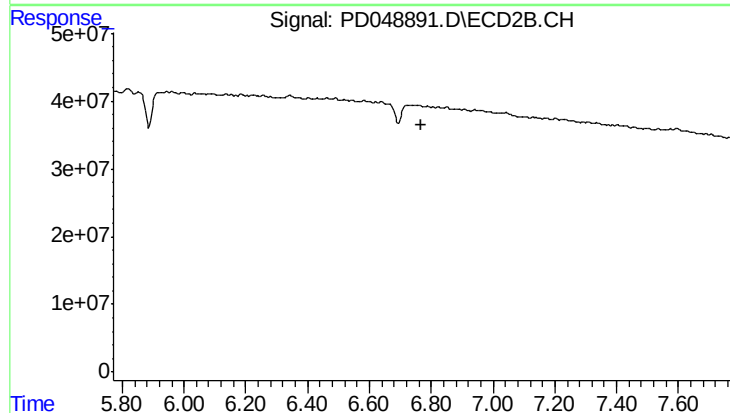


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.769 min
Response: 0
Conc: N.D.

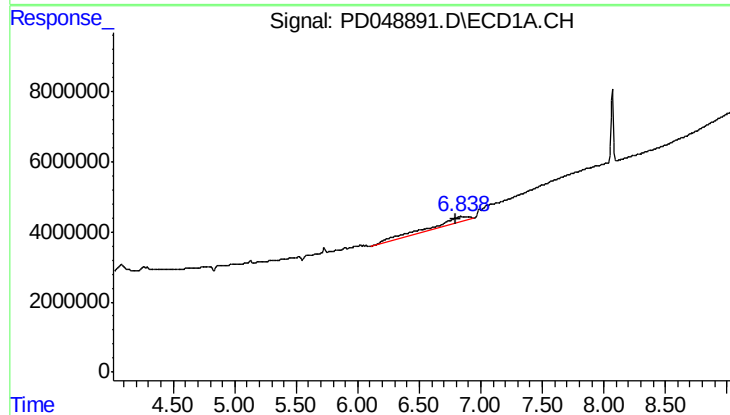


#20 Methoxychlor

R.T.: 6.847 min
Delta R.T.: 0.051 min
Response: 38385280
Conc: 49.28 ng/ml

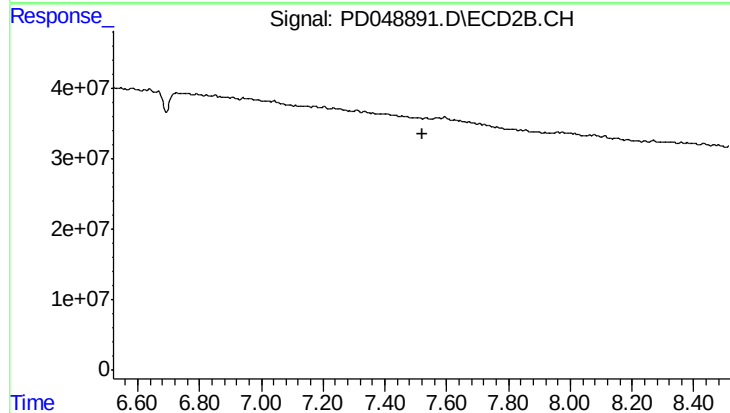

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

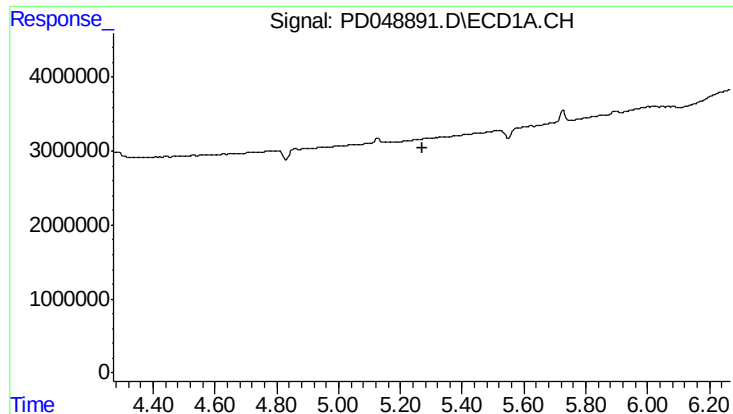

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

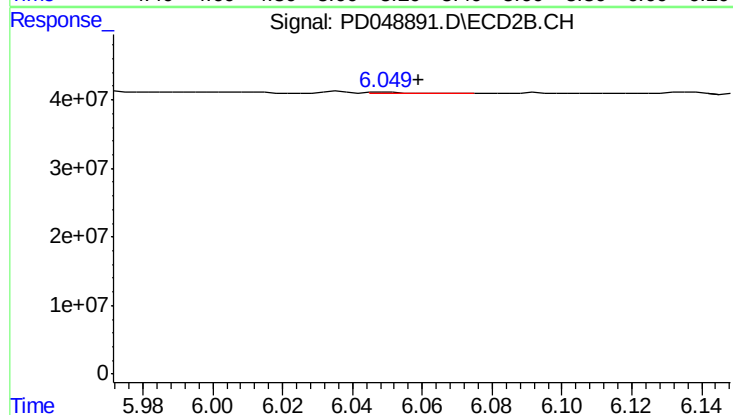


#25 Chlordane-3

R.T.: 6.050 min
Delta R.T.: -0.009 min
Response: 1150737
Conc: 0.47 ng/ml

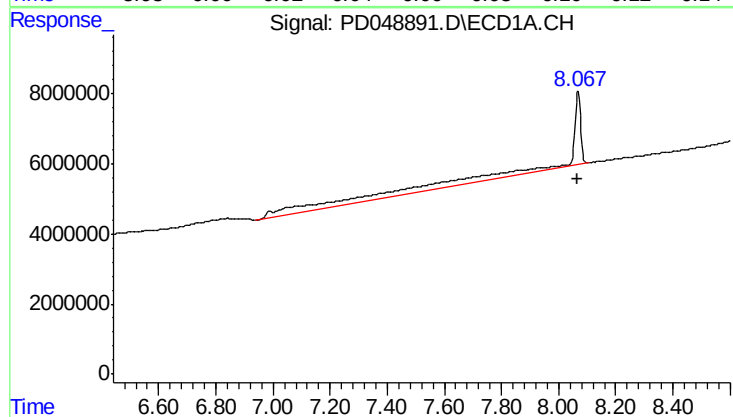

#28 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.001 min
Response: 111957271
Conc: 79.95 ng/ml

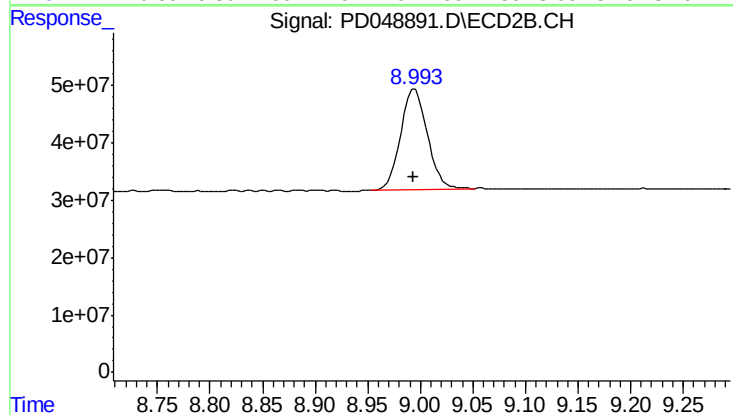

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 310708770
Conc: 20.57 ng/ml