

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048906.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2018 1:15
 Operator : AJ\SJ
 Sample : J4447-36
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SP-1-10

Manual Integrations
 APPROVED

Sohil
 8/14/2018 1:32:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 08:05:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.369	3.969	16972094	253.7E6	15.309m	18.897
28) SA Decachlor...	8.067	8.994	18965951	223.4E6	13.544m	14.791

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048906.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2018 1:15
Operator : AJ\SJ
Sample : J4447-36
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleID :
SP-1-10


Manual Integrations
APPROVED

Sohil
8/14/2018 1:32:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 08:05:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

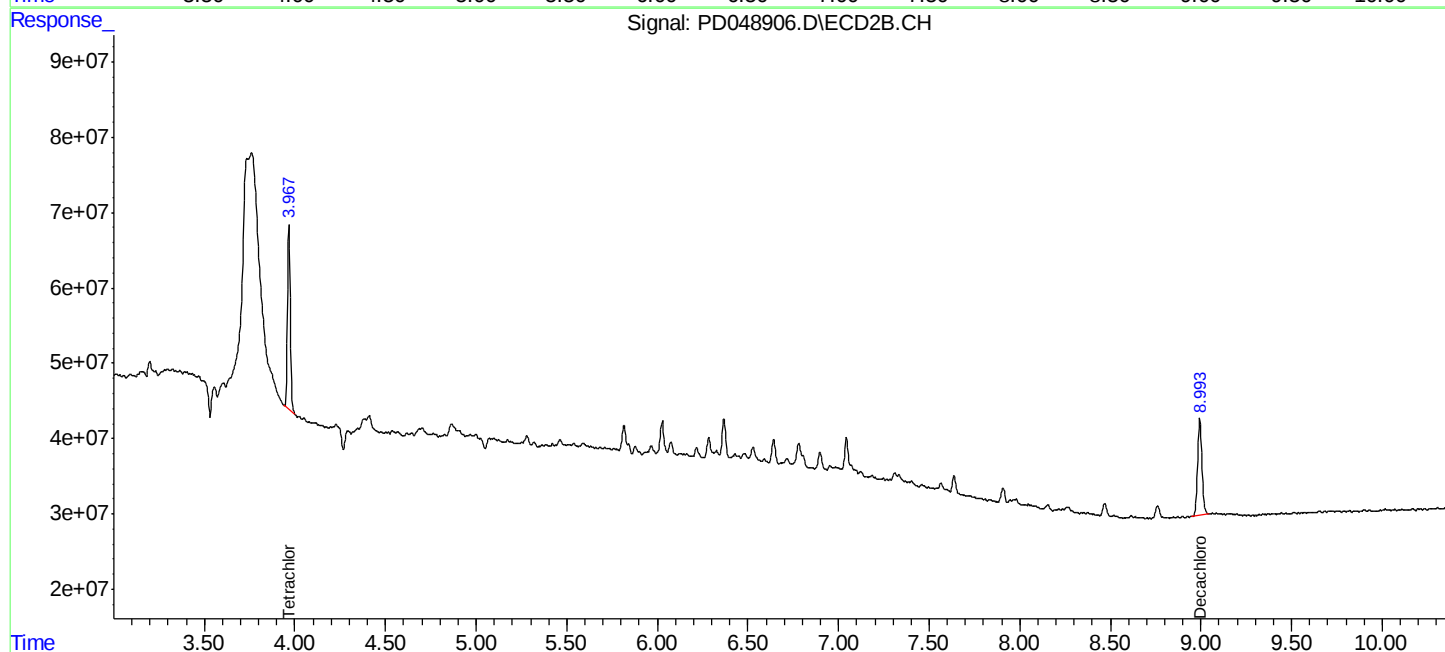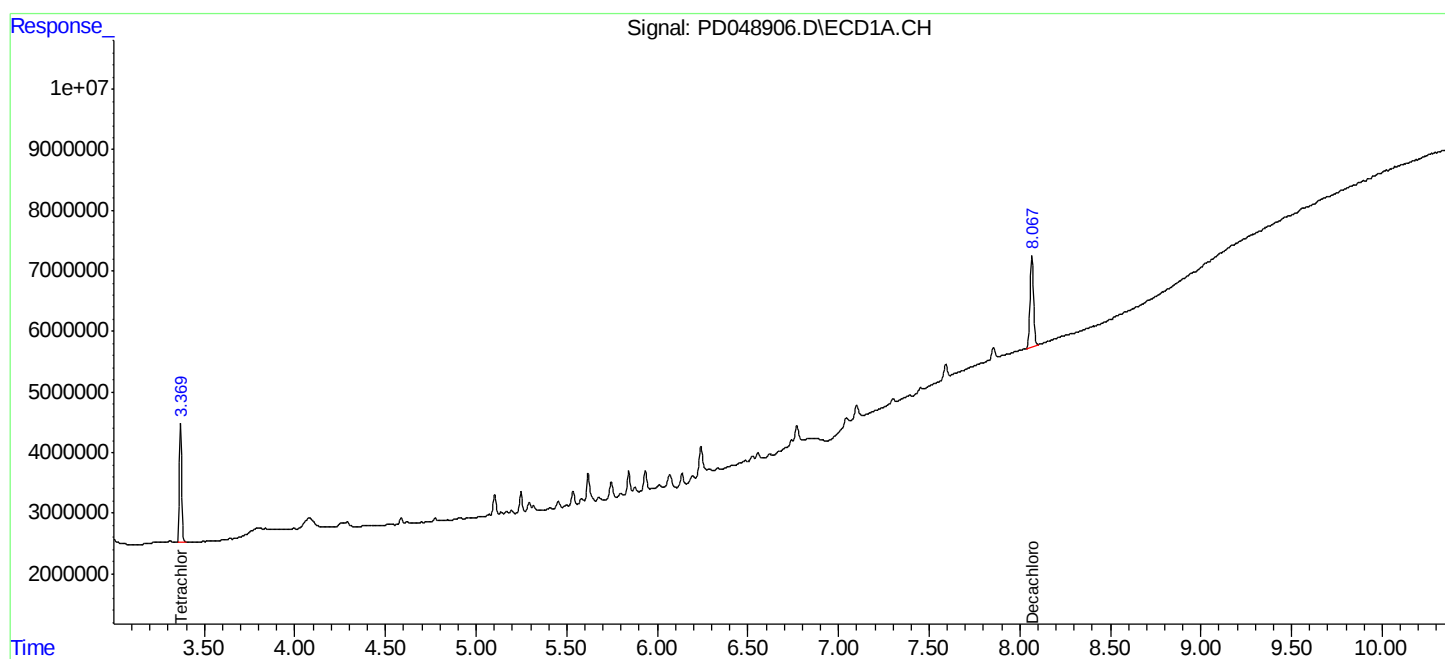

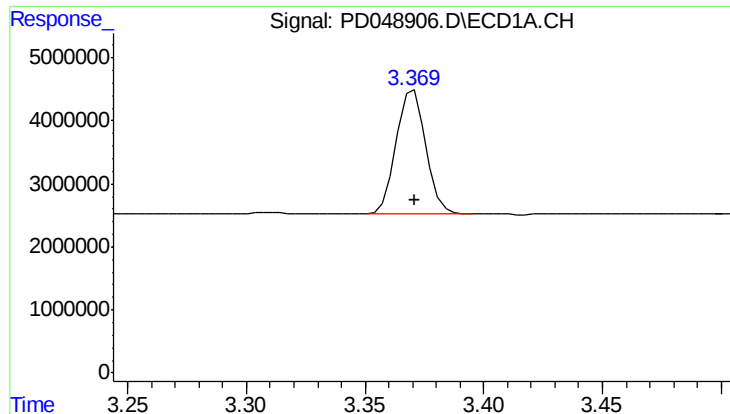


#1 Tetrachloro-m-xylene

R.T.: 3.369 min
Delta R.T.: -0.001 min
Response: 16972094
Conc: 15.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
SP-1-10


Manual Integrations
APPROVED

Sohil
8/14/2018 1:32:56 PM

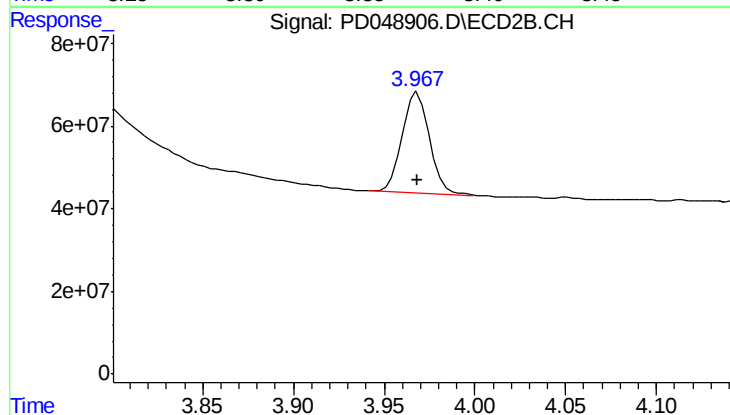


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: 0.000 min
Response: 253663500
Conc: 18.90 ng/ml

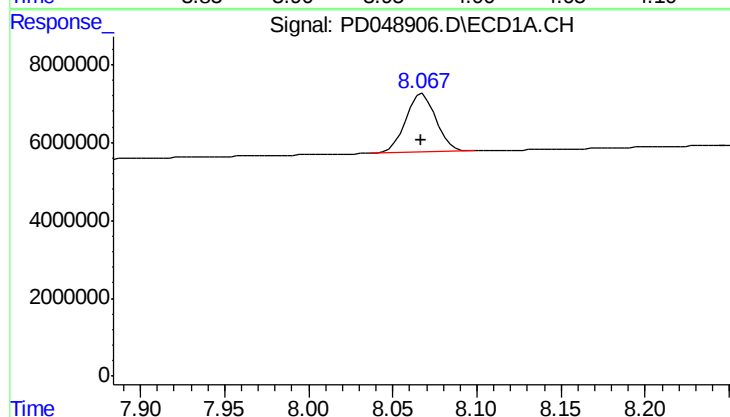

#28 Decachlorobiphenyl

R.T.: 8.067 min
Delta R.T.: 0.000 min
Response: 18965951
Conc: 13.54 ng/ml m

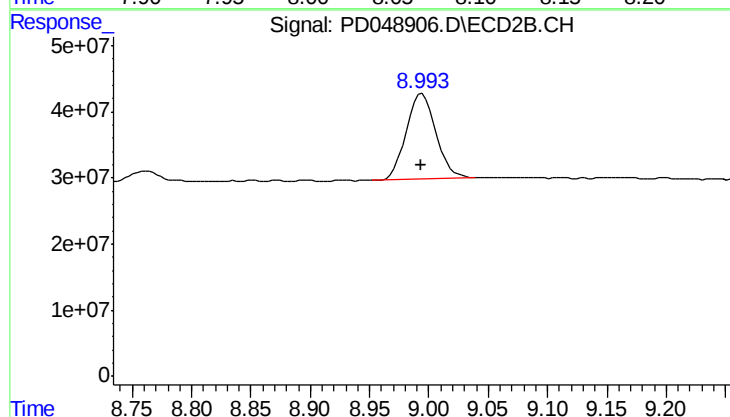

#28 Decachlorobiphenyl

R.T.: 8.994 min
Delta R.T.: 0.000 min
Response: 223389306
Conc: 14.79 ng/ml