

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
 Data File : PD048907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Aug 2018 1:28
 Operator : AJ\SJ
 Sample : J4449-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TILCON-MH-001

Manual Integrations
 APPROVED

Sohil
 8/14/2018 1:32:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 08:07:00 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 01 04:28:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.369	3.968	30355859	440.0E6	27.382m	32.774
28) SA Decachlor...	8.066	8.995	31261605	364.0E6	22.325m	24.099

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD081318\
Data File : PD048907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Aug 2018 1:28
Operator : AJ\SJ
Sample : J4449-01
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TILCON-MH-001


Manual Integrations
APPROVED

Sohil
8/14/2018 1:32:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 08:07:00 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073118.M
Quant Title : GC Extractables
QLast Update : Wed Aug 01 04:28:20 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

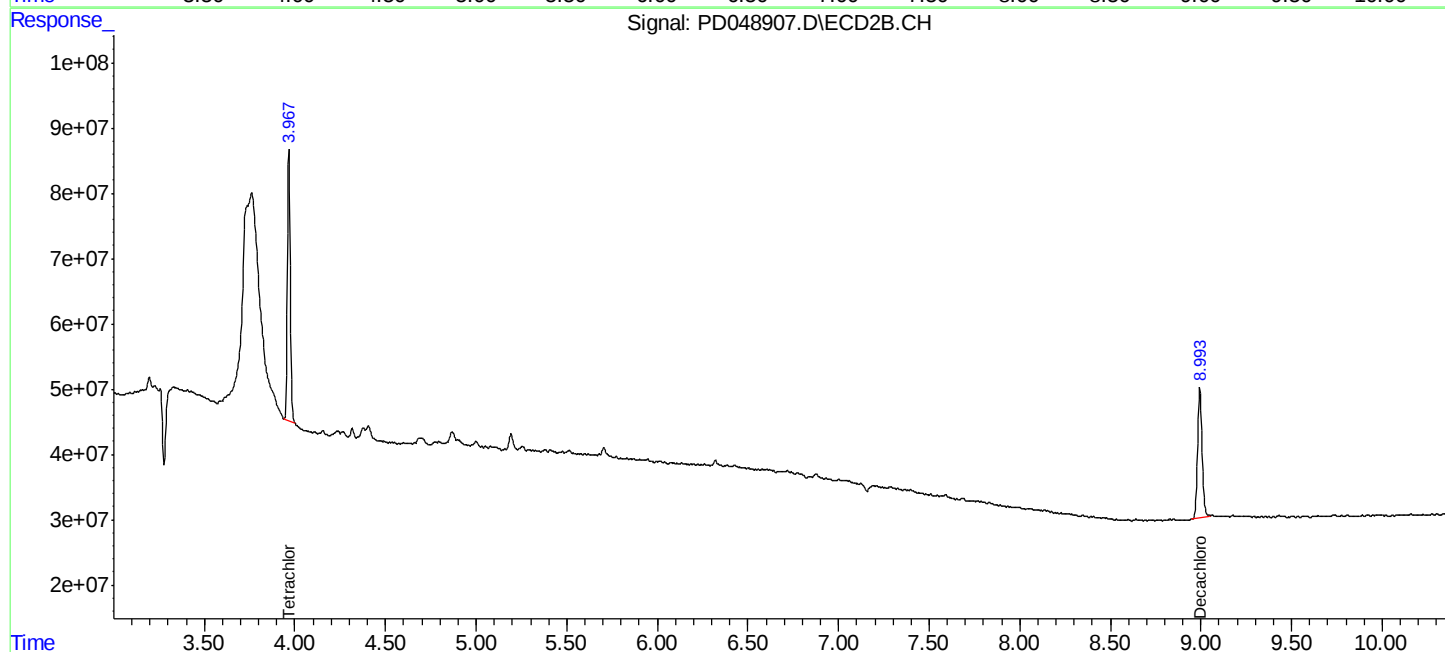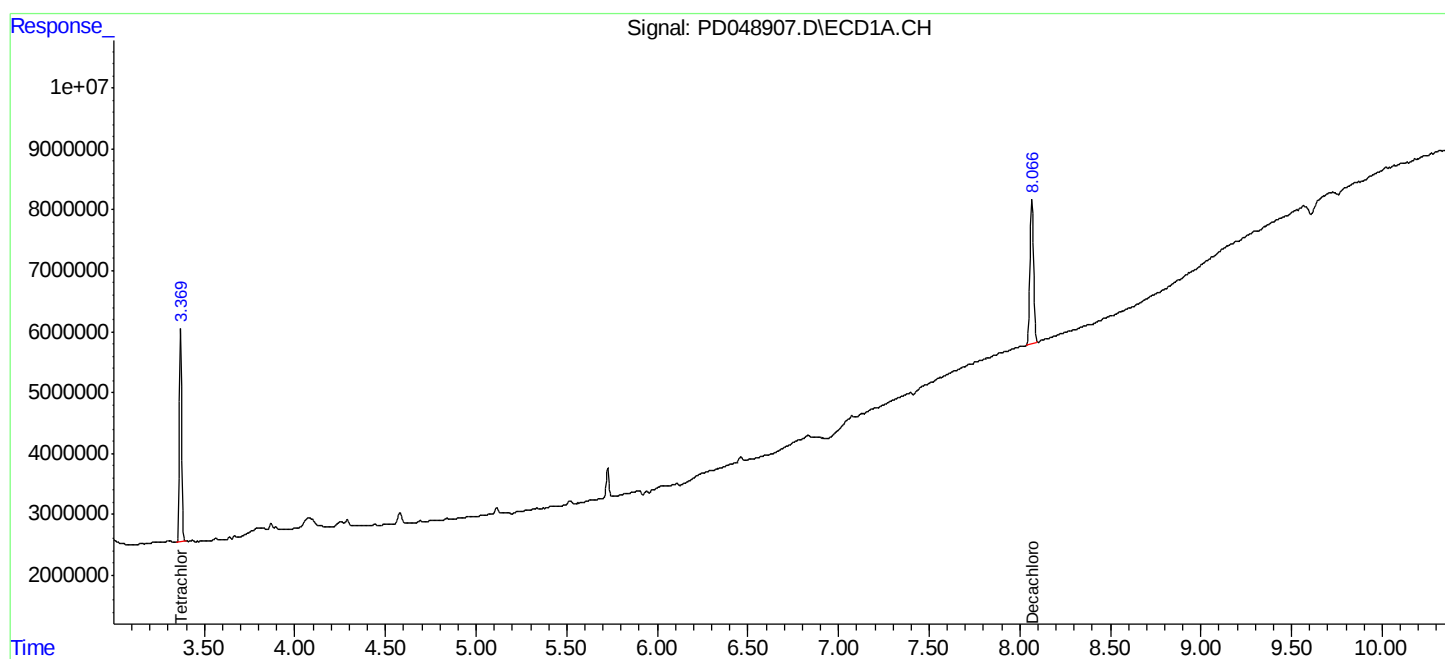

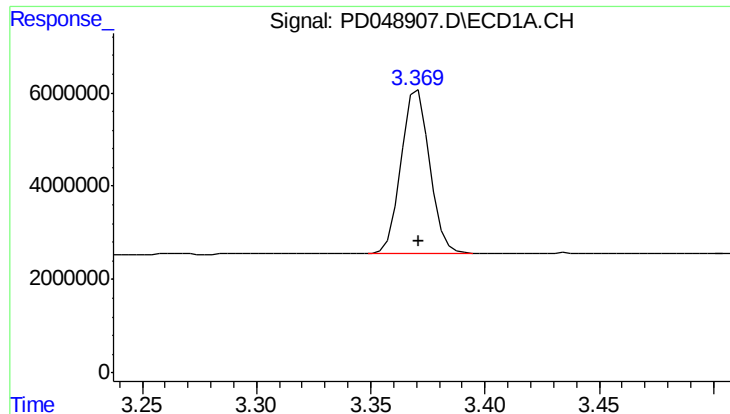


#1 Tetrachloro-m-xylene

R.T.: 3.369 min
Delta R.T.: -0.001 min
Response: 30355859
Conc: 27.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
TILCON-MH-001


Manual Integrations
APPROVED

Sohil
8/14/2018 1:32:57 PM

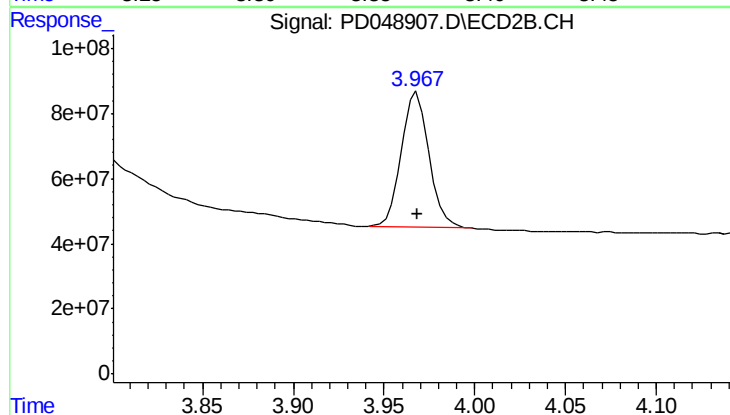


#1 Tetrachloro-m-xylene

R.T.: 3.968 min
Delta R.T.: 0.000 min
Response: 439951749
Conc: 32.77 ng/ml

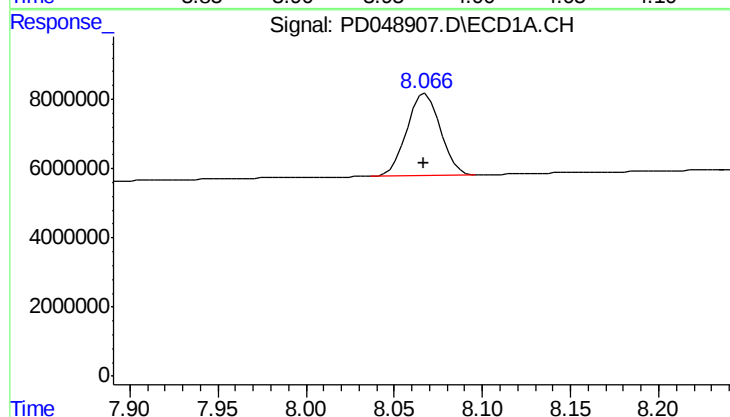

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: 0.000 min
Response: 31261605
Conc: 22.33 ng/ml m

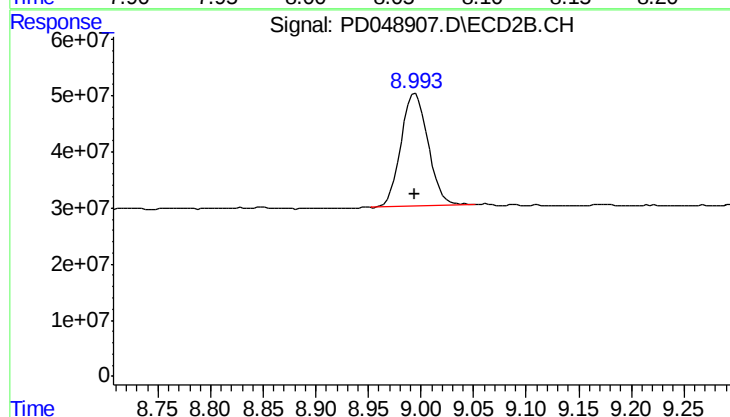

#28 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: 0.000 min
Response: 363968528
Conc: 24.10 ng/ml