

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081319\
 Data File : PD054265.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Aug 2019 12:40
 Operator : SM\AJ
 Sample : K4095-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SU-04-080919-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 04:33:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.312	3.983	16511017	22621532	28.688	25.968
28)	SA Decachlor...	8.007	9.025	14215157	19316379	21.117	20.836
Target Compounds							
3)	MA gamma-BHC...	4.025	0.000	562895	0	0.686	N.D. #
7)	B delta-BHC	0.000	5.015f	0	478368	N.D.	0.370 #
10)	B gamma-Chl...	0.000	6.069	0	179971	N.D.	0.137 #
23)	Chlordane-1	0.000	4.949f	0	56844	N.D.	1.517 #
25)	Chlordane-3	0.000	6.069	0	179971	N.D.	1.028 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081319\
Data File : PD054265.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Aug 2019 12:40
Operator : SM\AJ
Sample : K4095-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SU-04-080919-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD071919.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 04:33:23 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

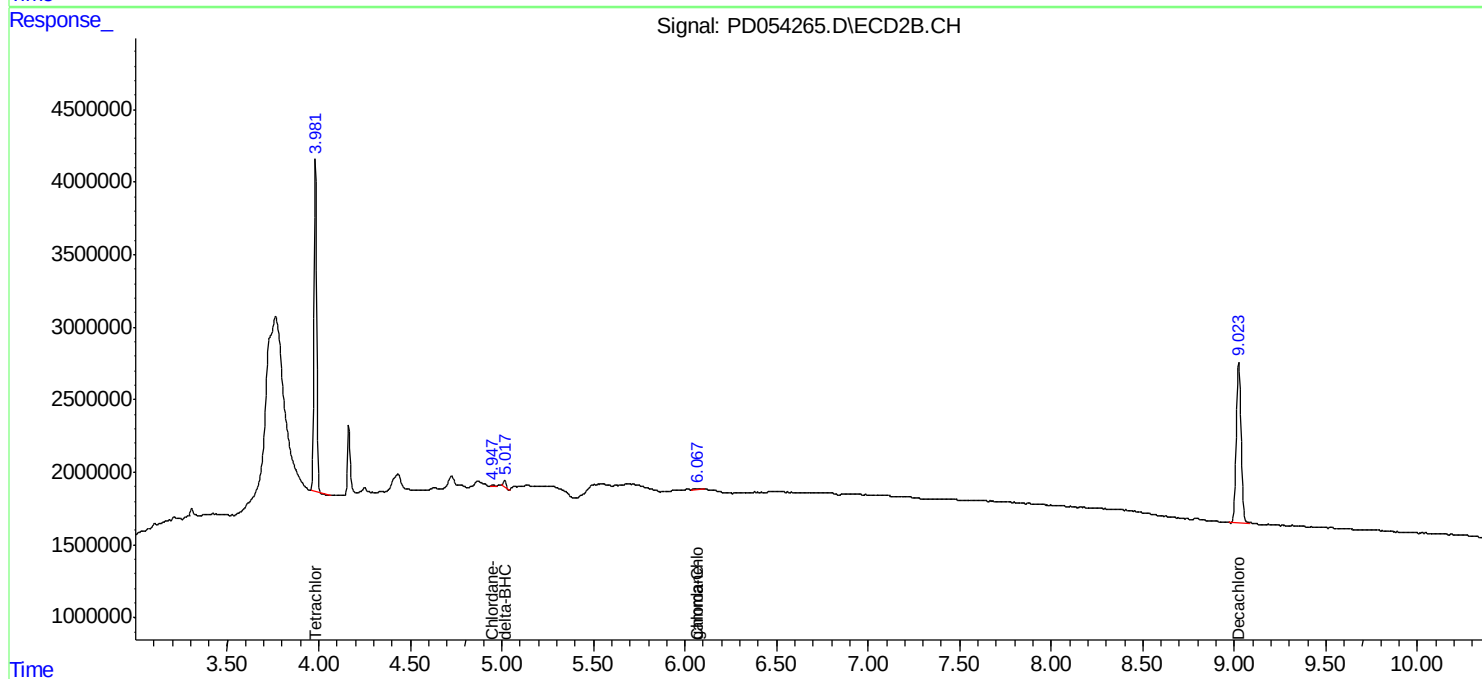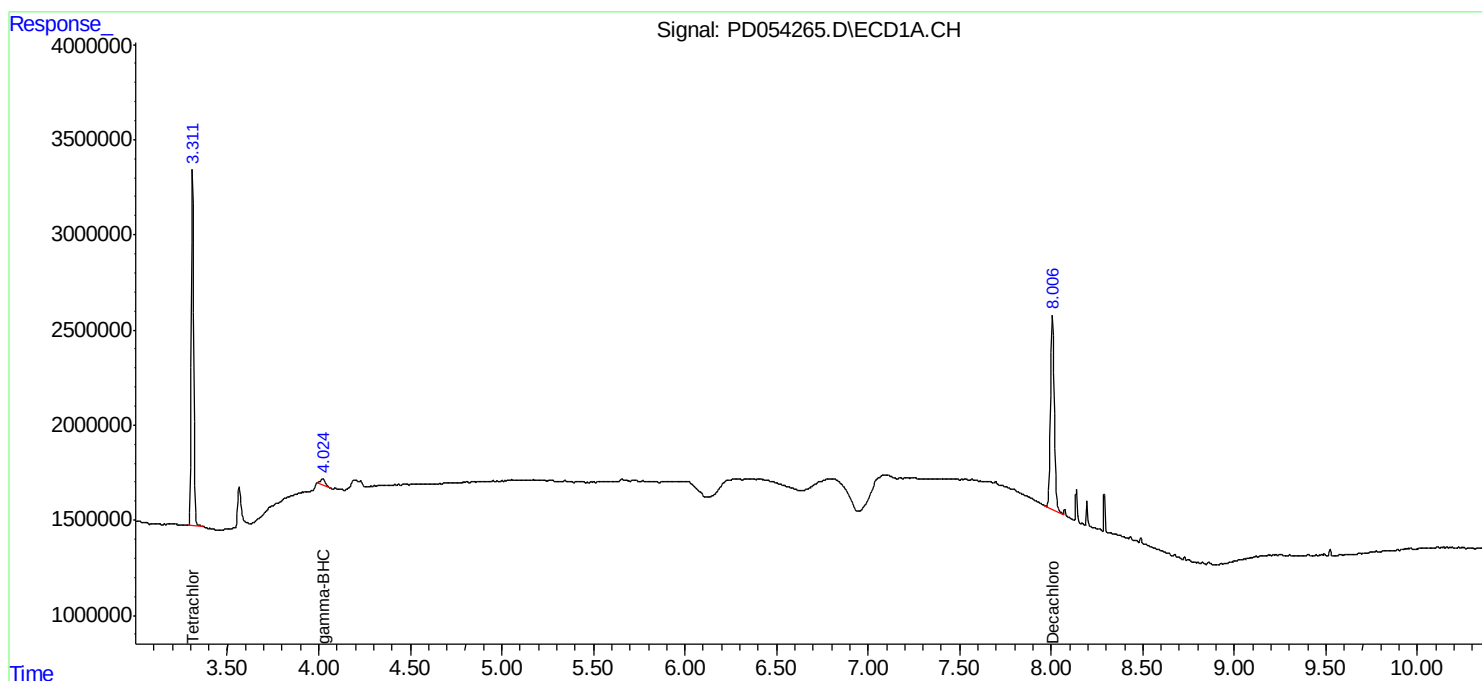


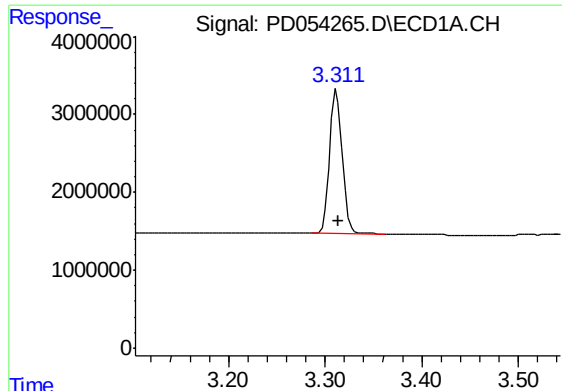

#1 Tetrachloro-m-xylene


R.T.: 3.312 min
Delta R.T.: 0.000 min
Response: 16511017
Conc: 28.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-04-080919-A

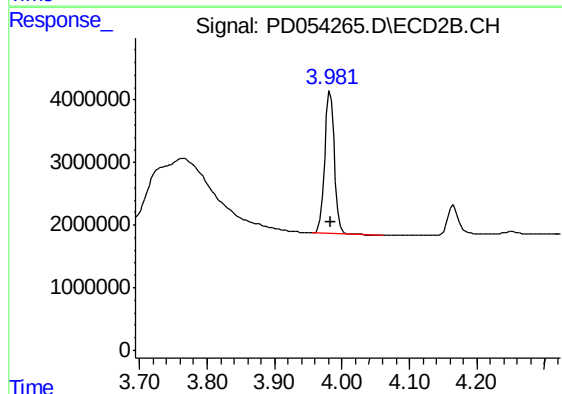


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 22621532
Conc: 25.97 ng/ml

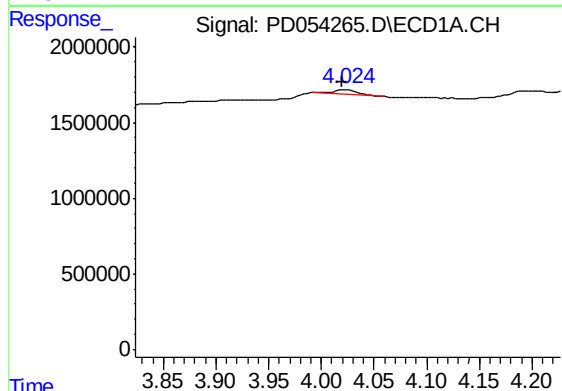


#3 gamma-BHC (Lindane)

R.T.: 4.025 min
Delta R.T.: 0.005 min
Response: 562895
Conc: 0.69 ng/ml

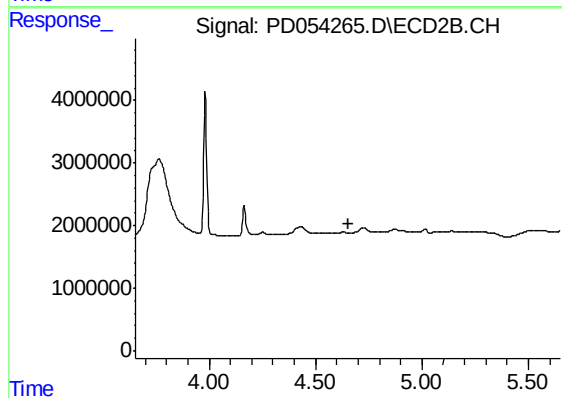

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.652 min
Response: 0
Conc: N.D.

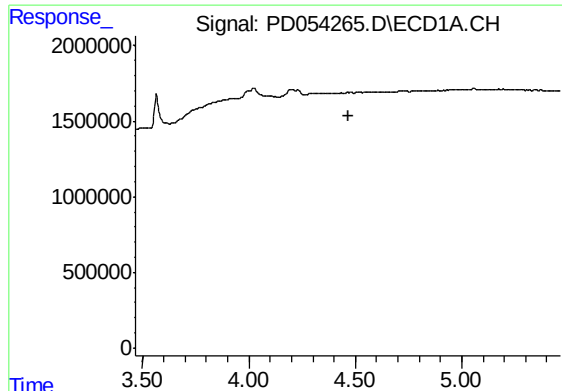

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SU-04-080919-A

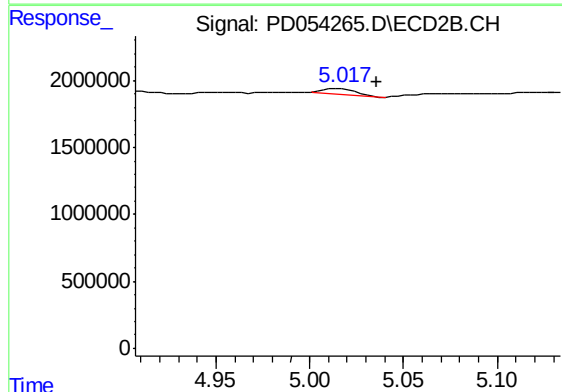


#7 delta-BHC

R.T.: 5.015 min
Delta R.T.: -0.021 min
Response: 478368
Conc: 0.37 ng/ml

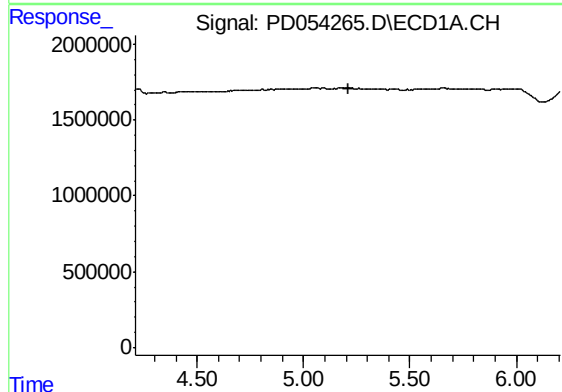


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

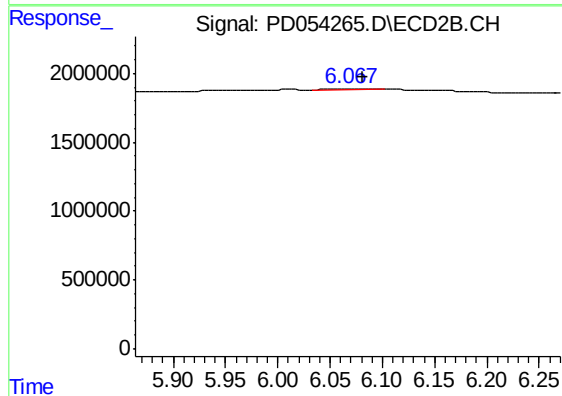

#10 gamma-Chlordane


R.T.: 6.069 min
Delta R.T.: -0.012 min
Response: 179971
Conc: 0.14 ng/ml

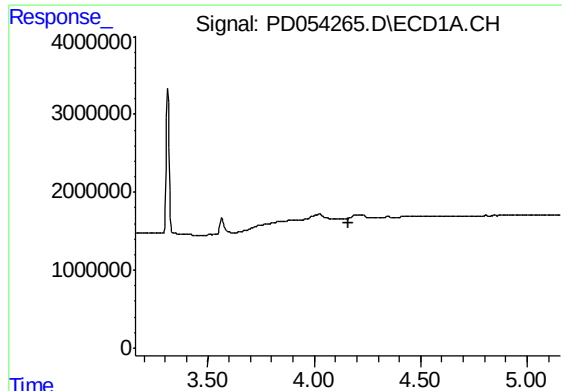

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
SU-04-080919-A

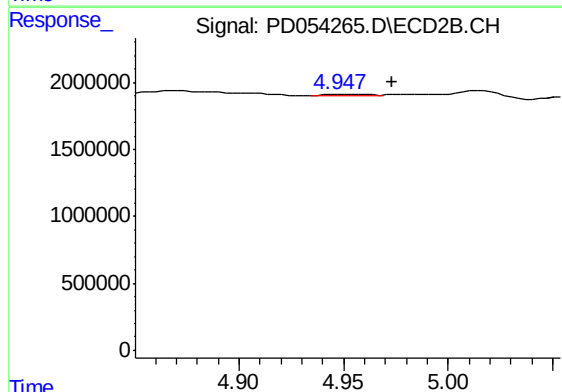


#23 Chlordane-1

R.T.: 4.949 min
Delta R.T.: -0.024 min
Response: 56844
Conc: 1.52 ng/ml

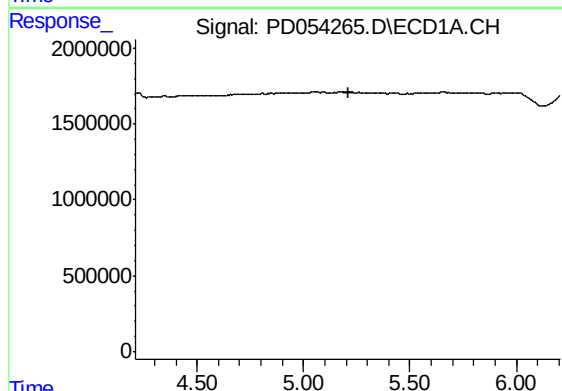


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

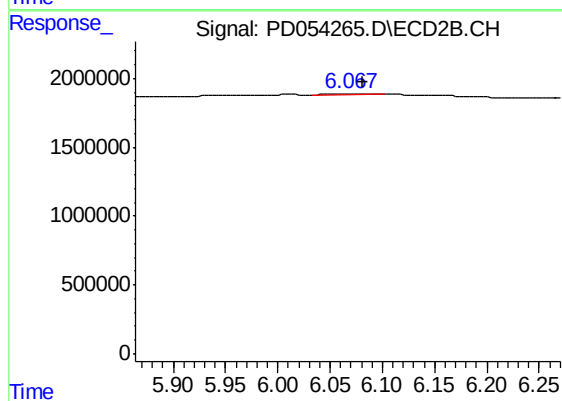

#25 Chlordane-3


R.T.: 6.069 min
Delta R.T.: -0.012 min
Response: 179971
Conc: 1.03 ng/ml

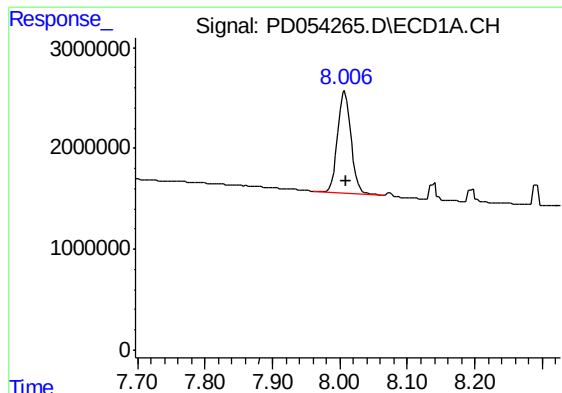

#28 Decachlorobiphenyl

R.T.: 8.007 min
Delta R.T.: -0.001 min
Response: 14215157
Conc: 21.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
SU-04-080919-A

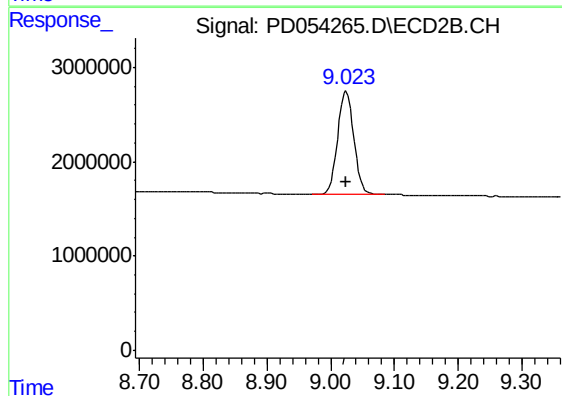

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 19316379
Conc: 20.84 ng/ml